

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072822\
 Data File : VV027051.D
 Acq On : 28 Jul 2022 22:02
 Operator : SY/MD
 Sample : VV0728WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK239

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
 Title : VOC Analysis

Signal : TIC: VV027051.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	74	81	101	rBV	382307	396647	15.15%	2.124%
2	1.561	155	162	176	rVB	321140	367830	14.05%	1.970%
3	2.102	319	330	344	rBV	650660	921463	35.20%	4.935%
4	2.285	378	387	396	rBV3	3385	5727	0.22%	0.031%
5	2.407	422	425	429	rBV3	555	440	0.02%	0.002%
6	2.503	446	455	470	rVB2	8929	15536	0.59%	0.083%
7	2.610	481	488	489	rBV4	2141	2299	0.09%	0.012%
8	2.754	527	533	537	rBV5	1174	1242	0.05%	0.007%
9	2.844	558	561	564	rVB4	444	298	0.01%	0.002%
10	2.947	590	593	598	rBV2	356	357	0.01%	0.002%
11	3.040	618	622	625	rBV3	309	273	0.01%	0.001%
12	3.108	640	643	646	rBV2	376	278	0.01%	0.001%
13	3.561	776	784	788	rVB2	327	396	0.02%	0.002%
14	3.584	788	791	795	rVB	399	281	0.01%	0.002%
15	3.635	799	807	809	rBV2	417	463	0.02%	0.002%
16	3.674	816	819	823	rBV2	396	300	0.01%	0.002%
17	3.793	852	856	861	rVB3	294	293	0.01%	0.002%
18	3.892	876	887	941	rBV2	142922	704530	26.92%	3.773%
19	4.343	1011	1027	1050	rBV	428193	1061104	40.54%	5.683%
20	4.661	1123	1126	1128	rBV2	666	405	0.02%	0.002%
21	4.751	1152	1154	1158	rVB3	464	355	0.01%	0.002%
22	4.892	1196	1198	1201	rVB2	485	297	0.01%	0.002%
23	5.040	1227	1244	1263	rBV2	1039270	2617482	100.00%	14.018%
24	5.381	1349	1350	1353	rBV	574	274	0.01%	0.001%
25	5.613	1409	1422	1466	rBV	571475	1214954	46.42%	6.507%
26	5.908	1502	1514	1528	rBV3	18233	41454	1.58%	0.222%
27	6.066	1549	1563	1598	rBV	578920	1228710	46.94%	6.580%
28	6.391	1662	1664	1670	rVB3	512	382	0.01%	0.002%
29	6.445	1679	1681	1687	rVB3	636	515	0.02%	0.003%
30	6.539	1707	1710	1713	rBV	472	303	0.01%	0.002%
31	6.593	1724	1727	1730	rBV2	523	374	0.01%	0.002%
32	6.651	1738	1745	1746	rBV2	805	742	0.03%	0.004%
33	6.789	1784	1788	1793	rVB2	628	566	0.02%	0.003%
34	6.870	1809	1813	1818	rVB2	329	321	0.01%	0.002%
35	6.986	1834	1849	1891	rBV	272940	527897	20.17%	2.827%
36	7.198	1909	1915	1921	rBV5	1022	1495	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072822\
 Data File : VV027051.D
 Acq On : 28 Jul 2022 22:02
 Operator : SY/MD
 Sample : VV0728WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK239

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
 Title : VOC Analysis

37	7.314	1938	1951	1986	rBV	1141305	2054582	78.49%	11.003%
38	7.619	2036	2046	2084	rVV	192336	357662	13.66%	1.915%
39	7.876	2124	2126	2130	rVB5	643	428	0.02%	0.002%
40	7.905	2130	2135	2138	rBV4	397	302	0.01%	0.002%
41	7.976	2150	2157	2158	rBV3	3604	3155	0.12%	0.017%
42	8.092	2179	2193	2225	rBV	592837	1279012	48.86%	6.850%
43	8.416	2288	2294	2305	rVV4	4293	7359	0.28%	0.039%
44	8.584	2341	2346	2350	rVB3	675	640	0.02%	0.003%
45	8.625	2356	2359	2361	rBV2	499	300	0.01%	0.002%
46	8.850	2414	2429	2458	rBV	887414	1476514	56.41%	7.907%
47	9.204	2535	2539	2543	rVB2	324	304	0.01%	0.002%
48	9.256	2550	2555	2558	rBV2	476	409	0.02%	0.002%
49	9.330	2575	2578	2580	rBV2	375	292	0.01%	0.002%
50	9.516	2634	2636	2642	rVB2	464	352	0.01%	0.002%
51	9.551	2642	2647	2650	rBV3	868	829	0.03%	0.004%
52	9.612	2664	2666	2670	rVB4	591	370	0.01%	0.002%
53	9.780	2715	2718	2721	rBV3	480	358	0.01%	0.002%
54	9.934	2760	2766	2769	rBV2	622	670	0.03%	0.004%
55	10.114	2819	2822	2825	rVB3	420	298	0.01%	0.002%
56	10.214	2840	2853	2877	rBV	878085	1381345	52.77%	7.398%
57	10.413	2913	2915	2924	rVB4	585	575	0.02%	0.003%
58	10.542	2950	2955	2959	rBV2	905	814	0.03%	0.004%
59	10.622	2976	2980	2982	rBV2	374	281	0.01%	0.002%
60	10.635	2982	2984	2990	rVB3	335	284	0.01%	0.002%
61	10.854	3049	3052	3056	rBV3	835	623	0.02%	0.003%
62	10.934	3071	3077	3081	rVB2	644	644	0.02%	0.003%
63	11.018	3100	3103	3109	rVV2	453	533	0.02%	0.003%
64	11.185	3149	3155	3163	rBV6	1849	2946	0.11%	0.016%
65	11.249	3163	3175	3196	rBV	816344	1270933	48.56%	6.807%
66	11.477	3243	3246	3253	rBV5	543	504	0.02%	0.003%
67	11.564	3270	3273	3277	rVB3	466	298	0.01%	0.002%
68	11.622	3277	3291	3312	rBV	1066413	1676971	64.07%	8.981%
69	11.947	3389	3392	3398	rBV4	551	460	0.02%	0.002%
70	12.394	3528	3531	3536	rBV2	490	424	0.02%	0.002%
71	12.468	3550	3554	3558	rVB2	487	461	0.02%	0.002%
72	12.497	3558	3563	3564	rBV2	469	355	0.01%	0.002%
73	12.648	3604	3610	3617	rBV5	2415	3077	0.12%	0.016%
74	12.735	3630	3637	3638	rBV2	569	551	0.02%	0.003%
75	12.757	3641	3644	3647	rVV3	590	448	0.02%	0.002%
76	12.796	3652	3656	3659	rVV2	384	349	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072822\
 Data File : VV027051.D
 Acq On : 28 Jul 2022 22:02
 Operator : SY/MD
 Sample : VV0728WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK239

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
 Title : VOC Analysis

77	12.966	3706	3709	3713	rBV3	332	270	0.01%	0.001%
78	13.037	3727	3731	3734	rBV2	454	458	0.02%	0.002%
79	13.130	3754	3760	3763	rBV2	534	502	0.02%	0.003%
80	13.275	3796	3805	3816	rBV6	2485	4561	0.17%	0.024%
81	13.349	3825	3828	3831	rVB2	525	366	0.01%	0.002%
82	13.394	3839	3842	3846	rBV3	337	280	0.01%	0.001%
83	13.458	3857	3862	3864	rBV4	468	420	0.02%	0.002%
84	13.516	3870	3880	3889	rBV3	4273	7710	0.29%	0.041%
85	13.596	3903	3905	3908	rVB3	519	276	0.01%	0.001%
86	13.718	3940	3943	3946	rVB3	479	292	0.01%	0.002%
87	13.747	3946	3952	3959	rBV5	3636	4487	0.17%	0.024%
88	13.844	3976	3982	3985	rBV2	622	713	0.03%	0.004%
89	13.898	3995	3999	4004	rBV2	717	677	0.03%	0.004%
90	14.648	4230	4232	4234	rBV2	485	317	0.01%	0.002%
91	14.773	4269	4271	4273	rBV	633	286	0.01%	0.002%
92	14.837	4285	4291	4292	rBV2	852	879	0.03%	0.005%
93	14.972	4331	4333	4337	rVB4	702	442	0.02%	0.002%
94	14.995	4337	4340	4342	rBV2	526	341	0.01%	0.002%
95	15.085	4365	4368	4370	rBV2	593	384	0.01%	0.002%
96	15.149	4385	4388	4390	rBV3	589	410	0.02%	0.002%
97	15.210	4404	4407	4410	rBV3	834	610	0.02%	0.003%
98	15.387	4456	4462	4471	rBV7	1290	1999	0.08%	0.011%
99	15.796	4586	4589	4594	rVB5	1613	1237	0.05%	0.007%
100	15.828	4594	4599	4602	rBV6	1151	1418	0.05%	0.008%




Sum of corrected areas: 18672330

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072822\
Data File : VV027051.D
Acq On : 28 Jul 2022 22:02
Operator : SY/MD
Sample : VV0728WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK239

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

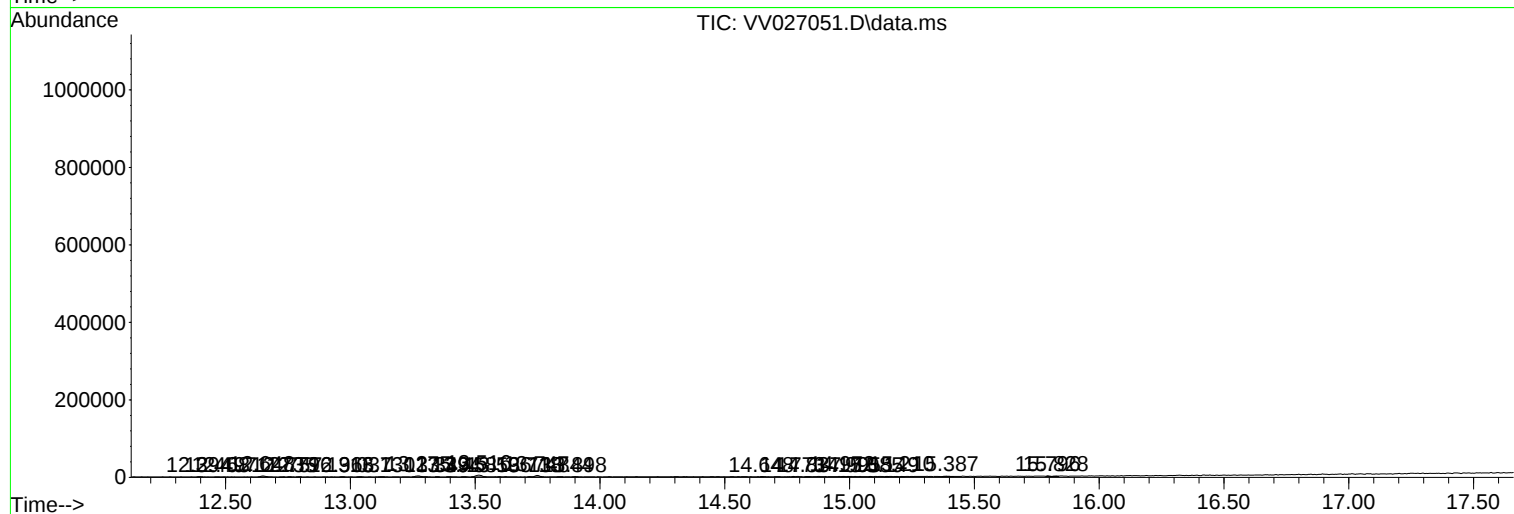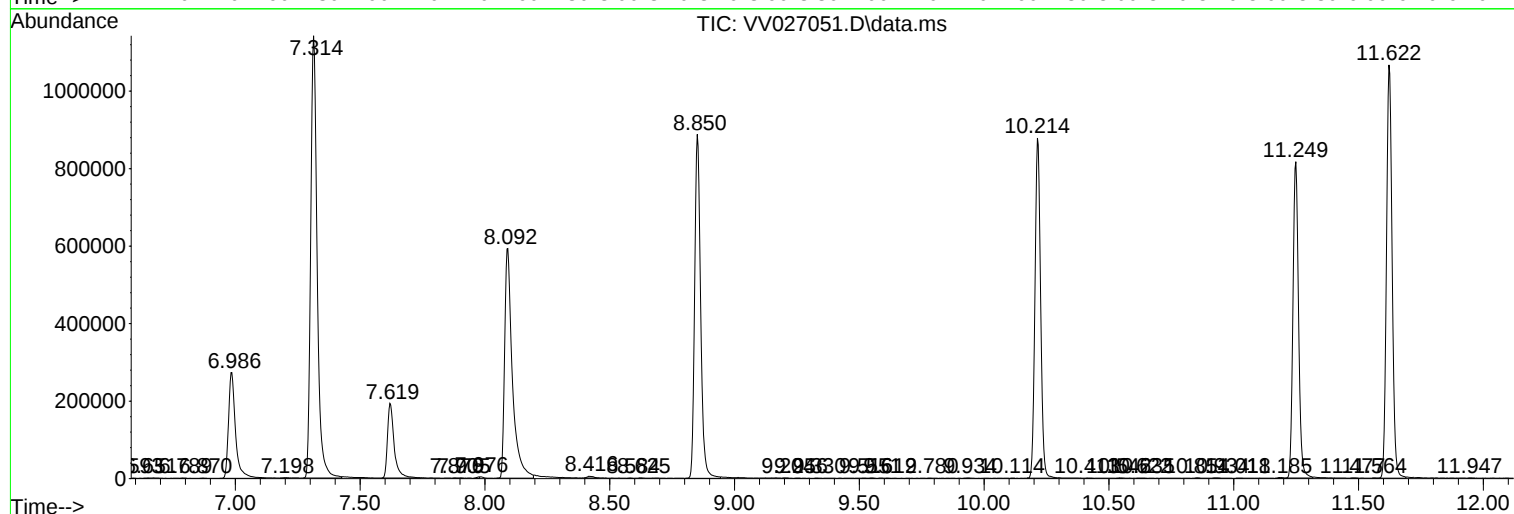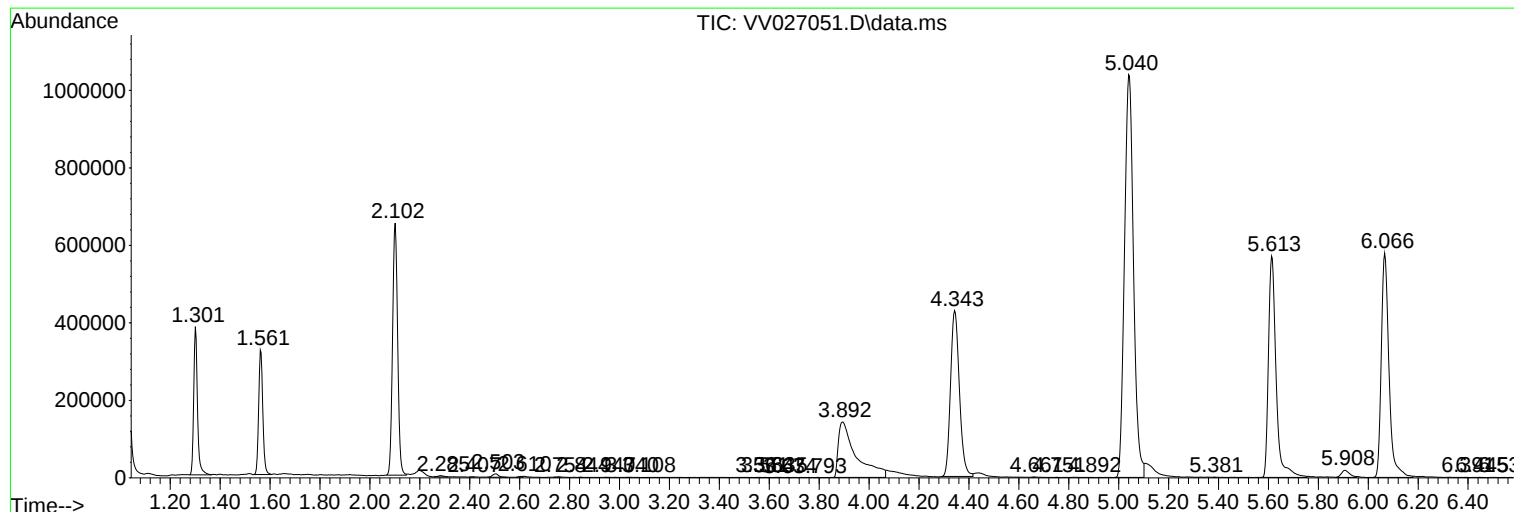

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072822\
Data File : VV027051.D
Acq On : 28 Jul 2022 22:02
Operator : SY/MD
Sample : VV0728WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK239

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072822\
Data File : VV027051.D
Acq On : 28 Jul 2022 22:02
Operator : SY/MD
Sample : VV0728WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK239

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc