

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072822\
 Data File : VV027055.D
 Acq On : 28 Jul 2022 23:40
 Operator : SY/MD
 Sample : N3899-02 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUR1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
 Title : VOC Analysis

Signal : TIC: VV027055.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	74	81	102	rVB	366502	383213	16.28%	2.212%
2	1.561	155	162	177	rBV	292998	335793	14.26%	1.938%
3	2.101	319	330	347	rBV	616140	877695	37.28%	5.066%
4	2.410	422	426	427	rBV2	521	375	0.02%	0.002%
5	2.503	444	455	465	rBV2	12086	19882	0.84%	0.115%
6	2.616	480	490	497	rBV7	1352	2639	0.11%	0.015%
7	2.693	511	514	517	rVB3	415	309	0.01%	0.002%
8	2.818	547	553	556	rBV4	520	525	0.02%	0.003%
9	2.918	581	584	594	rVB2	505	597	0.03%	0.003%
10	2.960	594	597	600	rBV2	337	251	0.01%	0.001%
11	3.104	639	642	649	rBV2	632	749	0.03%	0.004%
12	3.262	689	691	697	rVB2	498	431	0.02%	0.002%
13	3.513	766	769	774	rBV3	348	333	0.01%	0.002%
14	3.728	831	836	840	rBV2	297	293	0.01%	0.002%
15	3.760	840	846	850	rVB2	476	439	0.02%	0.003%
16	3.786	850	854	859	rBV2	477	484	0.02%	0.003%
17	3.834	866	869	873	rBV3	367	361	0.02%	0.002%
18	3.895	876	888	934	rBV2	109237	502032	21.32%	2.898%
19	4.342	1011	1027	1050	rBV	382068	944528	40.12%	5.452%
20	4.654	1122	1124	1129	rBV4	550	439	0.02%	0.003%
21	4.722	1142	1145	1152	rVB3	735	778	0.03%	0.004%
22	4.757	1152	1156	1160	rBV2	501	587	0.02%	0.003%
23	4.834	1178	1180	1183	rVB	409	263	0.01%	0.002%
24	4.876	1189	1193	1196	rBV2	422	278	0.01%	0.002%
25	4.918	1203	1206	1214	rVB3	496	530	0.02%	0.003%
26	4.969	1219	1222	1224	rBV	408	281	0.01%	0.002%
27	5.040	1227	1244	1264	rBV2	929381	2354444	100.00%	13.591%
28	5.391	1351	1353	1357	rBV3	512	292	0.01%	0.002%
29	5.439	1365	1368	1373	rVB4	387	391	0.02%	0.002%
30	5.481	1377	1381	1385	rBV3	480	473	0.02%	0.003%
31	5.612	1410	1422	1463	rBV	600558	1262891	53.64%	7.290%
32	5.905	1503	1513	1532	rBV3	15823	34890	1.48%	0.201%
33	6.066	1549	1563	1604	rBV	519711	1099180	46.69%	6.345%
34	6.355	1651	1653	1656	rVB2	554	295	0.01%	0.002%
35	6.384	1656	1662	1664	rVB3	317	268	0.01%	0.002%
36	6.413	1667	1671	1673	rBV	453	369	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072822\
 Data File : VV027055.D
 Acq On : 28 Jul 2022 23:40
 Operator : SY/MD
 Sample : N3899-02 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUR1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
 Title : VOC Analysis

37	6.516	1699	1703	1707	rVB3	323	305	0.01%	0.002%
38	6.542	1707	1711	1712	rBV3	423	308	0.01%	0.002%
39	6.600	1724	1729	1732	rVB	444	261	0.01%	0.002%
40	6.661	1741	1748	1751	rBV6	855	917	0.04%	0.005%
41	6.866	1810	1812	1818	rVB2	473	300	0.01%	0.002%
42	6.895	1818	1821	1826	rBV2	400	320	0.01%	0.002%
43	6.985	1835	1849	1885	rBV	239945	459359	19.51%	2.652%
44	7.313	1939	1951	1987	rBV	1044359	1872787	79.54%	10.810%
45	7.619	2036	2046	2077	rBV	166313	309345	13.14%	1.786%
46	7.844	2111	2116	2122	rBV5	722	790	0.03%	0.005%
47	7.886	2122	2129	2133	rBV6	555	789	0.03%	0.005%
48	7.982	2151	2159	2168	rVB7	2316	3918	0.17%	0.023%
49	8.021	2168	2171	2173	rBV2	402	319	0.01%	0.002%
50	8.091	2181	2193	2234	rBV	486548	1096490	46.57%	6.329%
51	8.349	2271	2273	2277	rVB4	769	511	0.02%	0.003%
52	8.464	2305	2309	2311	rBV3	710	431	0.02%	0.002%
53	8.577	2341	2344	2348	rBV3	721	601	0.03%	0.003%
54	8.599	2348	2351	2354	rBV2	424	292	0.01%	0.002%
55	8.657	2368	2369	2372	rVB2	590	248	0.01%	0.001%
56	8.680	2372	2376	2380	rBV3	433	377	0.02%	0.002%
57	8.786	2403	2409	2413	rVB3	437	387	0.02%	0.002%
58	8.850	2417	2429	2461	rBV	939807	1556379	66.10%	8.984%
59	9.172	2525	2529	2532	rVB2	563	536	0.02%	0.003%
60	9.259	2554	2556	2562	rVB2	343	344	0.01%	0.002%
61	9.284	2562	2564	2568	rBV	476	279	0.01%	0.002%
62	9.342	2577	2582	2585	rBV3	375	337	0.01%	0.002%
63	9.435	2606	2611	2613	rBV	323	263	0.01%	0.002%
64	9.596	2658	2661	2663	rBV3	459	269	0.01%	0.002%
65	9.715	2695	2698	2704	rVB2	431	456	0.02%	0.003%
66	9.905	2753	2757	2761	rBV2	387	369	0.02%	0.002%
67	9.988	2777	2783	2787	rBV3	412	505	0.02%	0.003%
68	10.043	2795	2800	2805	rBV2	287	307	0.01%	0.002%
69	10.214	2841	2853	2879	rBV	746435	1207798	51.30%	6.972%
70	10.365	2897	2900	2903	rVB3	388	239	0.01%	0.001%
71	10.458	2926	2929	2935	rVB3	302	239	0.01%	0.001%
72	10.580	2960	2967	2970	rBV4	392	405	0.02%	0.002%
73	10.635	2979	2984	2987	rVB2	369	329	0.01%	0.002%
74	10.850	3047	3051	3052	rBV3	559	395	0.02%	0.002%
75	10.992	3092	3095	3098	rBV2	343	258	0.01%	0.001%
76	11.088	3121	3125	3129	rBV3	464	333	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072822\
 Data File : VV027055.D
 Acq On : 28 Jul 2022 23:40
 Operator : SY/MD
 Sample : N3899-02 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUR1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
 Title : VOC Analysis

77	11.188	3151	3156	3163	rBV5	772	990	0.04%	0.006%
78	11.249	3163	3175	3200	rBV	886746	1363514	57.91%	7.871%
79	11.625	3279	3292	3316	rVV	962202	1539937	65.41%	8.889%
80	11.837	3356	3358	3361	rBV3	341	276	0.01%	0.002%
81	11.882	3369	3372	3376	rBV2	397	402	0.02%	0.002%
82	12.104	3438	3441	3443	rBV2	482	265	0.01%	0.002%
83	12.512	3564	3568	3571	rBV2	469	397	0.02%	0.002%
84	12.654	3605	3612	3617	rVB4	1052	1279	0.05%	0.007%
85	12.686	3617	3622	3625	rBV2	430	488	0.02%	0.003%
86	13.027	3723	3728	3733	rBV2	589	629	0.03%	0.004%
87	13.088	3743	3747	3750	rBV3	456	489	0.02%	0.003%
88	13.271	3803	3804	3812	rVB3	878	782	0.03%	0.005%
89	13.506	3868	3877	3902	rVB	34914	60442	2.57%	0.349%
90	13.635	3913	3917	3919	rVB3	636	398	0.02%	0.002%
91	13.725	3941	3945	3948	rBV2	497	489	0.02%	0.003%
92	13.918	3999	4005	4006	rBV2	480	533	0.02%	0.003%
93	14.049	4043	4046	4051	rBV2	472	406	0.02%	0.002%
94	14.123	4066	4069	4070	rBV	601	343	0.01%	0.002%
95	14.262	4108	4112	4115	rBV	428	368	0.02%	0.002%
96	14.413	4156	4159	4161	rBV4	557	352	0.01%	0.002%
97	14.586	4209	4213	4218	rVB3	689	583	0.02%	0.003%
98	14.644	4223	4231	4233	rBV5	1370	1955	0.08%	0.011%
99	14.734	4257	4259	4262	rVB3	499	246	0.01%	0.001%
100	14.815	4280	4284	4286	rBV3	1727	1545	0.07%	0.009%




Sum of corrected areas: 17323781

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072822\
Data File : VV027055.D
Acq On : 28 Jul 2022 23:40
Operator : SY/MD
Sample : N3899-02 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUR1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

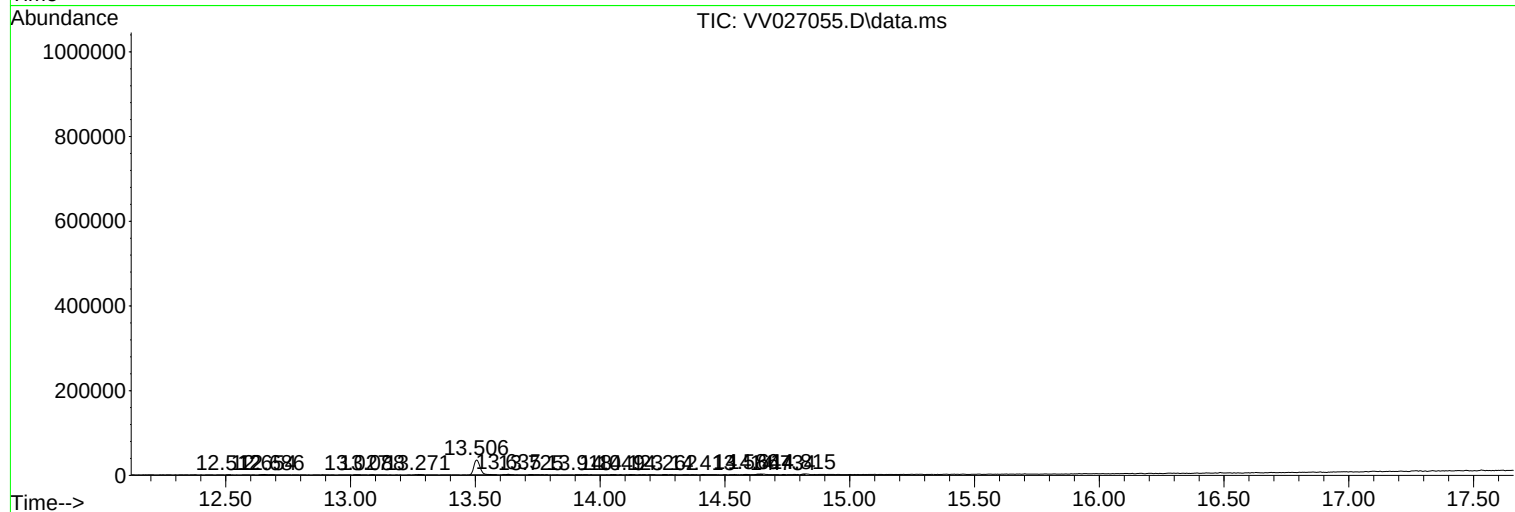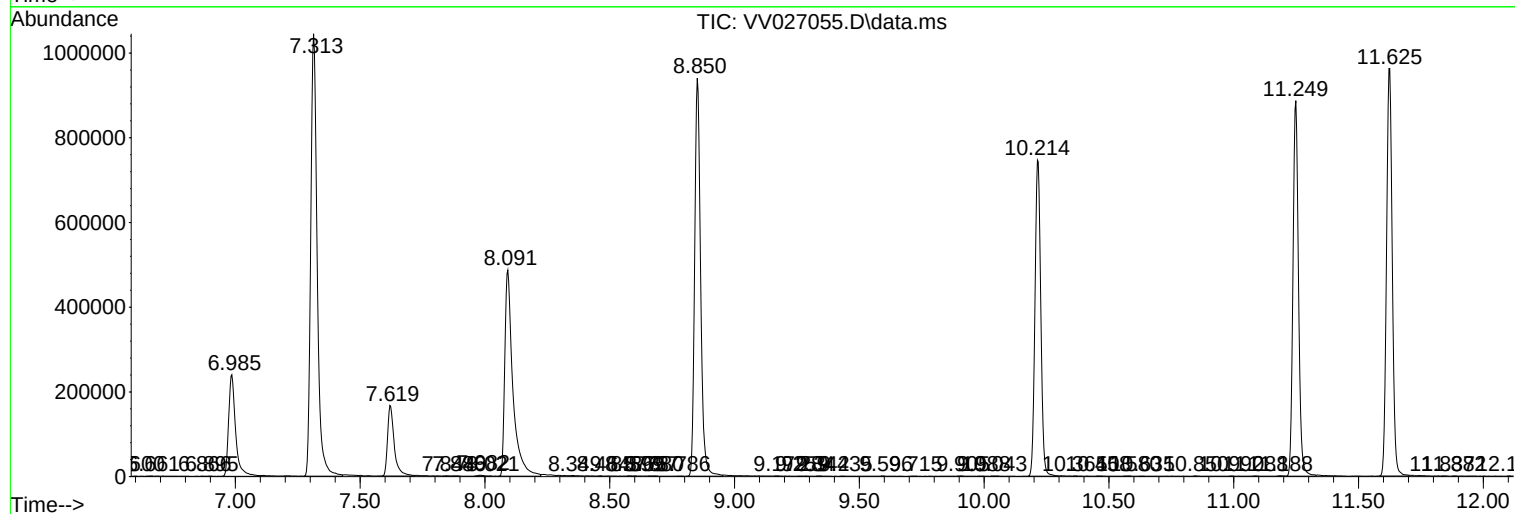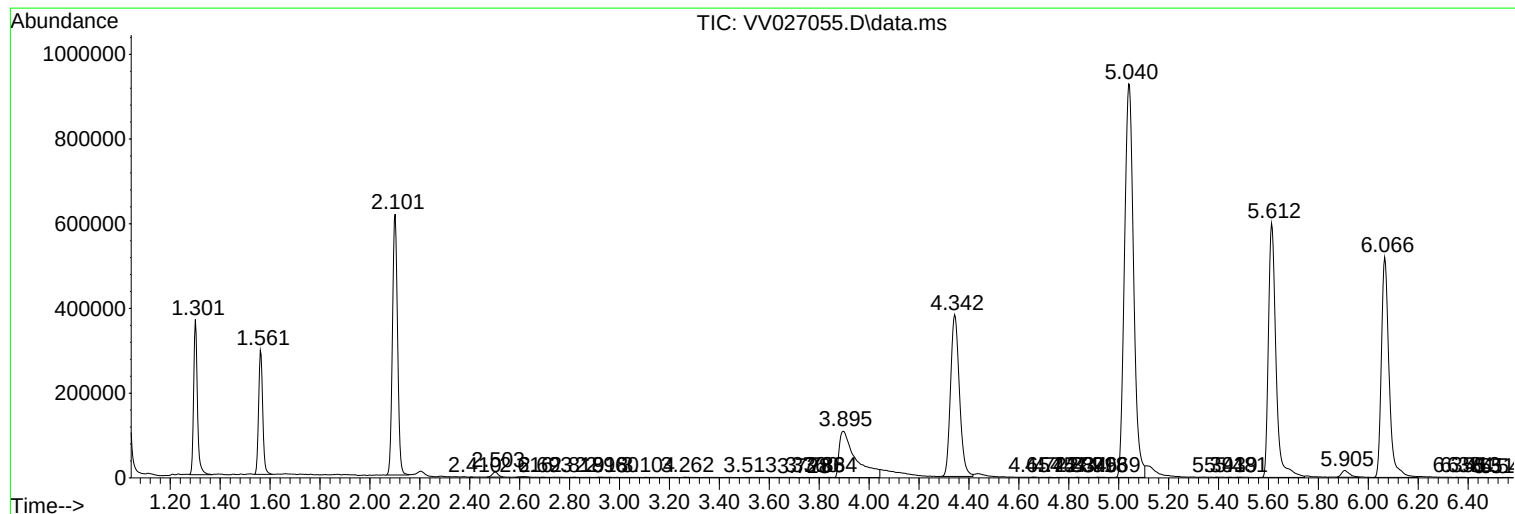

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072822\
Data File : VV027055.D
Acq On : 28 Jul 2022 23:40
Operator : SY/MD
Sample : N3899-02 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUR1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072822\
Data File : VV027055.D
Acq On : 28 Jul 2022 23:40
Operator : SY/MD
Sample : N3899-02 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUR1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc