

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072822\
 Data File : VV027059.D
 Acq On : 29 Jul 2022 01:18
 Operator : SY/MD
 Sample : N3899-14 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUS1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
 Title : VOC Analysis

Signal : TIC: VV027059.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	75	81	102	rVB	357755	378633	15.64%	2.211%
2	1.565	156	163	177	rVB	291321	332278	13.72%	1.941%
3	2.102	320	330	345	rBV	619732	875935	36.17%	5.116%
4	2.503	445	455	468	rBV3	10246	18256	0.75%	0.107%
5	2.703	515	517	519	rBV2	326	164	0.01%	0.001%
6	2.809	547	550	551	rBV	468	302	0.01%	0.002%
7	3.018	613	615	617	rBV2	155	80	0.00%	0.000%
8	3.056	624	627	629	rBV	368	266	0.01%	0.002%
9	3.101	638	641	643	rBV2	233	176	0.01%	0.001%
10	3.333	711	713	715	rBV	254	108	0.00%	0.001%
11	3.349	715	718	722	rBV3	340	299	0.01%	0.002%
12	3.417	734	739	743	rBV2	287	335	0.01%	0.002%
13	3.703	824	828	835	rVB2	528	617	0.03%	0.004%
14	3.735	835	838	840	rBV2	283	188	0.01%	0.001%
15	3.812	860	862	866	rVB	281	175	0.01%	0.001%
16	3.835	866	869	871	rBV	257	160	0.01%	0.001%
17	3.889	874	886	920	rBV2	115633	471169	19.46%	2.752%
18	4.343	1012	1027	1049	rBV	383793	944736	39.02%	5.518%
19	4.667	1126	1128	1129	rBV	327	93	0.00%	0.001%
20	4.902	1199	1201	1202	rVB	132	30	0.00%	0.000%
21	4.912	1202	1204	1205	rBV	358	163	0.01%	0.001%
22	4.941	1212	1213	1214	rBV	396	80	0.00%	0.000%
23	5.040	1227	1244	1302	rBV2	932973	2421434	100.00%	14.142%
24	5.613	1410	1422	1461	rBV	602560	1253366	51.76%	7.320%
25	6.066	1549	1563	1599	rBV	518350	1092668	45.12%	6.382%
26	6.375	1657	1659	1660	rBV	325	120	0.00%	0.001%
27	6.442	1678	1680	1681	rBV2	197	58	0.00%	0.000%
28	6.449	1681	1682	1686	rVV2	331	207	0.01%	0.001%
29	6.478	1689	1691	1693	rBV2	112	51	0.00%	0.000%
30	6.494	1693	1696	1698	rBV2	195	137	0.01%	0.001%
31	6.613	1727	1733	1735	rBV2	297	215	0.01%	0.001%
32	6.664	1743	1749	1752	rBV3	455	596	0.02%	0.003%
33	6.767	1778	1781	1782	rBV2	238	122	0.01%	0.001%
34	6.796	1786	1790	1793	rVB3	418	289	0.01%	0.002%
35	6.812	1793	1795	1797	rBV	204	131	0.01%	0.001%
36	6.822	1797	1798	1799	rVB	412	80	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW072822\
 Data File : VW027059.D
 Acq On : 29 Jul 2022 01:18
 Operator : SY/MD
 Sample : N3899-14 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUS1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
 Title : VOC Analysis

37	6.841	1799	1804	1809	rVB3	416	438	0.02%	0.003%
38	6.867	1809	1812	1813	rBV	135	92	0.00%	0.001%
39	6.905	1821	1824	1825	rBV	214	100	0.00%	0.001%
40	6.915	1825	1827	1829	rBV	149	83	0.00%	0.000%
41	6.982	1836	1848	1882	rBV	229012	442680	18.28%	2.585%
42	7.314	1939	1951	1987	rBV	1040960	1852540	76.51%	10.820%
43	7.619	2036	2046	2079	rBV	162033	303658	12.54%	1.773%
44	7.908	2133	2136	2140	rBV2	441	332	0.01%	0.002%
45	8.092	2182	2193	2233	rBV	480586	1094519	45.20%	6.392%
46	8.635	2361	2362	2368	rVB3	434	326	0.01%	0.002%
47	8.670	2368	2373	2378	rBV3	363	460	0.02%	0.003%
48	8.850	2417	2429	2466	rBV	939591	1562943	64.55%	9.128%
49	9.207	2538	2540	2543	rBV3	377	287	0.01%	0.002%
50	9.423	2604	2607	2609	rBV2	228	113	0.00%	0.001%
51	9.474	2620	2623	2625	rBV2	364	226	0.01%	0.001%
52	9.503	2630	2632	2635	rVB	349	178	0.01%	0.001%
53	9.519	2635	2637	2638	rBV	407	199	0.01%	0.001%
54	9.555	2643	2648	2651	rBV2	424	321	0.01%	0.002%
55	9.690	2688	2690	2692	rBV	212	81	0.00%	0.000%
56	9.706	2692	2695	2702	rVB2	398	457	0.02%	0.003%
57	9.799	2722	2724	2726	rBV	163	88	0.00%	0.001%
58	9.844	2735	2738	2741	rBV2	357	266	0.01%	0.002%
59	9.902	2752	2756	2759	rBV2	419	398	0.02%	0.002%
60	9.982	2779	2781	2782	rBV	130	33	0.00%	0.000%
61	10.011	2787	2790	2791	rBV	162	93	0.00%	0.001%
62	10.214	2841	2853	2876	rBV	752554	1204972	49.76%	7.038%
63	10.455	2925	2928	2929	rBV2	487	244	0.01%	0.001%
64	10.580	2963	2967	2972	rBV4	489	465	0.02%	0.003%
65	10.834	3041	3046	3048	rBV2	251	234	0.01%	0.001%
66	10.854	3048	3052	3055	rVB3	530	424	0.02%	0.002%
67	10.870	3055	3057	3060	rBV	269	158	0.01%	0.001%
68	10.982	3088	3092	3094	rBV2	303	269	0.01%	0.002%
69	11.040	3106	3110	3112	rBV	441	308	0.01%	0.002%
70	11.082	3121	3123	3127	rBV2	316	257	0.01%	0.002%
71	11.182	3150	3154	3156	rBV	513	368	0.02%	0.002%
72	11.249	3163	3175	3206	rBV	861747	1343526	55.48%	7.847%
73	11.622	3279	3291	3318	rBV	955814	1515636	62.59%	8.852%
74	12.532	3572	3574	3576	rBV3	427	240	0.01%	0.001%
75	12.857	3674	3675	3679	rBV	309	265	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072822\
Data File : VV027059.D
Acq On : 29 Jul 2022 01:18
Operator : SY/MD
Sample : N3899-14 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUS1

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
Title : VOC Analysis




Sum of corrected areas: 17121994

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072822\
Data File : VV027059.D
Acq On : 29 Jul 2022 01:18
Operator : SY/MD
Sample : N3899-14 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUS1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

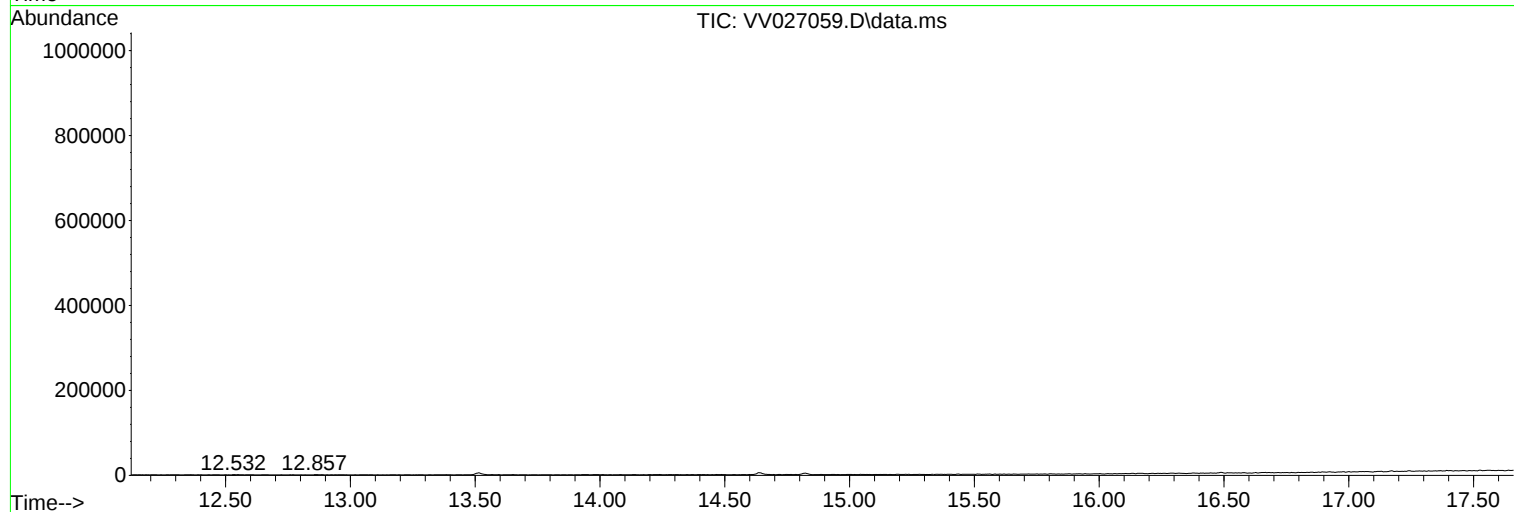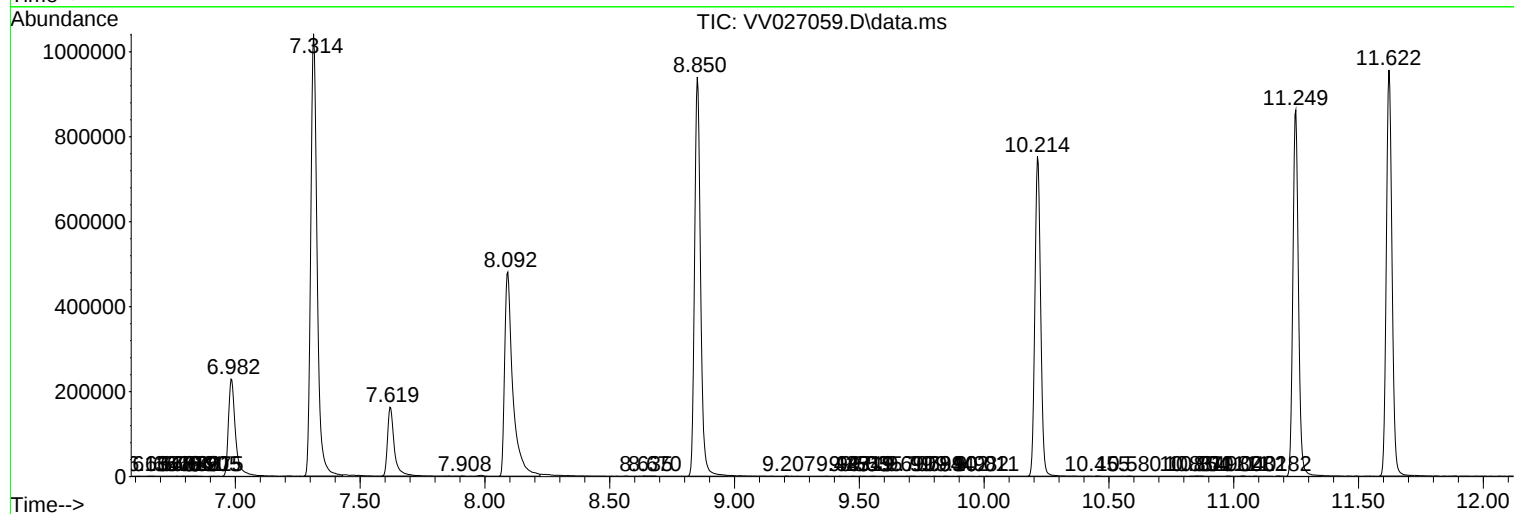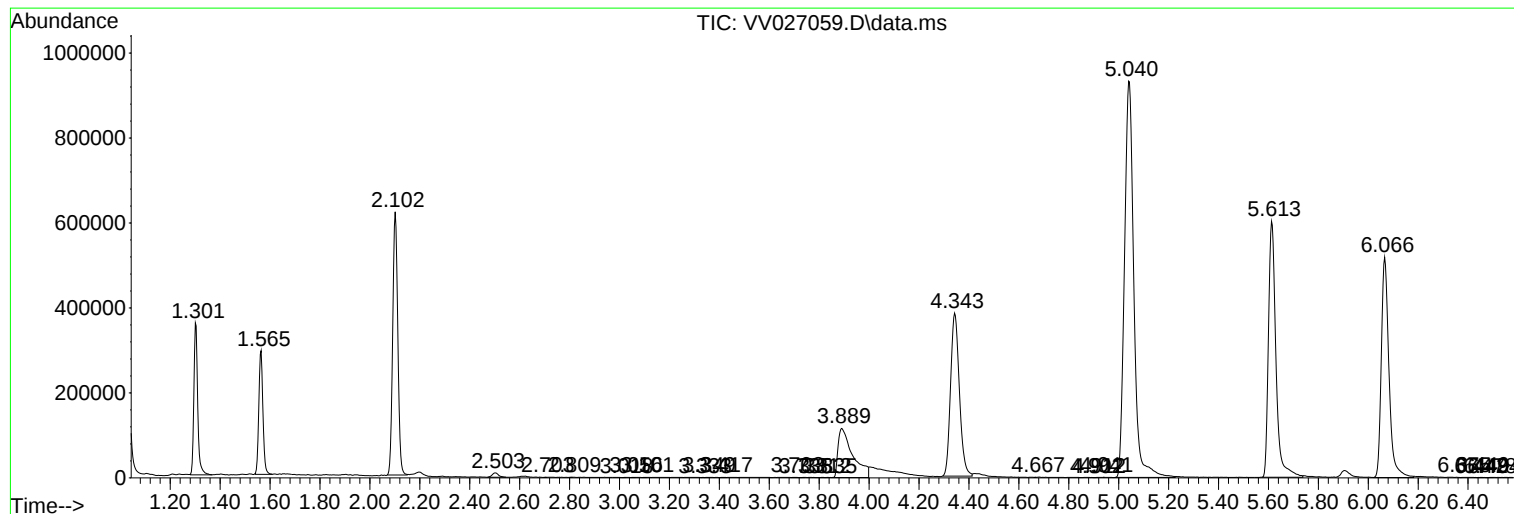

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072822\
Data File : VV027059.D
Acq On : 29 Jul 2022 01:18
Operator : SY/MD
Sample : N3899-14 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUS1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072822\
Data File : VV027059.D
Acq On : 29 Jul 2022 01:18
Operator : SY/MD
Sample : N3899-14 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUS1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc