

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072822\
 Data File : VV027060.D
 Acq On : 29 Jul 2022 01:43
 Operator : SY/MD
 Sample : N3899-15 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUS2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M

Title : VOC Analysis

Signal : TIC: VV027060.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	75	81	103	rVB	361353	383113	15.76%	2.234%
2	1.564	155	163	177	rBV	294590	336387	13.84%	1.961%
3	2.101	320	330	345	rBV	619078	874640	35.98%	5.099%
4	2.500	446	454	469	rVB2	15906	26704	1.10%	0.156%
5	2.989	603	606	609	rBV	264	199	0.01%	0.001%
6	3.030	618	619	622	rBV	263	171	0.01%	0.001%
7	3.050	622	625	627	rBV3	358	231	0.01%	0.001%
8	3.182	662	666	669	rBV3	420	386	0.02%	0.002%
9	3.204	670	673	675	rBV	338	238	0.01%	0.001%
10	3.301	700	703	705	rBV2	222	159	0.01%	0.001%
11	3.323	707	710	714	rVB2	398	330	0.01%	0.002%
12	3.349	714	718	719	rBV	222	111	0.00%	0.001%
13	3.461	751	753	755	rBV	182	78	0.00%	0.000%
14	3.493	761	763	768	rVB3	218	202	0.01%	0.001%
15	3.526	769	773	774	rBV	317	174	0.01%	0.001%
16	3.609	796	799	800	rBV	288	155	0.01%	0.001%
17	3.664	810	816	818	rBV2	267	266	0.01%	0.002%
18	3.715	829	832	837	rBV2	398	349	0.01%	0.002%
19	3.770	847	849	852	rBV	194	101	0.00%	0.001%
20	3.796	852	857	859	rBV2	323	283	0.01%	0.002%
21	3.892	876	887	918	rBV2	112355	471519	19.40%	2.749%
22	4.342	1012	1027	1050	rBV	384921	950523	39.10%	5.542%
23	4.805	1165	1171	1173	rBV2	454	587	0.02%	0.003%
24	4.825	1176	1177	1179	rBV	183	75	0.00%	0.000%
25	4.837	1179	1181	1183	rBV	168	101	0.00%	0.001%
26	4.850	1183	1185	1186	rVV	322	77	0.00%	0.000%
27	4.915	1203	1205	1206	rBV	311	131	0.01%	0.001%
28	5.040	1227	1244	1289	rBV2	931073	2430970	100.00%	14.173%
29	5.481	1379	1381	1383	rBV	503	254	0.01%	0.001%
30	5.612	1409	1422	1462	rBV	585775	1236820	50.88%	7.211%
31	5.908	1504	1514	1531	rVB4	15451	33057	1.36%	0.193%
32	6.066	1548	1563	1596	rBV	519432	1095413	45.06%	6.387%
33	6.310	1637	1639	1640	rBV2	404	166	0.01%	0.001%
34	6.358	1650	1654	1657	rBV2	307	264	0.01%	0.002%
35	6.378	1657	1660	1662	rBV2	319	250	0.01%	0.001%
36	6.490	1692	1695	1699	rBV2	541	376	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072822\
 Data File : VV027060.D
 Acq On : 29 Jul 2022 01:43
 Operator : SY/MD
 Sample : N3899-15 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUS2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
 Title : VOC Analysis

37	6.509	1699	1701	1703	rVB	316	119	0.00%	0.001%
38	6.574	1717	1721	1724	rVB	441	251	0.01%	0.001%
39	6.596	1724	1728	1729	rBV2	395	252	0.01%	0.001%
40	6.632	1737	1739	1740	rBV2	278	130	0.01%	0.001%
41	6.673	1751	1752	1754	rBV	160	62	0.00%	0.000%
42	6.709	1760	1763	1764	rBV2	215	97	0.00%	0.001%
43	6.744	1772	1774	1779	rVB	478	300	0.01%	0.002%
44	6.767	1779	1781	1782	rBV	295	145	0.01%	0.001%
45	6.828	1798	1800	1802	rBV2	139	86	0.00%	0.001%
46	6.844	1802	1805	1806	rBV	186	100	0.00%	0.001%
47	6.853	1806	1808	1813	rVB3	210	157	0.01%	0.001%
48	6.905	1821	1824	1828	rBV3	268	203	0.01%	0.001%
49	6.927	1828	1831	1833	rBV2	256	134	0.01%	0.001%
50	6.940	1833	1835	1838	rBV2	145	92	0.00%	0.001%
51	6.982	1838	1848	1880	rBV	233248	448701	18.46%	2.616%
52	7.313	1939	1951	1986	rBV	1033925	1860105	76.52%	10.845%
53	7.619	2036	2046	2074	rBV	163116	302499	12.44%	1.764%
54	7.860	2118	2121	2123	rBV2	571	390	0.02%	0.002%
55	7.921	2137	2140	2143	rBV2	445	414	0.02%	0.002%
56	7.982	2153	2159	2166	rBV5	1948	2898	0.12%	0.017%
57	8.091	2182	2193	2235	rBV	485415	1090981	44.88%	6.361%
58	8.558	2334	2338	2341	rBV3	481	448	0.02%	0.003%
59	8.667	2370	2372	2377	rBV4	208	137	0.01%	0.001%
60	8.725	2385	2390	2392	rBV2	240	235	0.01%	0.001%
61	8.751	2397	2398	2400	rBV	156	83	0.00%	0.000%
62	8.792	2406	2411	2417	rBV4	469	539	0.02%	0.003%
63	8.850	2417	2429	2457	rBV	913832	1545501	63.58%	9.011%
64	9.140	2517	2519	2521	rBV2	485	255	0.01%	0.001%
65	9.175	2527	2530	2531	rBV2	319	175	0.01%	0.001%
66	9.236	2546	2549	2552	rBV2	348	298	0.01%	0.002%
67	9.284	2560	2564	2565	rBV2	521	288	0.01%	0.002%
68	9.342	2580	2582	2584	rBV2	409	135	0.01%	0.001%
69	9.377	2591	2593	2595	rBV	380	207	0.01%	0.001%
70	9.445	2609	2614	2616	rBV2	315	307	0.01%	0.002%
71	9.622	2666	2669	2674	rVB2	323	289	0.01%	0.002%
72	9.680	2685	2687	2690	rVB3	171	85	0.00%	0.000%
73	9.696	2690	2692	2696	rBV2	373	298	0.01%	0.002%
74	9.799	2722	2724	2728	rBV	266	233	0.01%	0.001%
75	9.815	2728	2729	2730	rVV	601	129	0.01%	0.001%
76	9.840	2730	2737	2742	rVV3	228	341	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072822\
 Data File : VV027060.D
 Acq On : 29 Jul 2022 01:43
 Operator : SY/MD
 Sample : N3899-15 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUS2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
 Title : VOC Analysis

77	9.863	2742	2744	2748	rVB2	413	270	0.01%	0.002%
78	9.892	2748	2753	2757	rBV2	391	517	0.02%	0.003%
79	9.937	2762	2767	2770	rBV2	324	297	0.01%	0.002%
80	9.976	2776	2779	2784	rBV3	288	234	0.01%	0.001%
81	10.014	2788	2791	2793	rBV2	272	146	0.01%	0.001%
82	10.037	2793	2798	2799	rBV	300	243	0.01%	0.001%
83	10.098	2813	2817	2820	rBV2	552	478	0.02%	0.003%
84	10.117	2821	2823	2825	rVV2	316	135	0.01%	0.001%
85	10.213	2840	2853	2876	rBV	744479	1210219	49.78%	7.056%
86	10.763	3021	3024	3028	rBV	223	195	0.01%	0.001%
87	10.812	3036	3039	3040	rBV	198	99	0.00%	0.001%
88	10.850	3047	3051	3052	rBV3	547	418	0.02%	0.002%
89	10.889	3061	3063	3069	rBV3	416	352	0.01%	0.002%
90	11.004	3096	3099	3101	rBV	223	151	0.01%	0.001%
91	11.123	3133	3136	3140	rBV3	396	306	0.01%	0.002%
92	11.146	3141	3143	3144	rBV	262	112	0.00%	0.001%
93	11.172	3150	3151	3153	rBV	191	71	0.00%	0.000%
94	11.249	3162	3175	3199	rBV	841512	1314272	54.06%	7.663%
95	11.541	3262	3266	3267	rBV2	354	220	0.01%	0.001%
96	11.570	3272	3275	3279	rBV3	666	581	0.02%	0.003%
97	11.622	3279	3291	3321	rBV	957837	1518437	62.46%	8.853%
98	13.827	3975	3977	3979	rBV	471	220	0.01%	0.001%
99	14.027	4037	4039	4043	rVB3	687	385	0.02%	0.002%
100	14.741	4258	4261	4262	rBV2	823	462	0.02%	0.003%




Sum of corrected areas: 17151779

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072822\
Data File : VV027060.D
Acq On : 29 Jul 2022 01:43
Operator : SY/MD
Sample : N3899-15 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUS2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

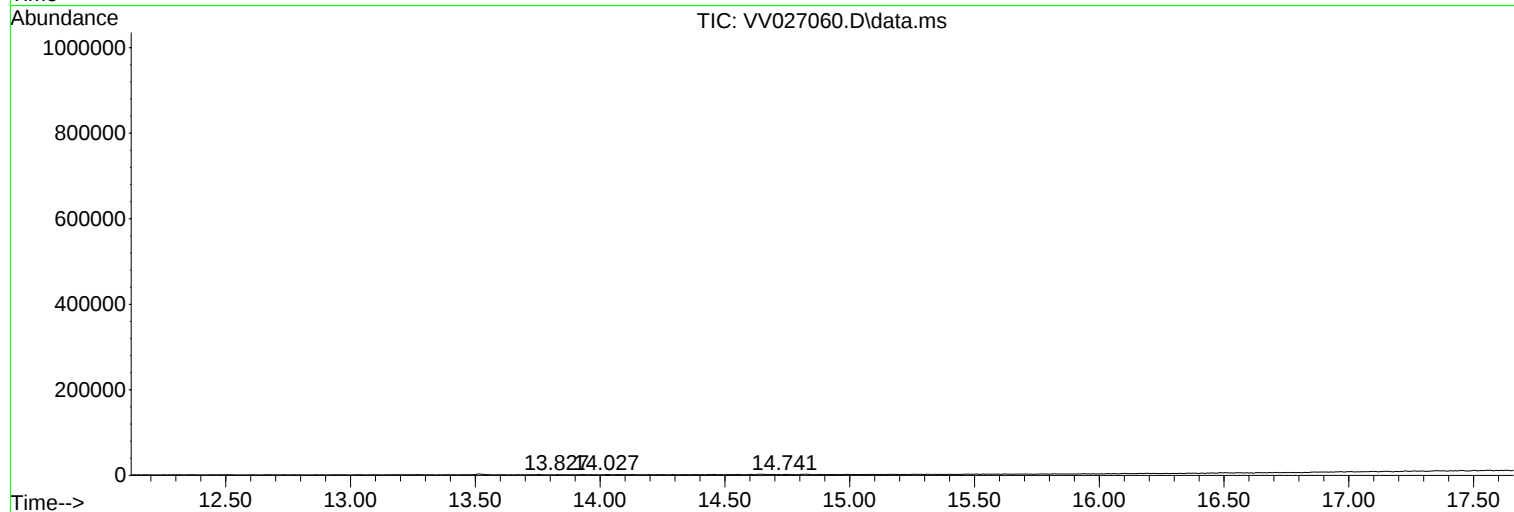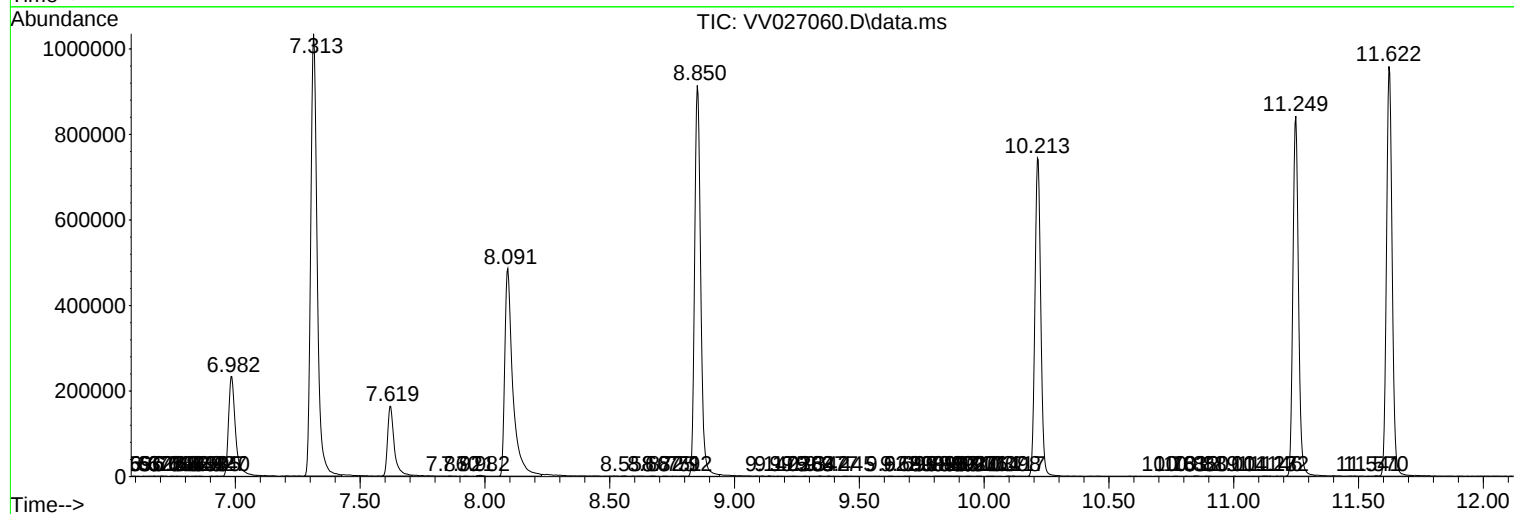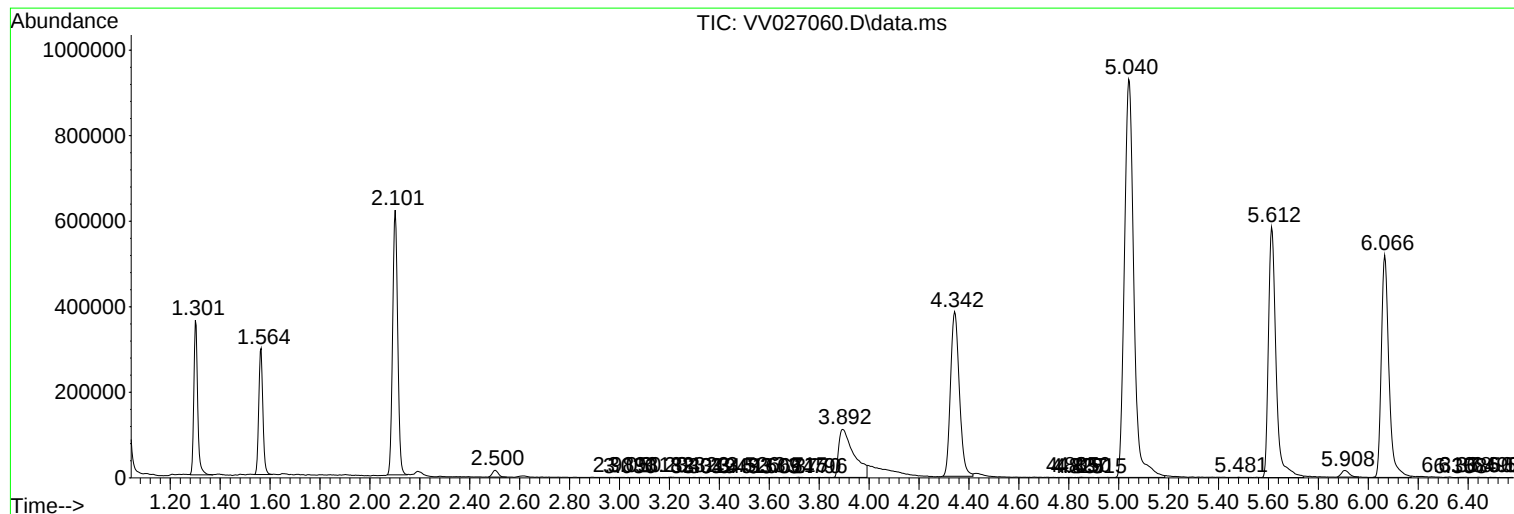

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072822\
Data File : VV027060.D
Acq On : 29 Jul 2022 01:43
Operator : SY/MD
Sample : N3899-15 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUS2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072822\
Data File : VV027060.D
Acq On : 29 Jul 2022 01:43
Operator : SY/MD
Sample : N3899-15 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUS2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc