

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072822\
 Data File : VV027061.D
 Acq On : 29 Jul 2022 02:07
 Operator : SY/MD
 Sample : N3899-16 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUS3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M

Title : VOC Analysis

Signal : TIC: VV027061.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	74	81	100	rVB	348447	371294	15.62%	2.220%
2	1.564	154	163	175	rBV	282873	328776	13.83%	1.966%
3	2.101	320	330	345	rBV	607264	854142	35.92%	5.107%
4	2.503	446	455	470	rVB2	14374	25349	1.07%	0.152%
5	2.609	480	488	489	rBV4	1374	1355	0.06%	0.008%
6	2.712	519	520	525	rVB3	560	363	0.02%	0.002%
7	2.818	550	553	558	rVB2	575	434	0.02%	0.003%
8	2.841	558	560	564	rBV2	429	346	0.01%	0.002%
9	2.992	605	607	613	rVB	461	294	0.01%	0.002%
10	3.111	637	644	649	rBV3	473	622	0.03%	0.004%
11	3.137	649	652	658	rVB2	362	332	0.01%	0.002%
12	3.195	666	670	675	rVB3	342	311	0.01%	0.002%
13	3.352	715	719	721	rBV	359	278	0.01%	0.002%
14	3.635	799	807	813	rBV3	399	603	0.03%	0.004%
15	3.831	865	868	874	rVB2	405	361	0.02%	0.002%
16	3.886	874	885	919	rBV2	109572	432663	18.20%	2.587%
17	4.342	1011	1027	1054	rBV2	381557	945789	39.78%	5.655%
18	4.654	1121	1124	1128	rVV4	612	528	0.02%	0.003%
19	4.686	1131	1134	1138	rBV3	543	370	0.02%	0.002%
20	4.818	1172	1175	1178	rVB2	477	245	0.01%	0.001%
21	4.902	1197	1201	1203	rBV2	364	289	0.01%	0.002%
22	4.982	1222	1226	1228	rBV	888	606	0.03%	0.004%
23	5.040	1228	1244	1284	rVV2	910842	2377666	100.00%	14.217%
24	5.307	1325	1327	1330	rVB2	666	340	0.01%	0.002%
25	5.326	1330	1333	1336	rVB3	808	516	0.02%	0.003%
26	5.346	1336	1339	1343	rBV2	1065	858	0.04%	0.005%
27	5.400	1352	1356	1359	rBV3	618	558	0.02%	0.003%
28	5.465	1373	1376	1378	rBV2	385	259	0.01%	0.002%
29	5.612	1407	1422	1457	rBV	583341	1219351	51.28%	7.291%
30	5.908	1502	1514	1530	rBV4	15990	35417	1.49%	0.212%
31	6.066	1548	1563	1599	rBV	513294	1082834	45.54%	6.475%
32	6.307	1634	1638	1645	rVB4	586	682	0.03%	0.004%
33	6.452	1680	1683	1685	rBV2	498	366	0.02%	0.002%
34	6.490	1691	1695	1698	rBV	421	332	0.01%	0.002%
35	6.596	1724	1728	1730	rBV2	334	266	0.01%	0.002%
36	6.657	1745	1747	1750	rBV3	371	239	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072822\
 Data File : VV027061.D
 Acq On : 29 Jul 2022 02:07
 Operator : SY/MD
 Sample : N3899-16 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUS3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
 Title : VOC Analysis

37	6.799	1786	1791	1793	rVB2	419	280	0.01%	0.002%
38	6.815	1793	1796	1800	rVB2	503	314	0.01%	0.002%
39	6.847	1800	1806	1807	rBV2	453	415	0.02%	0.002%
40	6.918	1824	1828	1830	rBV2	359	306	0.01%	0.002%
41	6.982	1836	1848	1874	rBV	225246	431237	18.14%	2.579%
42	7.313	1939	1951	1983	rBV	992682	1772844	74.56%	10.601%
43	7.619	2036	2046	2078	rBV	160642	297197	12.50%	1.777%
44	7.812	2103	2106	2108	rBV3	545	360	0.02%	0.002%
45	7.863	2118	2122	2127	rVB6	379	373	0.02%	0.002%
46	7.940	2144	2146	2150	rVB3	503	366	0.02%	0.002%
47	7.972	2150	2156	2157	rBV4	1807	1407	0.06%	0.008%
48	8.091	2182	2193	2237	rBV	471480	1107131	46.56%	6.620%
49	8.394	2285	2287	2290	rBV3	525	267	0.01%	0.002%
50	8.484	2311	2315	2318	rBV3	506	393	0.02%	0.002%
51	8.545	2332	2334	2338	rVB3	569	339	0.01%	0.002%
52	8.625	2352	2359	2360	rBV4	610	587	0.02%	0.004%
53	8.741	2391	2395	2399	rBV3	445	359	0.02%	0.002%
54	8.850	2418	2429	2458	rBV	887672	1494081	62.84%	8.934%
55	9.146	2518	2521	2528	rVB5	359	382	0.02%	0.002%
56	9.181	2528	2532	2536	rBV3	317	325	0.01%	0.002%
57	9.255	2553	2555	2558	rVB2	535	314	0.01%	0.002%
58	9.477	2619	2624	2627	rBV2	330	382	0.02%	0.002%
59	9.590	2657	2659	2664	rVV2	482	345	0.01%	0.002%
60	9.657	2676	2680	2685	rBV3	504	421	0.02%	0.003%
61	10.111	2818	2821	2825	rBV2	284	261	0.01%	0.002%
62	10.214	2841	2853	2875	rBV	760306	1206524	50.74%	7.214%
63	10.374	2898	2903	2904	rBV3	347	316	0.01%	0.002%
64	10.410	2909	2914	2919	rVB4	404	492	0.02%	0.003%
65	10.632	2978	2983	2991	rBV2	517	708	0.03%	0.004%
66	10.670	2991	2995	2997	rBV2	397	266	0.01%	0.002%
67	10.734	3008	3015	3020	rBV2	480	723	0.03%	0.004%
68	10.844	3045	3049	3051	rBV	469	408	0.02%	0.002%
69	10.921	3070	3073	3078	rVB	469	361	0.02%	0.002%
70	10.995	3094	3096	3101	rVV2	500	321	0.01%	0.002%
71	11.059	3114	3116	3120	rVB3	430	294	0.01%	0.002%
72	11.114	3127	3133	3136	rBV3	438	419	0.02%	0.003%
73	11.136	3136	3140	3145	rBV	400	422	0.02%	0.003%
74	11.197	3156	3159	3162	rVB2	454	304	0.01%	0.002%
75	11.249	3162	3175	3200	rBV	793612	1255153	52.79%	7.505%
76	11.513	3254	3257	3265	rVB3	625	480	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072822\
 Data File : VV027061.D
 Acq On : 29 Jul 2022 02:07
 Operator : SY/MD
 Sample : N3899-16 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUS3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
 Title : VOC Analysis

77	11.564	3269	3273	3279	rBV3	628	791	0.03%	0.005%
78	11.622	3279	3291	3313	rBV	925699	1449865	60.98%	8.669%
79	11.863	3363	3366	3370	rBV3	488	398	0.02%	0.002%
80	12.152	3453	3456	3458	rBV2	398	241	0.01%	0.001%
81	12.207	3470	3473	3476	rBV2	415	284	0.01%	0.002%
82	12.934	3696	3699	3703	rVB2	426	276	0.01%	0.002%
83	13.255	3794	3799	3802	rBV2	372	384	0.02%	0.002%
84	13.352	3827	3829	3833	rBV2	358	248	0.01%	0.001%
85	13.448	3856	3859	3862	rBV2	474	328	0.01%	0.002%
86	13.500	3869	3875	3876	rBV3	657	513	0.02%	0.003%
87	14.107	4061	4064	4067	rBV2	477	437	0.02%	0.003%
88	14.168	4077	4083	4086	rBV3	634	694	0.03%	0.004%
89	14.229	4099	4102	4109	rBV4	649	587	0.02%	0.004%
90	14.426	4161	4163	4165	rBV3	526	297	0.01%	0.002%
91	14.477	4173	4179	4182	rBV3	796	798	0.03%	0.005%
92	14.654	4229	4234	4237	rBV3	808	778	0.03%	0.005%
93	14.773	4268	4271	4272	rBV2	567	283	0.01%	0.002%
94	14.969	4328	4332	4334	rVB3	537	333	0.01%	0.002%
95	15.139	4382	4385	4390	rVB4	895	610	0.03%	0.004%
96	15.168	4390	4394	4398	rBV4	917	855	0.04%	0.005%
97	15.223	4408	4411	4412	rBV2	837	460	0.02%	0.003%
98	15.390	4461	4463	4466	rBV2	650	421	0.02%	0.003%
99	15.609	4529	4531	4536	rBV2	752	641	0.03%	0.004%
100	16.088	4678	4680	4682	rBV2	1246	582	0.02%	0.003%




Sum of corrected areas: 16724015

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072822\
Data File : VV027061.D
Acq On : 29 Jul 2022 02:07
Operator : SY/MD
Sample : N3899-16 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUS3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
Quant Title : VOC Analysis

TIC Library :
TIC Integration Parameters: LSCINT.P

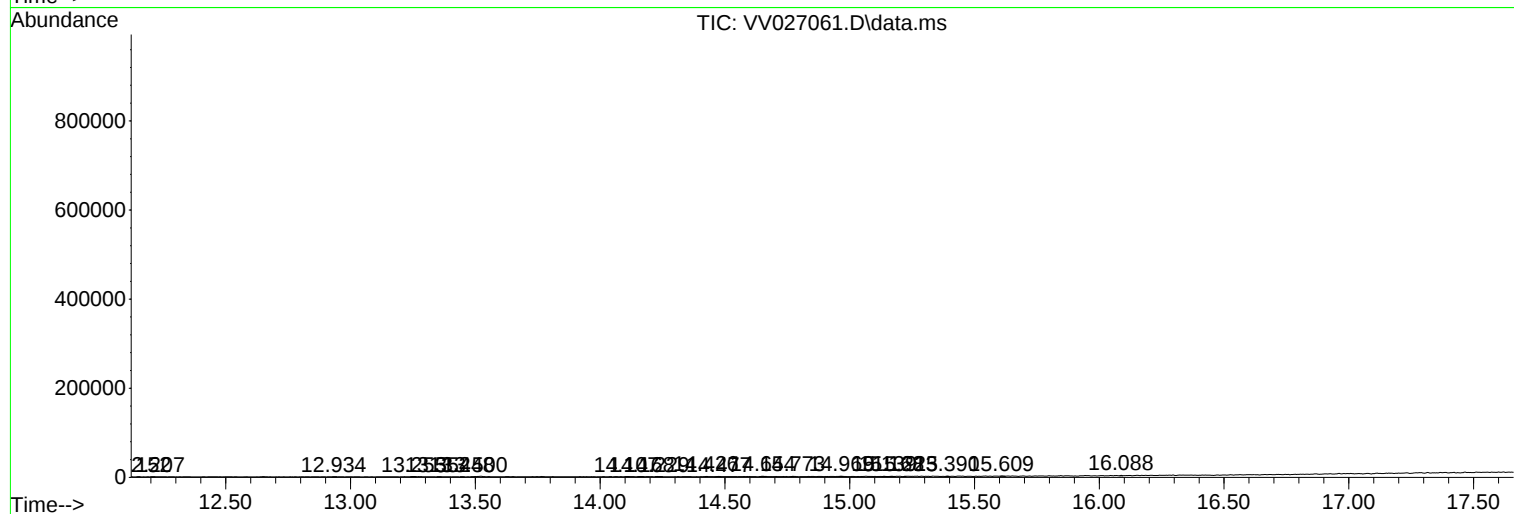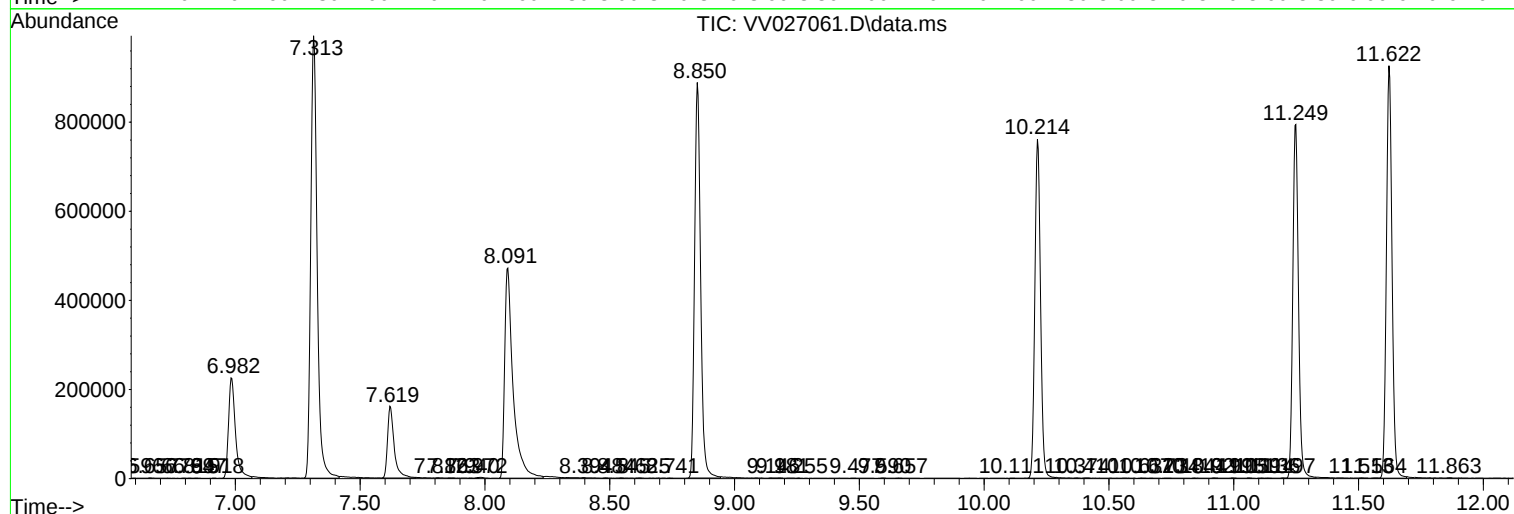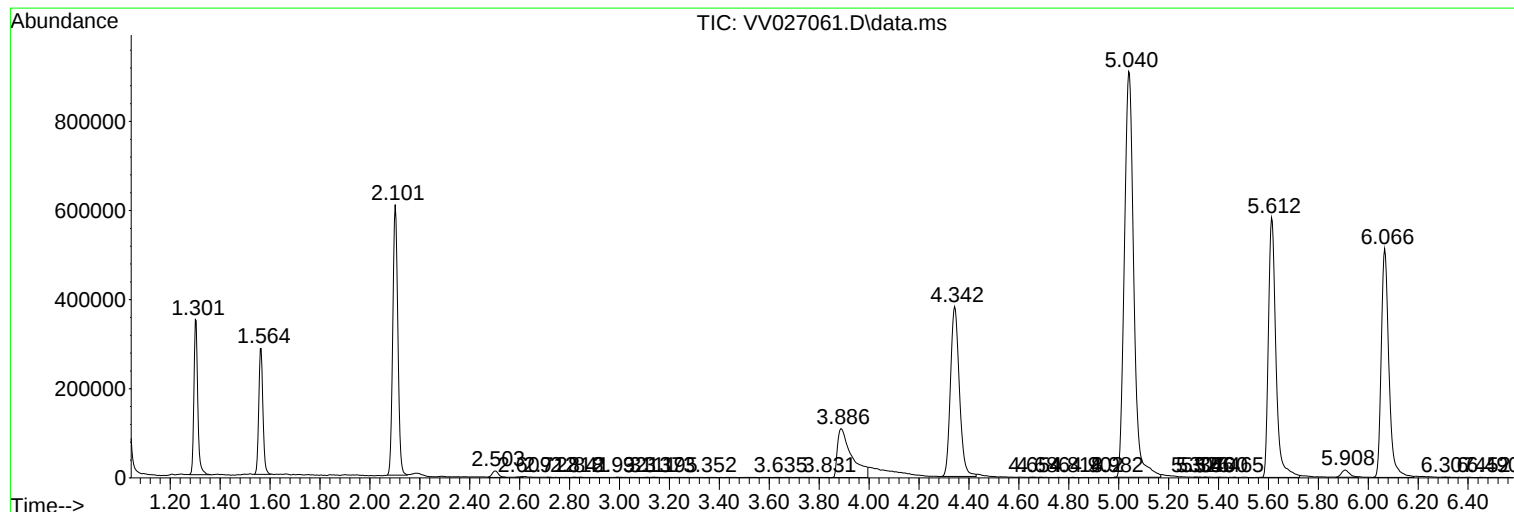

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072822\
Data File : VV027061.D
Acq On : 29 Jul 2022 02:07
Operator : SY/MD
Sample : N3899-16 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUS3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
Quant Title : VOC Analysis

TIC Library :
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072822\
Data File : VV027061.D
Acq On : 29 Jul 2022 02:07
Operator : SY/MD
Sample : N3899-16 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUS3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
Quant Title : VOC Analysis

TIC Library :
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc