
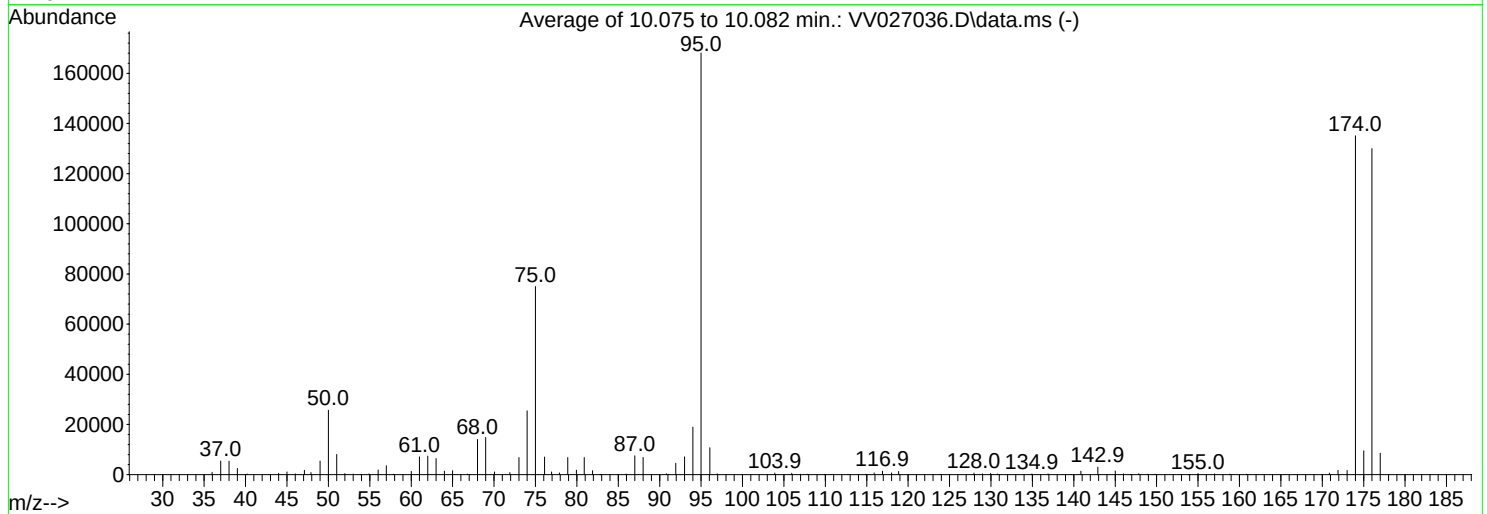


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072822\
 Data File : VV027036.D
 Acq On : 28 Jul 2022 09:47
 Operator : SY/MD
 Sample : BFB301
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB301

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
 Title : VOC Analysis
 Last Update : Sat Jul 30 01:28:32 2022

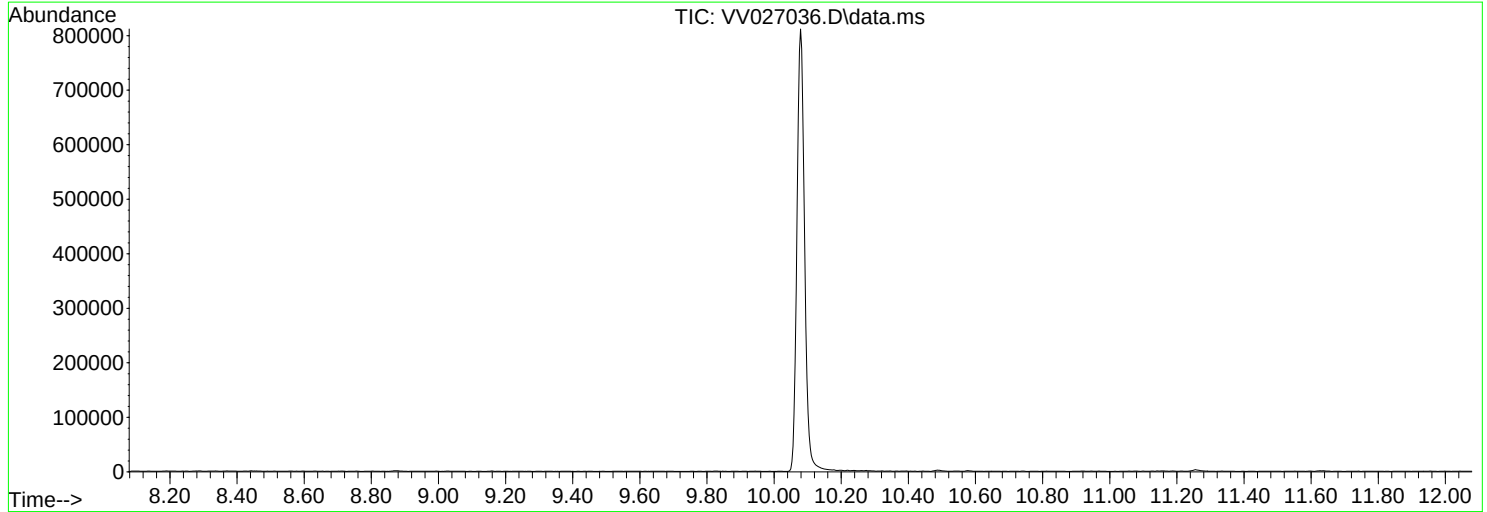

AutoFind: Scans 2810, 2811, 2812; Background Corrected with Scan 2798

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.3	25725	PASS
75	95	30	80	44.6	75013	PASS
95	95	100	100	100.0	168149	PASS
96	95	5	9	6.4	10703	PASS
173	174	0.00	2	1.2	1662	PASS
174	95	50	120	80.3	135064	PASS
175	174	5	9	7.1	9542	PASS
176	174	95	105	96.2	129979	PASS
177	176	5	10	6.6	8546	PASS

m/z	Abundance
40.00	320.0
44.00	701.0

Instrument :
MSVOA_V
ClientSampleId :
BFB301

m/z	Abundance
36.00	1005.0
37.00	5457.0
38.00	5415.0
39.00	2502.0
39.90	385.0
40.20	362.0
42.80	120.0
44.00	1291.0
45.00	1024.0
46.00	287.0
47.10	1713.0
47.90	870.0
49.00	5382.0
50.00	25312.0
51.00	7878.0
52.00	438.0
53.00	200.0
53.90	137.0
54.90	353.0
56.00	1885.0
57.00	3545.0
57.80	193.0
60.00	1277.0
61.00	6979.0
62.00	7498.0
63.00	6276.0
64.00	1410.0
65.00	1580.0
66.00	155.0
66.80	370.0
68.00	13688.0
69.00	14824.0
70.00	1211.0
71.90	894.0
73.00	6624.0
74.00	25040.0
75.00	74616.0
76.10	6979.0
76.90	1166.0
77.90	716.0
78.90	7002.0
80.00	1850.0
80.90	6676.0
81.90	1488.0
85.90	259.0
87.00	7322.0
88.00	7019.0
90.80	596.0
91.90	4456.0
93.00	6939.0
94.00	18112.0
95.00	165440.0
96.10	10684.0
97.00	306.0
103.90	629.0
104.90	144.0
106.00	636.0
107.00	172.0
107.90	152.0
110.00	102.0
110.90	206.0
112.70	143.0
114.80	182.0
115.90	739.0
116.90	1381.0
118.00	618.0
118.90	1320.0
123.80	118.0
128.00	695.0
129.00	306.0
129.90	501.0
130.80	276.0
134.90	333.0
136.90	339.0
140.90	1432.0
142.00	237.0
142.90	2959.0
145.00	1452.0
146.00	366.0
147.80	321.0
148.90	191.0
149.80	151.0
152.80	118.0
155.00	481.0
157.00	256.0
158.80	188.0
160.90	161.0
170.90	620.0
171.90	1637.0
173.00	1630.0
174.00	131016.0
175.00	9305.0

Instrument :
MSVOA_V
ClientSampleId :
BFB301

176.00	124952.0
177.00	8627.0
178.10	147.0

Instrument :
MSVOA_V
ClientSampleId :
BFB301

m/z	Abundance
35.90	920.0
37.00	5591.0
38.00	5615.0
39.00	2602.0
39.80	392.0
40.20	335.0
42.80	125.0
44.00	1214.0
45.00	1086.0
46.00	367.0
47.10	1828.0
47.90	897.0
49.00	5612.0
50.00	26576.0
51.00	8303.0
52.00	455.0
53.00	201.0
53.90	153.0
54.90	310.0
56.00	1945.0
57.00	3731.0
57.90	218.0
60.00	1339.0
61.00	7315.0
62.00	7687.0
63.00	6579.0
64.00	1437.0
65.00	1684.0
66.00	179.0
66.80	336.0
68.00	14521.0
69.00	15349.0
70.10	1102.0
71.90	860.0
73.00	7138.0
74.00	26328.0
75.00	77472.0
76.10	7353.0
76.90	1191.0
77.90	725.0
78.90	7112.0
79.90	1868.0
80.90	7003.0
81.90	1666.0
85.90	283.0
87.00	7826.0
88.00	6987.0
90.80	534.0
92.00	4651.0
93.00	7325.0
94.00	19536.0
95.00	173952.0
96.10	11031.0
96.90	307.0
103.90	712.0
104.90	144.0
105.90	585.0
107.00	178.0
107.90	156.0
109.90	111.0
111.00	186.0
112.70	144.0
114.90	230.0
115.90	738.0
116.90	1419.0
118.00	732.0
118.90	1360.0
123.90	146.0
128.00	698.0
129.00	310.0
129.90	559.0
130.80	313.0
134.90	367.0
136.90	362.0
140.90	1445.0
142.00	198.0
142.90	3085.0
145.00	1568.0
146.00	344.0
147.90	408.0
148.90	171.0
149.80	178.0
152.10	109.0
152.80	111.0
155.00	502.0
157.00	324.0
158.80	221.0
160.80	207.0
170.80	656.0
171.90	1802.0
173.00	1667.0
174.00	139264.0

Instrument :
MSVOA_V
ClientSampleId :
BFB301

175.00	9784.0
176.00	134400.0
177.00	8888.0
178.10	156.0

Instrument :
MSVOA_V
ClientSampleId :
BFB301

m/z	Abundance
35.90	898.0
37.00	5219.0
38.00	5094.0
39.00	2465.0
39.80	431.0
42.80	105.0
44.00	1117.0
45.00	1057.0
46.00	359.0
47.10	1710.0
47.90	807.0
49.00	5263.0
50.00	25288.0
51.00	7883.0
52.00	443.0
52.80	171.0
53.10	180.0
53.80	188.0
54.90	305.0
56.00	1745.0
57.00	3527.0
57.90	186.0
60.00	1364.0
61.00	7020.0
62.00	7025.0
63.00	6457.0
64.00	1323.0
65.00	1630.0
66.00	165.0
67.00	304.0
68.00	13956.0
69.00	14275.0
70.10	1013.0
71.90	790.0
73.00	6810.0
74.00	24936.0
75.00	72952.0
76.10	6689.0
77.00	945.0
77.90	610.0
78.90	6474.0
79.90	1698.0
80.90	6867.0
81.90	1662.0
82.80	113.0
86.00	251.0
87.00	7419.0
88.00	6648.0
91.10	494.0
92.00	4553.0
93.00	7064.0
94.00	19144.0
95.00	165056.0
96.00	10393.0
97.00	307.0
103.90	673.0
104.90	134.0
105.90	527.0
107.00	218.0
107.70	160.0
108.00	145.0
109.80	105.0
110.70	159.0
111.00	159.0
112.80	165.0
115.00	229.0
115.90	660.0
116.90	1458.0
118.00	671.0
118.80	1185.0
123.90	136.0
127.90	600.0
128.90	320.0
130.00	536.0
130.80	283.0
135.00	313.0
136.90	295.0
139.70	130.0
140.80	1370.0
142.90	2935.0
145.00	1458.0
146.00	261.0
146.80	107.0
147.90	476.0
148.90	155.0
149.80	176.0
152.10	115.0
153.80	105.0
155.00	457.0
157.00	344.0
158.80	238.0
160.80	218.0

Instrument :
MSVOA_V
ClientSampleId :
BFB301

170.80	622.0
171.90	1784.0
173.00	1689.0
174.00	134912.0
175.00	9536.0
176.00	130584.0
177.00	8124.0
177.90	170.0

Instrument :
MSVOA_V
ClientSampleId :
BFB301