

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW072823\
 Data File : VW031779.D
 Acq On : 28 Jul 2023 11:17
 Operator : SY/MD
 Sample : 03754-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Jul 28 22:40:02 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jul 28 22:38:33 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.539	114	297627	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	340415	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.191	152	151900	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	122300	40.308	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	80.620%		
7) Chloroethane-d5	1.529	69	125345	45.080	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	90.160%		
11) 1,1-Dichloroethene-d2	2.060	65	57300	40.799	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	81.600%		
21) 2-Butanone-d5	3.790	46	248334	118.283	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	118.280%		
24) Chloroform-d	4.253	84	320571	51.390	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	102.780%		
26) 1,2-Dichloroethane-d4	4.947	65	214084	55.158	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	110.320%		
32) Benzene-d6	4.966	84	494756	45.897	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	91.800%		
36) 1,2-Dichloropropane-d6	5.995	67	191666	47.334	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	94.660%		
41) Toluene-d8	7.249	98	368232	40.755	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	81.500%		
43) trans-1,3-Dichloroprop...	7.558	79	77729	44.660	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	89.320%		
47) 2-Hexanone-d5	8.031	63	144180	94.953	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	94.950%		
56) 1,1,2,2-Tetrachloroeth...	10.159	84	288689	51.745	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	103.480%		
66) 1,2-Dichlorobenzene-d4	11.567	152	172625	56.129	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	112.260%		
Target Compounds					Qvalue	
37) 1,2-Dichloropropane	5.831	63	2793	0.785	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072823\
Data File : VV031779.D
Acq On : 28 Jul 2023 11:17
Operator : SY/MD
Sample : 03754-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Time: Jul 28 22:40:02 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jul 28 22:38:33 2023
Response via : Initial Calibration

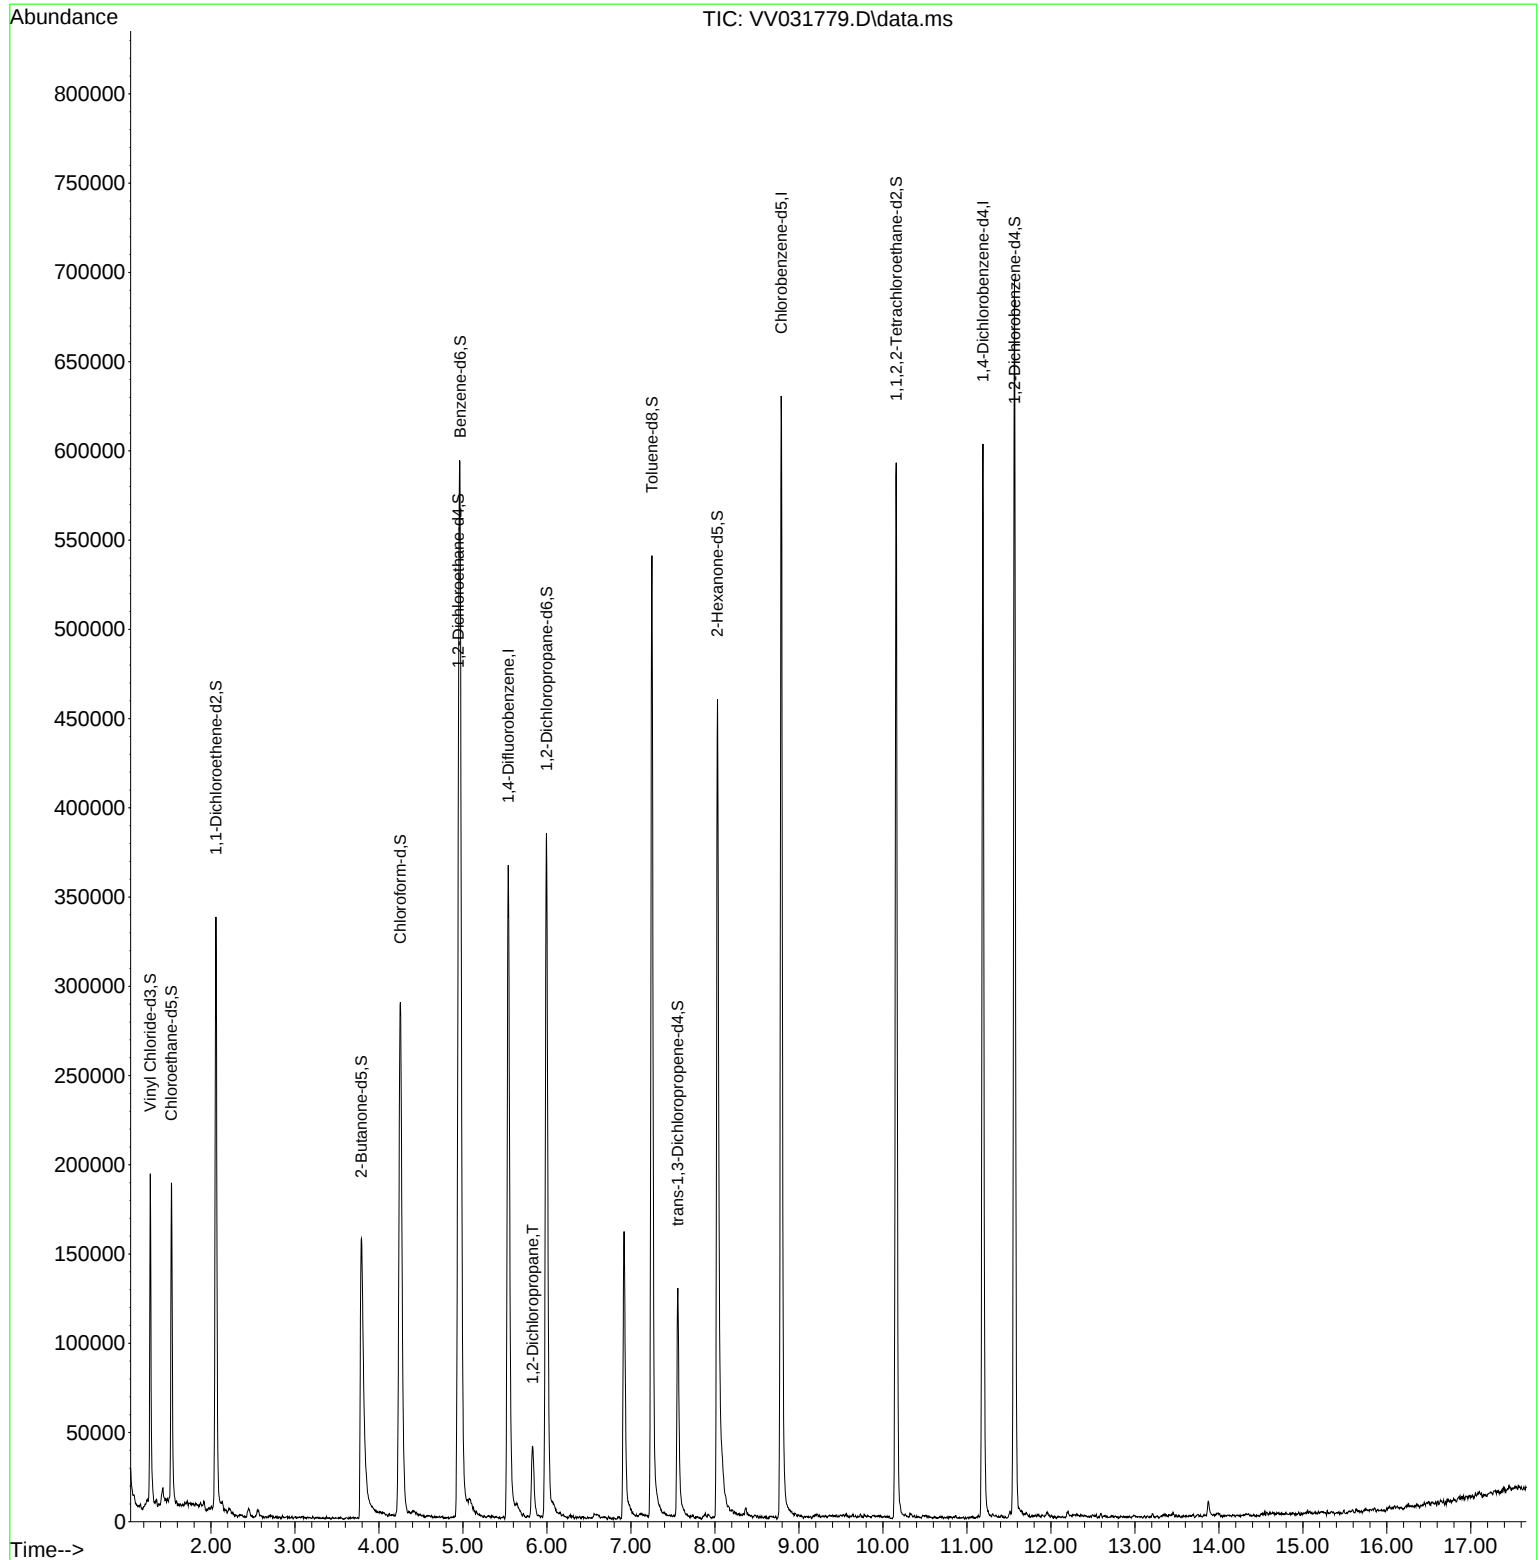

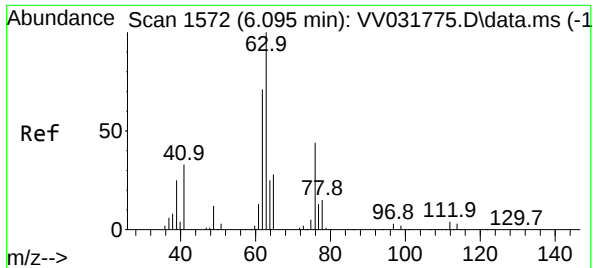

#37
 1,2-Dichloropropane
 Concen: 0.785 ug/L
 RT: 5.831 min Scan# 14
 Delta R.T. -0.264 min
 Lab File: VV031779.D
 Acq: 28 Jul 2023 11:17

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Tgt Ion: 63 Resp: 2793
 Ion Ratio Lower Upper
 63 100
 112 5.1 3.7 5.5

