

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072823\
 Data File : VV031776.D
 Acq On : 28 Jul 2023 09:36
 Operator : SY/MD
 Sample : VV0728WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK375

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
 Title : VOC Analysis

Signal : TIC: VV031776.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	87	rVB	223126	238636	13.38%	1.803%
2	1.529	146	152	170	rVB	200875	250485	14.05%	1.893%
3	2.057	308	316	331	rVB	405290	587968	32.97%	4.443%
4	2.323	397	399	403	rBV4	1479	1103	0.06%	0.008%
5	2.520	457	460	463	rBV5	1287	972	0.05%	0.007%
6	2.629	492	494	499	rVB5	1195	871	0.05%	0.007%
7	2.812	548	551	552	rBV3	752	416	0.02%	0.003%
8	2.860	563	566	567	rBV3	1093	544	0.03%	0.004%
9	2.899	575	578	582	rBV4	979	703	0.04%	0.005%
10	2.944	590	592	593	rBV2	454	126	0.01%	0.001%
11	3.021	612	616	618	rBV3	562	487	0.03%	0.004%
12	3.056	625	627	630	rBV4	829	456	0.03%	0.003%
13	3.169	659	662	663	rBV2	868	353	0.02%	0.003%
14	3.188	666	668	670	rBV3	912	386	0.02%	0.003%
15	3.262	690	691	695	rVB3	984	537	0.03%	0.004%
16	3.291	695	700	706	rBV6	1193	1415	0.08%	0.011%
17	3.323	706	710	713	rVV4	965	902	0.05%	0.007%
18	3.355	717	720	722	rBV4	570	358	0.02%	0.003%
19	3.381	726	728	730	rBV3	752	334	0.02%	0.003%
20	3.394	730	732	736	rVB4	754	388	0.02%	0.003%
21	3.413	736	738	741	rBV3	1154	857	0.05%	0.006%
22	3.439	744	746	748	rBV3	544	324	0.02%	0.002%
23	3.484	756	760	762	rBV5	800	602	0.03%	0.005%
24	3.513	765	769	770	rBV2	477	360	0.02%	0.003%
25	3.671	813	818	819	rBV4	1037	606	0.03%	0.005%
26	3.712	827	831	833	rBV4	875	698	0.04%	0.005%
27	3.786	837	854	898	rBV	163051	495261	27.77%	3.742%
28	4.253	984	999	1026	rBV	314676	813690	45.63%	6.148%
29	4.696	1133	1137	1139	rBV4	1370	889	0.05%	0.007%
30	4.857	1185	1187	1189	rBV3	932	460	0.03%	0.003%
31	4.957	1201	1218	1243	rBV3	661834	1783223	100.00%	13.474%
32	5.285	1319	1320	1321	rBV	1056	333	0.02%	0.003%
33	5.539	1386	1399	1422	rBV	418842	884623	49.61%	6.684%
34	5.825	1480	1488	1501	rVB4	42326	79918	4.48%	0.604%
35	5.992	1528	1540	1568	rBV	428456	884543	49.60%	6.683%
36	6.381	1656	1661	1668	rBV9	1822	2063	0.12%	0.016%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072823\
 Data File : VV031776.D
 Acq On : 28 Jul 2023 09:36
 Operator : SY/MD
 Sample : VV0728WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK375

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
 Title : VOC Analysis

37	6.410	1668	1670	1671	rBV2	952	483	0.03%	0.004%
38	6.523	1702	1705	1707	rBV2	432	254	0.01%	0.002%
39	6.561	1707	1717	1721	rBV10	4026	6392	0.36%	0.048%
40	6.715	1763	1765	1772	rBV5	1040	789	0.04%	0.006%
41	6.809	1791	1794	1797	rBV4	1441	865	0.05%	0.007%
42	6.851	1805	1807	1810	rBV4	1160	798	0.04%	0.006%
43	6.915	1817	1827	1853	rBV2	181568	354193	19.86%	2.676%
44	7.246	1919	1930	1958	rBV	620208	1127436	63.22%	8.519%
45	7.555	2017	2026	2053	rBV	142239	260348	14.60%	1.967%
46	7.767	2090	2092	2095	rBV4	1954	1209	0.07%	0.009%
47	7.857	2118	2120	2127	rBV8	1451	1748	0.10%	0.013%
48	7.960	2150	2152	2154	rBV2	901	383	0.02%	0.003%
49	8.031	2164	2174	2215	rBV	484451	987667	55.39%	7.463%
50	8.677	2372	2375	2378	rBV5	1407	1016	0.06%	0.008%
51	8.789	2397	2410	2438	rBV	693161	1170062	65.62%	8.841%
52	9.217	2540	2543	2548	rBV7	1629	1187	0.07%	0.009%
53	9.272	2557	2560	2563	rBV3	1152	933	0.05%	0.007%
54	9.358	2584	2587	2589	rBV3	910	531	0.03%	0.004%
55	9.403	2600	2601	2603	rBV3	870	277	0.02%	0.002%
56	9.413	2603	2604	2605	rBV	970	371	0.02%	0.003%
57	9.448	2613	2615	2616	rBV2	871	276	0.02%	0.002%
58	9.564	2649	2651	2652	rBV2	1249	559	0.03%	0.004%
59	9.677	2683	2686	2687	rBV3	1000	347	0.02%	0.003%
60	9.809	2723	2727	2732	rBV5	1503	1815	0.10%	0.014%
61	10.005	2784	2788	2789	rBV4	1382	860	0.05%	0.006%
62	10.156	2825	2835	2863	rVB	612733	978088	54.85%	7.390%
63	10.317	2883	2885	2889	rBV5	1207	894	0.05%	0.007%
64	10.397	2906	2910	2912	rBV7	991	846	0.05%	0.006%
65	10.542	2953	2955	2957	rBV2	1342	682	0.04%	0.005%
66	10.612	2974	2977	2978	rBV2	1182	553	0.03%	0.004%
67	10.989	3092	3094	3099	rBV4	1436	1030	0.06%	0.008%
68	11.021	3103	3104	3106	rBV2	1118	509	0.03%	0.004%
69	11.053	3110	3114	3115	rBV4	843	556	0.03%	0.004%
70	11.191	3146	3157	3176	rBV	680038	1055550	59.19%	7.976%
71	11.410	3223	3225	3226	rBV2	858	372	0.02%	0.003%
72	11.458	3237	3240	3243	rBV4	1406	1047	0.06%	0.008%
73	11.477	3244	3246	3249	rVV2	1079	487	0.03%	0.004%
74	11.564	3262	3273	3291	rBV	770337	1223651	68.62%	9.246%
75	11.776	3336	3339	3340	rBV3	823	356	0.02%	0.003%
76	11.831	3354	3356	3358	rBV2	811	450	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072823\
 Data File : VV031776.D
 Acq On : 28 Jul 2023 09:36
 Operator : SY/MD
 Sample : VV0728WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK375

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M

Title : VOC Analysis

77	11.934	3385	3388	3389	rBV2	882	400	0.02%	0.003%
78	12.037	3417	3420	3423	rBV3	1365	1125	0.06%	0.009%
79	12.053	3423	3425	3427	rBV3	1051	483	0.03%	0.004%
80	12.108	3439	3442	3445	rBV3	1257	801	0.04%	0.006%
81	12.230	3479	3480	3482	rBV2	855	386	0.02%	0.003%
82	12.294	3496	3500	3502	rBV3	1257	888	0.05%	0.007%
83	12.336	3510	3513	3516	rBV3	719	549	0.03%	0.004%
84	12.413	3532	3537	3539	rBV4	1202	1006	0.06%	0.008%
85	12.593	3582	3593	3594	rBV9	5724	7339	0.41%	0.055%




Sum of corrected areas: 13234737

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072823\
Data File : VV031776.D
Acq On : 28 Jul 2023 09:36
Operator : SY/MD
Sample : VV0728WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK375

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

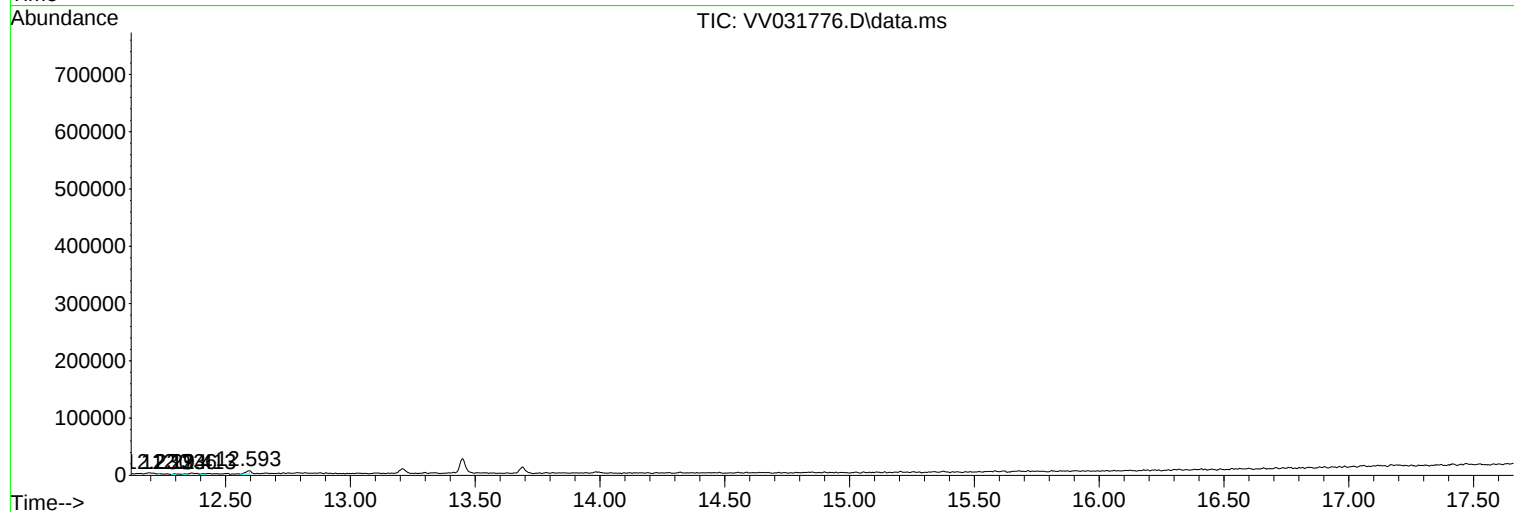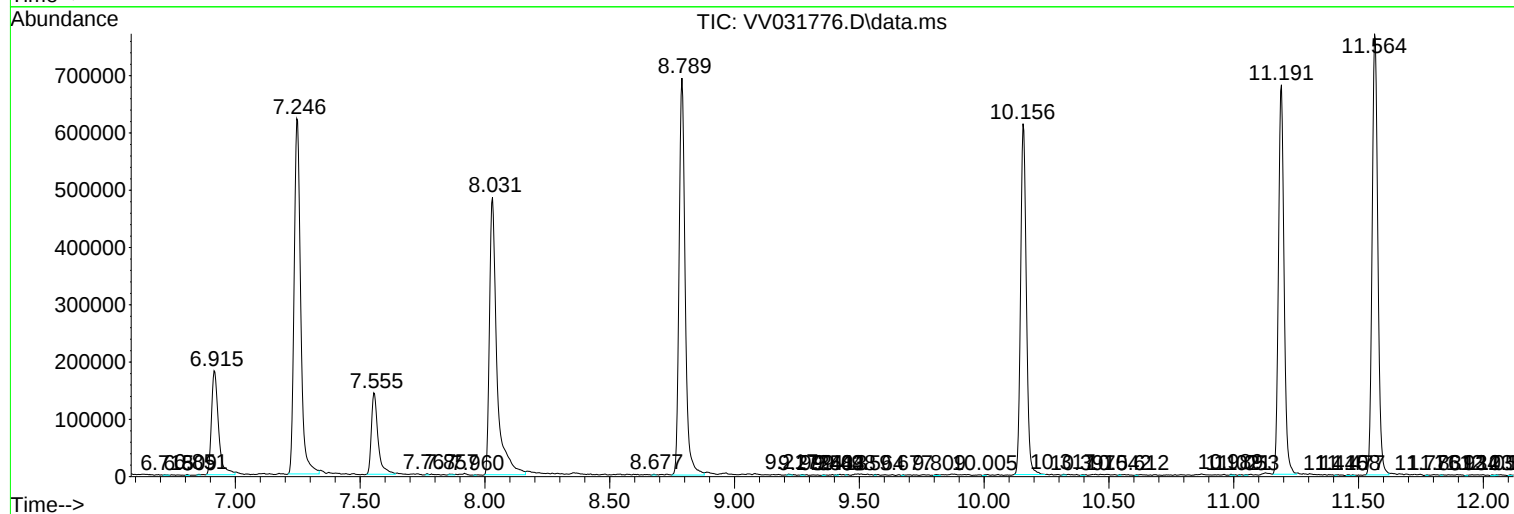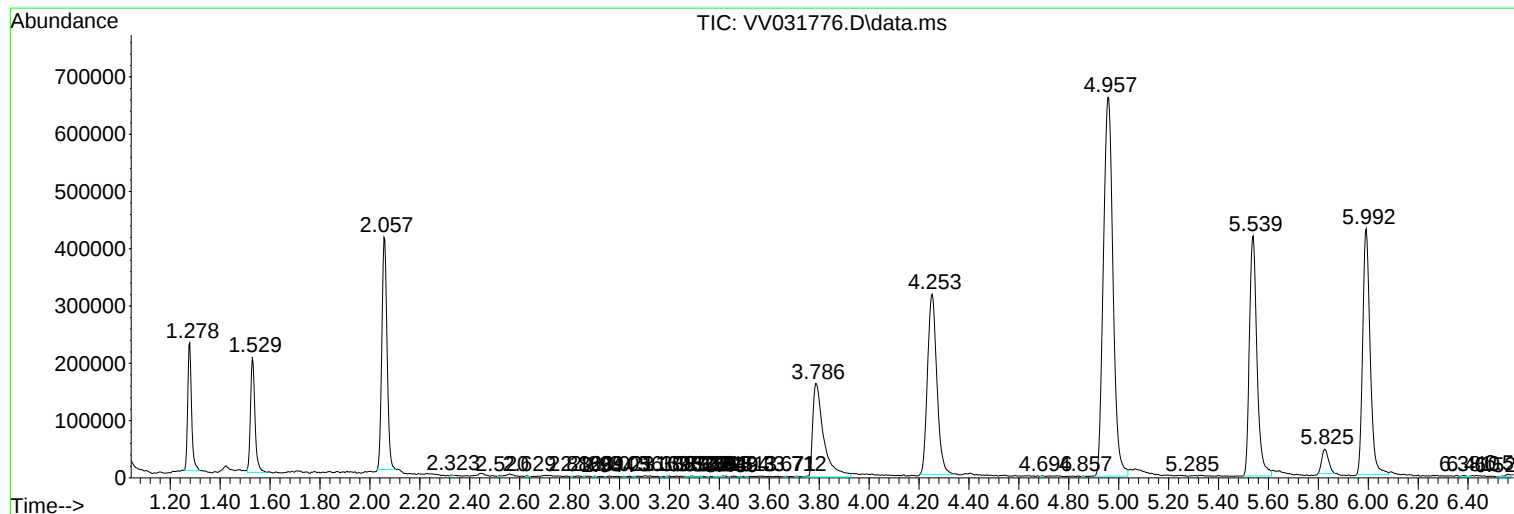

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072823\
Data File : VV031776.D
Acq On : 28 Jul 2023 09:36
Operator : SY/MD
Sample : VV0728WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK375

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072823\
Data File : VV031776.D
Acq On : 28 Jul 2023 09:36
Operator : SY/MD
Sample : VV0728WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK375

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
