

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072823\
 Data File : VV031779.D
 Acq On : 28 Jul 2023 11:17
 Operator : SY/MD
 Sample : 03754-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
 Title : VOC Analysis

Signal : TIC: VV031779.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	88	rVB	184201	198884	12.39%	1.676%
2	1.529	146	152	167	rVB	179242	220819	13.75%	1.861%
3	2.060	308	317	334	rVB	328298	474271	29.54%	3.998%
4	2.680	508	510	511	rBV2	753	220	0.01%	0.002%
5	2.741	527	529	533	rBV3	1235	657	0.04%	0.006%
6	2.806	547	549	550	rBV	734	295	0.02%	0.002%
7	2.838	557	559	560	rBV2	800	325	0.02%	0.003%
8	2.851	561	563	566	rVV5	1310	714	0.04%	0.006%
9	2.989	603	606	607	rBV2	1101	507	0.03%	0.004%
10	3.146	652	655	658	rBV4	966	748	0.05%	0.006%
11	3.211	673	675	682	rVB5	1527	1326	0.08%	0.011%
12	3.243	682	685	687	rBV4	936	622	0.04%	0.005%
13	3.298	700	702	705	rBV3	517	194	0.01%	0.002%
14	3.333	710	713	715	rBV3	782	448	0.03%	0.004%
15	3.359	719	721	724	rBV2	628	338	0.02%	0.003%
16	3.375	724	726	729	rBV3	1299	665	0.04%	0.006%
17	3.446	744	748	749	rBV2	1022	638	0.04%	0.005%
18	3.545	777	779	782	rBV4	807	336	0.02%	0.003%
19	3.574	787	788	790	rVB	198	41	0.00%	0.000%
20	3.590	790	793	795	rBV4	407	297	0.02%	0.003%
21	3.645	807	810	813	rBV2	1158	595	0.04%	0.005%
22	3.661	813	815	817	rBV2	1019	487	0.03%	0.004%
23	3.719	829	833	836	rBV4	781	708	0.04%	0.006%
24	3.793	846	856	894	rBV	156718	468270	29.16%	3.947%
25	4.256	986	1000	1028	rVB2	286114	737307	45.92%	6.215%
26	4.806	1168	1171	1174	rBV5	662	440	0.03%	0.004%
27	4.841	1180	1182	1184	rBV3	588	367	0.02%	0.003%
28	4.960	1200	1219	1245	rBV2	592441	1605718	100.00%	13.534%
29	5.436	1365	1367	1371	rVB5	1150	706	0.04%	0.006%
30	5.465	1371	1376	1377	rBV2	805	742	0.05%	0.006%
31	5.481	1379	1381	1386	rVB4	1696	1353	0.08%	0.011%
32	5.539	1386	1399	1425	rBV	366380	772824	48.13%	6.514%
33	5.828	1480	1489	1507	rVB3	38872	83174	5.18%	0.701%
34	5.995	1526	1541	1563	rBV	383431	800994	49.88%	6.751%
35	6.246	1618	1619	1623	rBV4	779	438	0.03%	0.004%
36	6.269	1623	1626	1627	rBV3	1360	846	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072823\
 Data File : VV031779.D
 Acq On : 28 Jul 2023 11:17
 Operator : SY/MD
 Sample : 03754-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
 Title : VOC Analysis

37	6.317	1639	1641	1643	rVB2	1474	516	0.03%	0.004%
38	6.416	1669	1672	1673	rBV3	1241	753	0.05%	0.006%
39	6.735	1766	1771	1774	rBV6	1937	1854	0.12%	0.016%
40	6.770	1781	1782	1783	rBV	375	75	0.00%	0.001%
41	6.780	1783	1785	1788	rVB2	875	500	0.03%	0.004%
42	6.796	1788	1790	1795	rBV4	1016	891	0.06%	0.008%
43	6.844	1800	1805	1808	rBV5	1233	1130	0.07%	0.010%
44	6.876	1814	1815	1817	rBV	679	324	0.02%	0.003%
45	6.918	1817	1828	1853	rBV	160914	315396	19.64%	2.658%
46	7.249	1919	1931	1959	rBV	538457	989204	61.61%	8.338%
47	7.558	2018	2027	2050	rBV	127233	227580	14.17%	1.918%
48	7.709	2072	2074	2078	rBV4	1636	1183	0.07%	0.010%
49	7.834	2111	2113	2115	rVB	707	320	0.02%	0.003%
50	7.863	2115	2122	2123	rBV7	1681	1724	0.11%	0.015%
51	8.031	2164	2174	2211	rBV	457958	925975	57.67%	7.805%
52	8.368	2274	2279	2284	rBV9	3933	4956	0.31%	0.042%
53	8.510	2320	2323	2327	rVB6	1638	1304	0.08%	0.011%
54	8.558	2335	2338	2341	rBV3	1354	880	0.05%	0.007%
55	8.587	2345	2347	2349	rBV2	825	387	0.02%	0.003%
56	8.635	2359	2362	2364	rVB4	1079	505	0.03%	0.004%
57	8.654	2364	2368	2369	rBV3	1482	961	0.06%	0.008%
58	8.789	2400	2410	2435	rBV	626656	1034091	64.40%	8.716%
59	9.609	2663	2665	2667	rBV3	1147	652	0.04%	0.005%
60	10.159	2824	2836	2858	rBV	590995	950810	59.21%	8.014%
61	10.474	2928	2934	2938	rBV8	1747	2304	0.14%	0.019%
62	10.735	3012	3015	3018	rBV4	706	491	0.03%	0.004%
63	10.776	3026	3028	3030	rVB	1038	380	0.02%	0.003%
64	10.792	3030	3033	3034	rBV3	783	513	0.03%	0.004%
65	10.908	3065	3069	3071	rBV3	800	494	0.03%	0.004%
66	10.982	3090	3092	3095	rVB2	1055	511	0.03%	0.004%
67	11.005	3095	3099	3102	rBV4	1000	915	0.06%	0.008%
68	11.082	3121	3123	3126	rVB2	960	465	0.03%	0.004%
69	11.191	3146	3157	3175	rBV	600993	937044	58.36%	7.898%
70	11.567	3263	3274	3289	rBV	690729	1074535	66.92%	9.057%
71	12.191	3465	3468	3469	rBV2	2456	1291	0.08%	0.011%
72	12.815	3660	3662	3665	rBV5	863	660	0.04%	0.006%
73	13.101	3749	3751	3752	rBV	742	314	0.02%	0.003%
74	13.153	3760	3767	3771	rBV7	1252	1780	0.11%	0.015%
75	13.207	3781	3784	3790	rBV6	1929	2252	0.14%	0.019%
76	14.050	4044	4046	4050	rBV4	1063	749	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072823\
Data File : VV031779.D
Acq On : 28 Jul 2023 11:17
Operator : SY/MD
Sample : 03754-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
Title : VOC Analysis




Sum of corrected areas: 11863983

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072823\
Data File : VV031779.D
Acq On : 28 Jul 2023 11:17
Operator : SY/MD
Sample : 03754-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

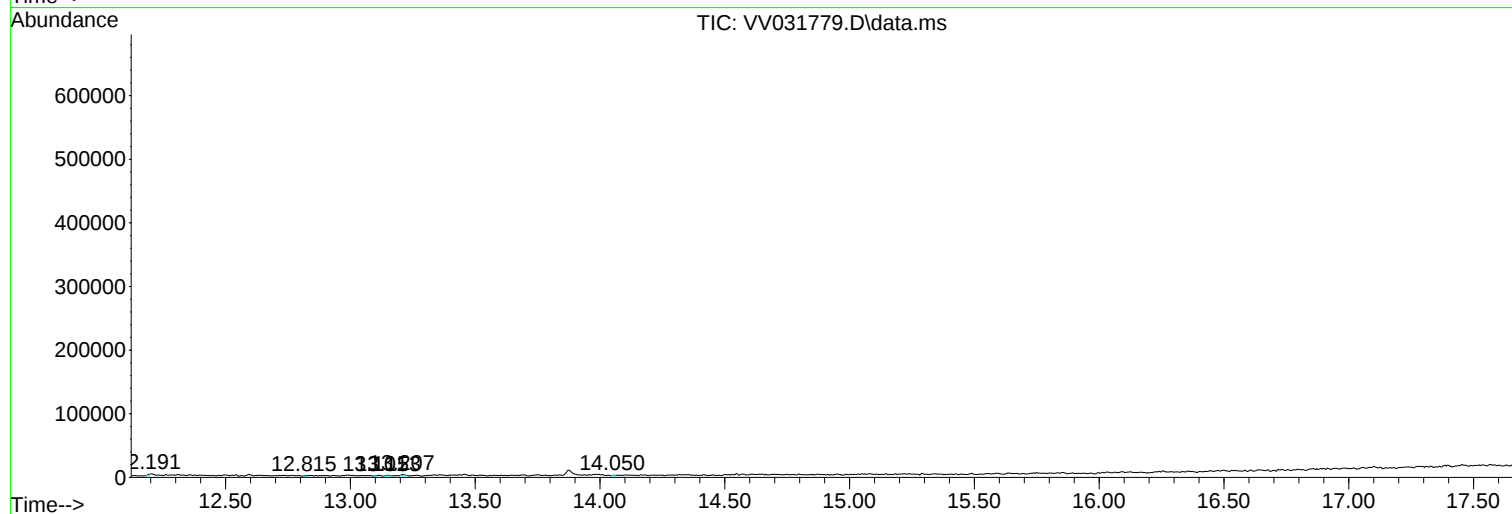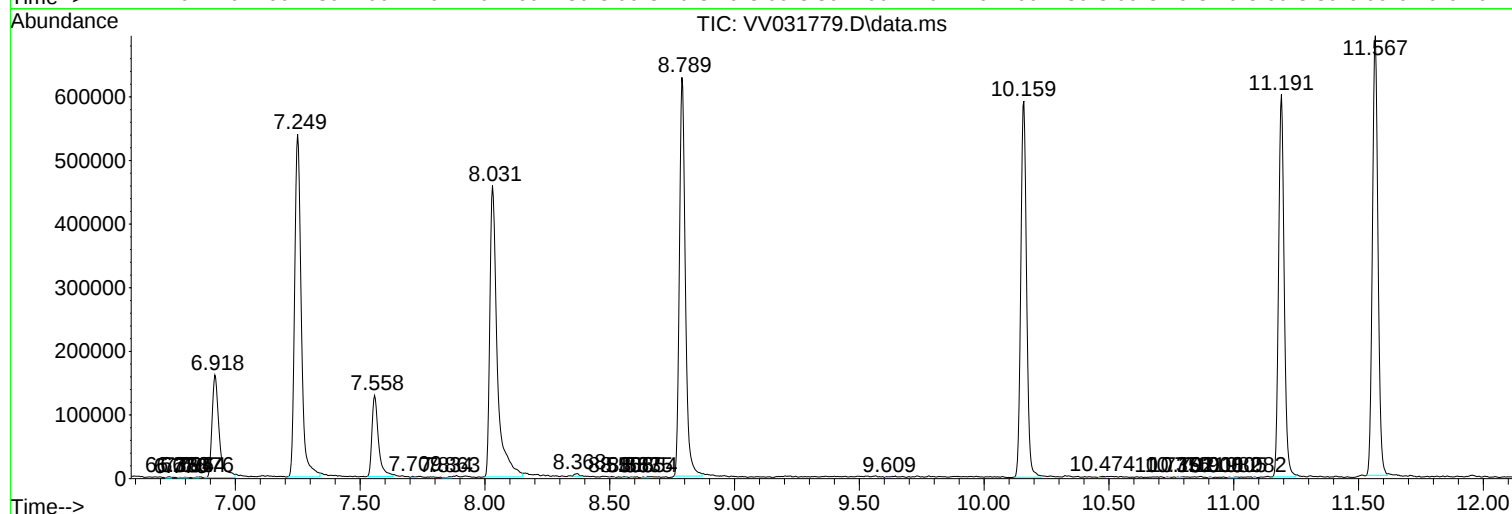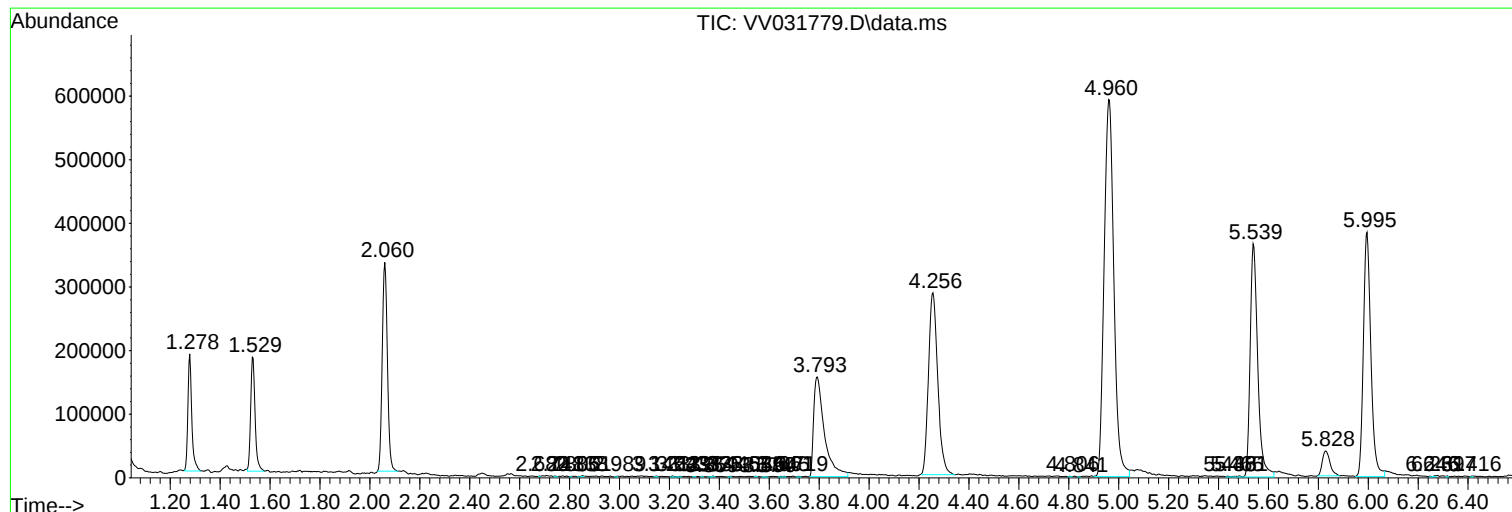

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072823\
Data File : VV031779.D
Acq On : 28 Jul 2023 11:17
Operator : SY/MD
Sample : 03754-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072823\
Data File : VV031779.D
Acq On : 28 Jul 2023 11:17
Operator : SY/MD
Sample : 03754-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------