


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072823\
Data File : VV031774.D
Acq On : 28 Jul 2023 08:31
Operator : SY/MD
Sample : BFB201
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB201

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072523WMA.M
Title : VOC Analysis
Last Update : Fri Jul 28 22:38:33 2023

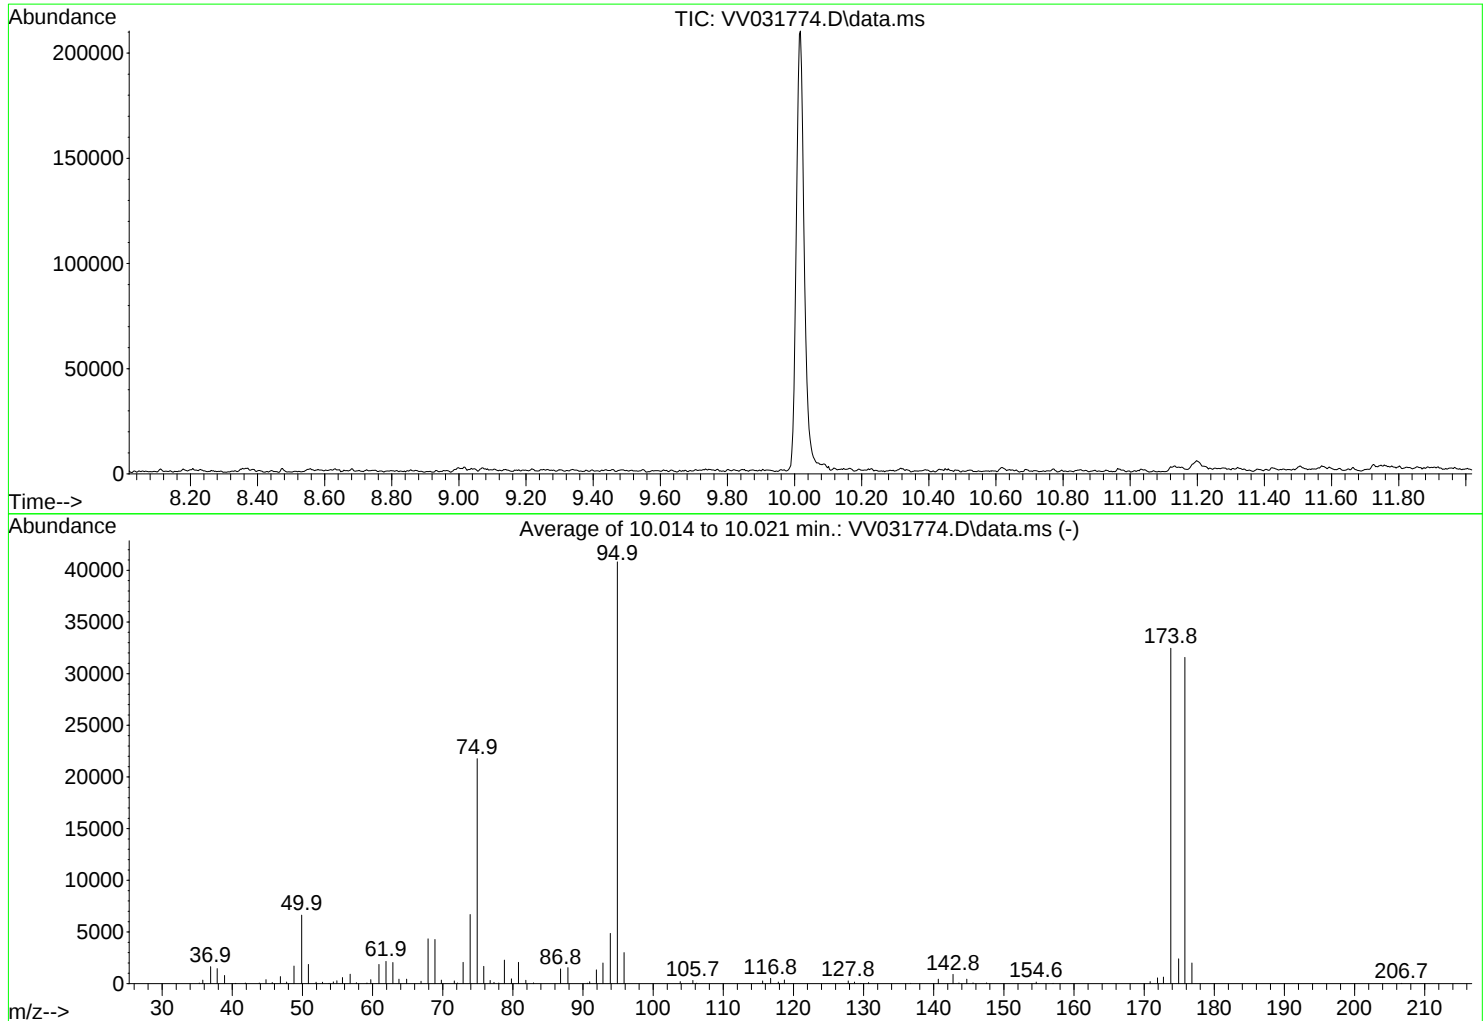

AutoFind: Scans 2791, 2792, 2793; Background Corrected with Scan 2780

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.2	6627	PASS
75	95	30	80	53.3	21765	PASS
95	95	100	100	100.0	40819	PASS
96	95	5	9	7.3	3000	PASS
173	174	0.00	2	1.9	628	PASS
174	95	50	120	79.5	32451	PASS
175	174	5	9	7.4	2401	PASS
176	174	95	105	97.3	31573	PASS
177	176	5	10	6.4	2005	PASS

m/z	Abundance
36.60	140.0
39.80	424.0
41.30	143.0
42.80	127.0
43.90	659.0
47.90	129.0

Instrument :
MSVOA_V
ClientSampleId :
BFB201

m/z	Abundance
35.80	342.0
36.90	1613.0
37.90	1586.0
38.90	690.0
39.90	295.0
40.50	107.0
41.90	105.0
43.80	630.0
44.80	484.0
45.70	124.0
46.90	716.0
47.70	345.0
48.80	1752.0
49.90	6935.0
50.90	2034.0
52.00	130.0
52.90	160.0
53.80	116.0
54.90	291.0
55.70	567.0
56.80	993.0
59.70	422.0
60.90	1973.0
61.90	2225.0
62.90	2272.0
63.80	428.0
64.90	354.0
66.90	135.0
67.90	4369.0
68.90	4655.0
69.80	429.0
71.60	208.0
72.10	185.0
72.90	2083.0
73.90	6911.0
74.90	22360.0
75.90	1927.0
76.80	366.0
77.30	117.0
78.80	2278.0
79.80	457.0
80.80	1950.0
81.90	334.0
82.90	124.0
86.80	1367.0
87.80	1599.0
90.90	212.0
91.90	1484.0
92.80	2050.0
93.90	5142.0
94.90	41744.0
95.90	3218.0
103.80	250.0
105.70	293.0
106.20	151.0
115.60	304.0
116.80	452.0
117.80	178.0
118.70	382.0
127.80	230.0
128.70	116.0
130.70	108.0
140.70	397.0
142.70	968.0
143.60	133.0
144.70	493.0
145.70	119.0
147.60	120.0
154.70	199.0
170.80	204.0
171.90	602.0
172.70	585.0
173.80	32672.0
174.90	2613.0
175.80	31832.0
176.80	2069.0
206.70	118.0

Instrument :
MSVOA_V
ClientSampleId :
BFB201

m/z	Abundance
35.80	350.0
36.90	1726.0
37.80	1453.0
38.90	822.0
39.80	314.0
41.80	106.0
43.80	743.0
44.80	389.0
45.70	106.0
46.90	708.0
47.70	290.0
48.80	1733.0
49.90	6781.0
50.90	1869.0
51.90	138.0
52.80	135.0
54.40	232.0
54.90	282.0
55.70	609.0
56.80	936.0
57.70	126.0
59.70	398.0
60.90	1943.0
61.90	2174.0
62.90	2032.0
63.80	445.0
64.80	463.0
66.90	250.0
67.90	4414.0
68.90	4454.0
69.80	330.0
71.60	270.0
72.90	2188.0
73.90	6923.0
74.90	22592.0
75.90	1698.0
76.80	334.0
77.30	142.0
78.00	169.0
78.80	2345.0
79.80	488.0
80.80	2138.0
81.80	315.0
83.00	123.0
86.80	1436.0
87.90	1588.0
91.00	195.0
91.90	1431.0
92.80	2019.0
93.90	5021.0
94.90	42016.0
95.90	3116.0
103.90	193.0
105.70	329.0
115.60	282.0
116.70	535.0
117.80	163.0
118.70	357.0
127.80	289.0
128.70	183.0
130.70	117.0
140.60	467.0
142.80	903.0
143.60	120.0
144.70	476.0
145.50	103.0
147.50	105.0
154.60	146.0
170.80	213.0
171.90	585.0
172.80	648.0
173.80	33744.0
174.90	2500.0
175.80	32688.0
176.80	2064.0

Instrument :
MSVOA_V
ClientSampleId :
BFB201

m/z	Abundance
35.30	168.0
35.80	320.0
36.90	1579.0
37.80	1344.0
38.90	842.0
39.80	410.0
42.80	129.0
43.90	814.0
44.70	276.0
45.70	119.0
46.80	614.0
47.60	209.0
48.80	1620.0
49.90	6166.0
50.80	1671.0
51.90	157.0
52.80	120.0
54.40	262.0
54.90	277.0
55.70	592.0
56.80	812.0
57.70	163.0
59.20	173.0
59.80	362.0
60.90	1640.0
61.90	2069.0
62.90	1821.0
63.70	421.0
64.80	504.0
66.90	337.0
67.90	4211.0
68.90	3726.0
69.80	289.0
71.70	302.0
72.90	1903.0
73.90	6225.0
74.90	20344.0
75.80	1387.0
76.70	248.0
77.30	131.0
78.80	2226.0
79.80	473.0
80.80	2106.0
81.80	339.0
86.80	1475.0
87.80	1452.0
90.60	146.0
91.00	143.0
91.90	1086.0
92.90	1939.0
93.90	4441.0
94.90	38696.0
95.80	2666.0
103.90	149.0
105.60	292.0
115.60	198.0
116.70	544.0
117.90	135.0
118.70	312.0
127.80	265.0
128.70	187.0
129.60	116.0
130.70	103.0
136.70	106.0
140.60	426.0
142.80	806.0
144.70	348.0
154.50	108.0
157.00	109.0
170.90	203.0
171.90	495.0
172.80	651.0
173.80	30936.0
174.90	2089.0
175.80	30200.0
176.80	1882.0

Instrument :
MSVOA_V
ClientSampleId :
BFB201