
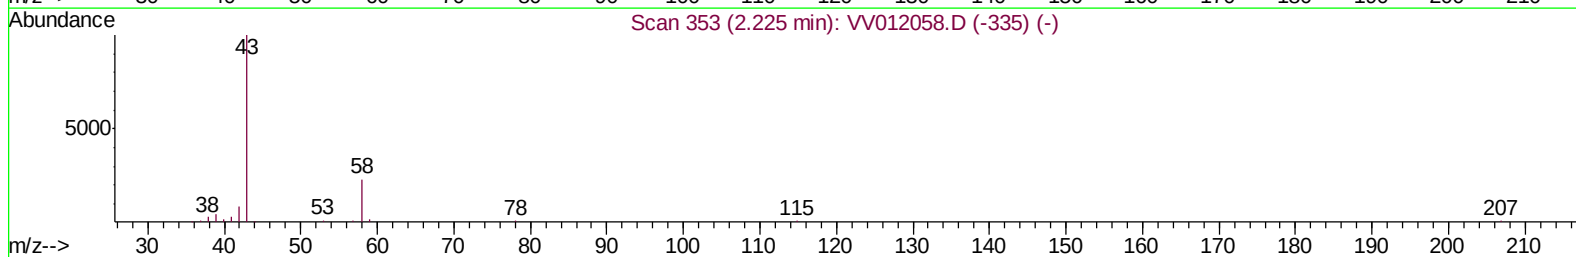
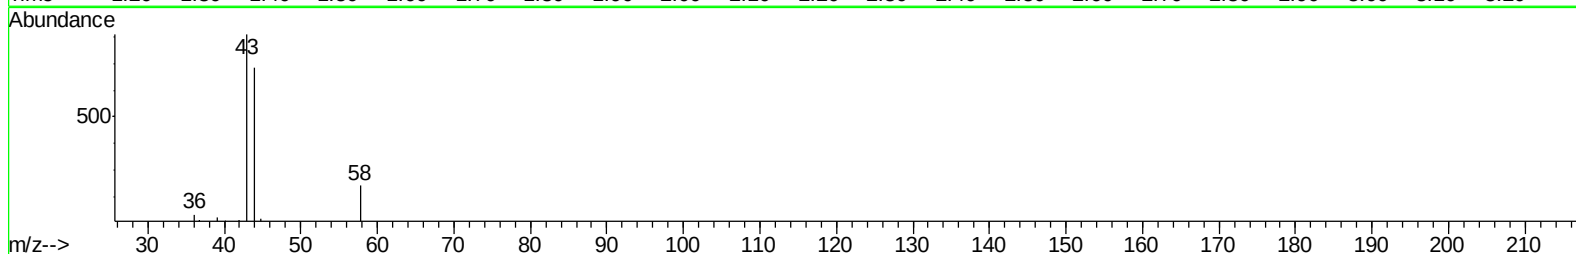


Data File : VV012063.D
Acq On : 29 Jul 2019 15:34
Operator : SY/MD
Sample : MDL01
Misc : 25ML/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Quant Time: Jul 30 08:49:44 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SFAMVTR072919WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Jul 30 08:46:06 2019
Response via : Initial Calibration

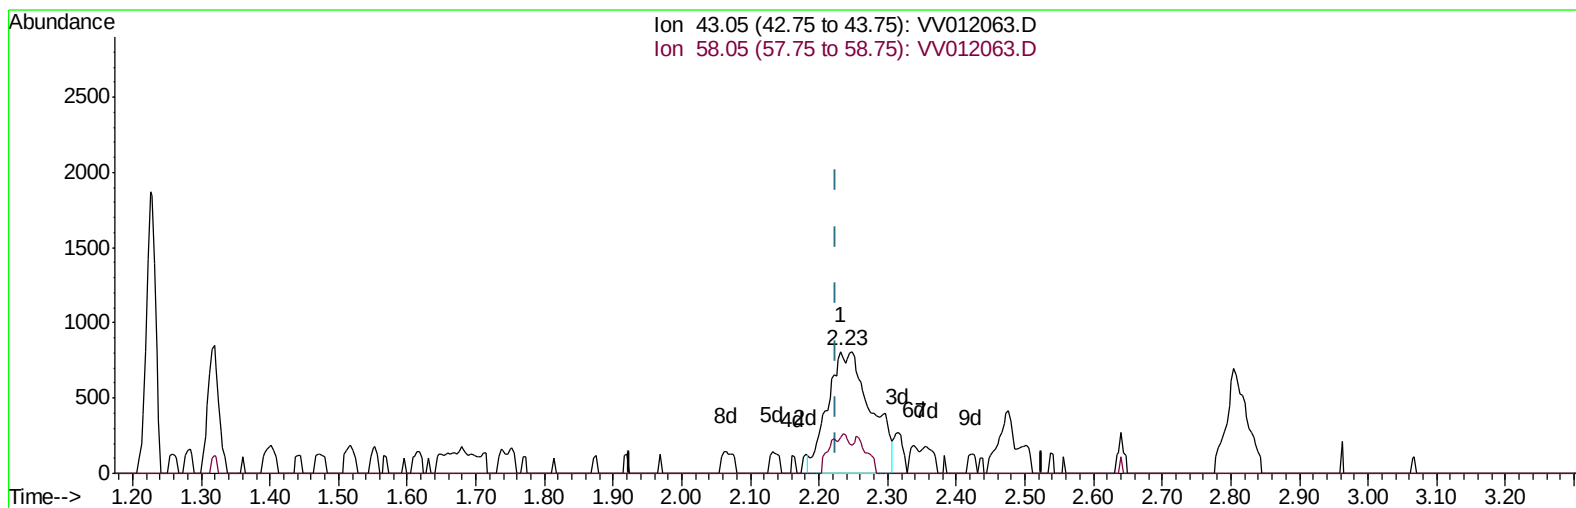

TIC: VV012063.D

(13) Acetone (T)

2.232min (+0.006) 2.81ug/L m

response 3545

Ion	Exp%	Act%
43.05	100	100
58.05	25.80	7.48
0.00	0.00	0.00
0.00	0.00	0.00