
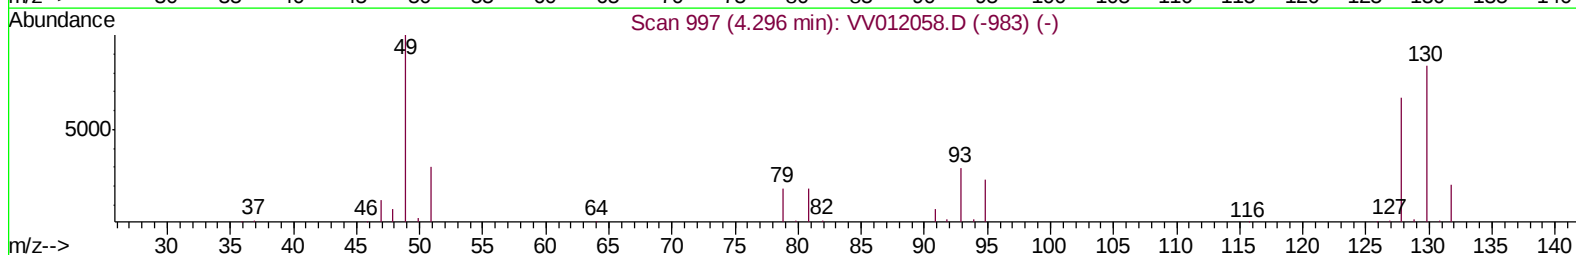
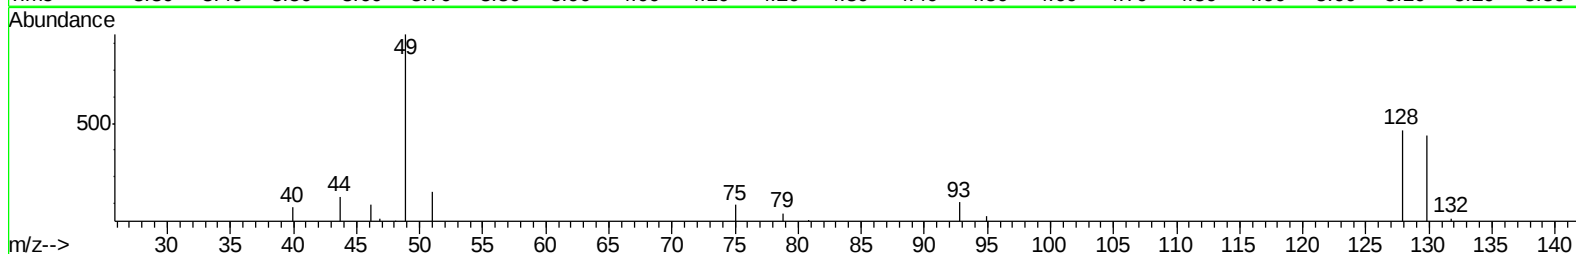


Data File : VV012064.D
Acq On : 29 Jul 2019 15:59
Operator : SY/MD
Sample : MDL02
Misc : 25ML/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Quant Time: Jul 30 08:50:11 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SFAMVTR072919WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Jul 30 08:46:06 2019
Response via : Initial Calibration

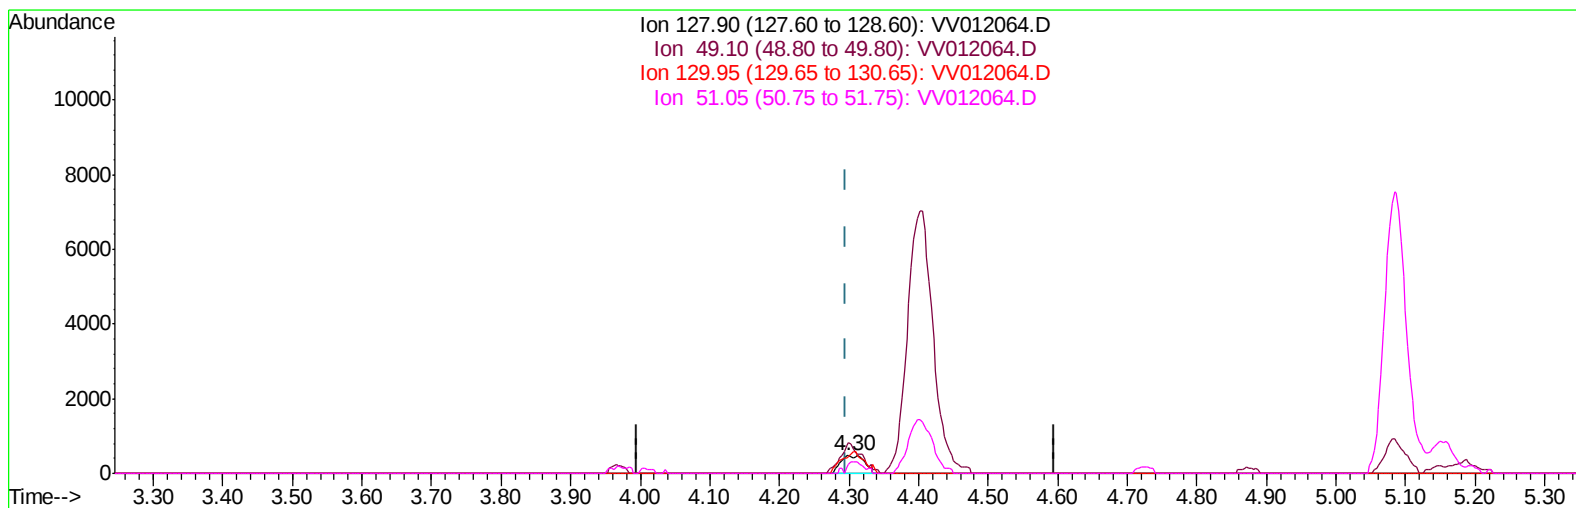

TIC: VV012064.D

(23) Bromochloromethane (T)

4.299min (+0.003) 0.26ug/L m

response 1114

Ion	Exp%	Act%
127.90	100	100
49.10	150.10	175.63
129.95	127.00	95.38
51.05	45.20	50.84