


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV072919\
 Data File : VV012055.D
 Acq On : 29 Jul 2019 09:46
 Operator : SY/MD
 Sample : BFB40
 Misc : 25ML/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB400

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SFAMVTR072919WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Tue Jul 30 08:46:06 2019

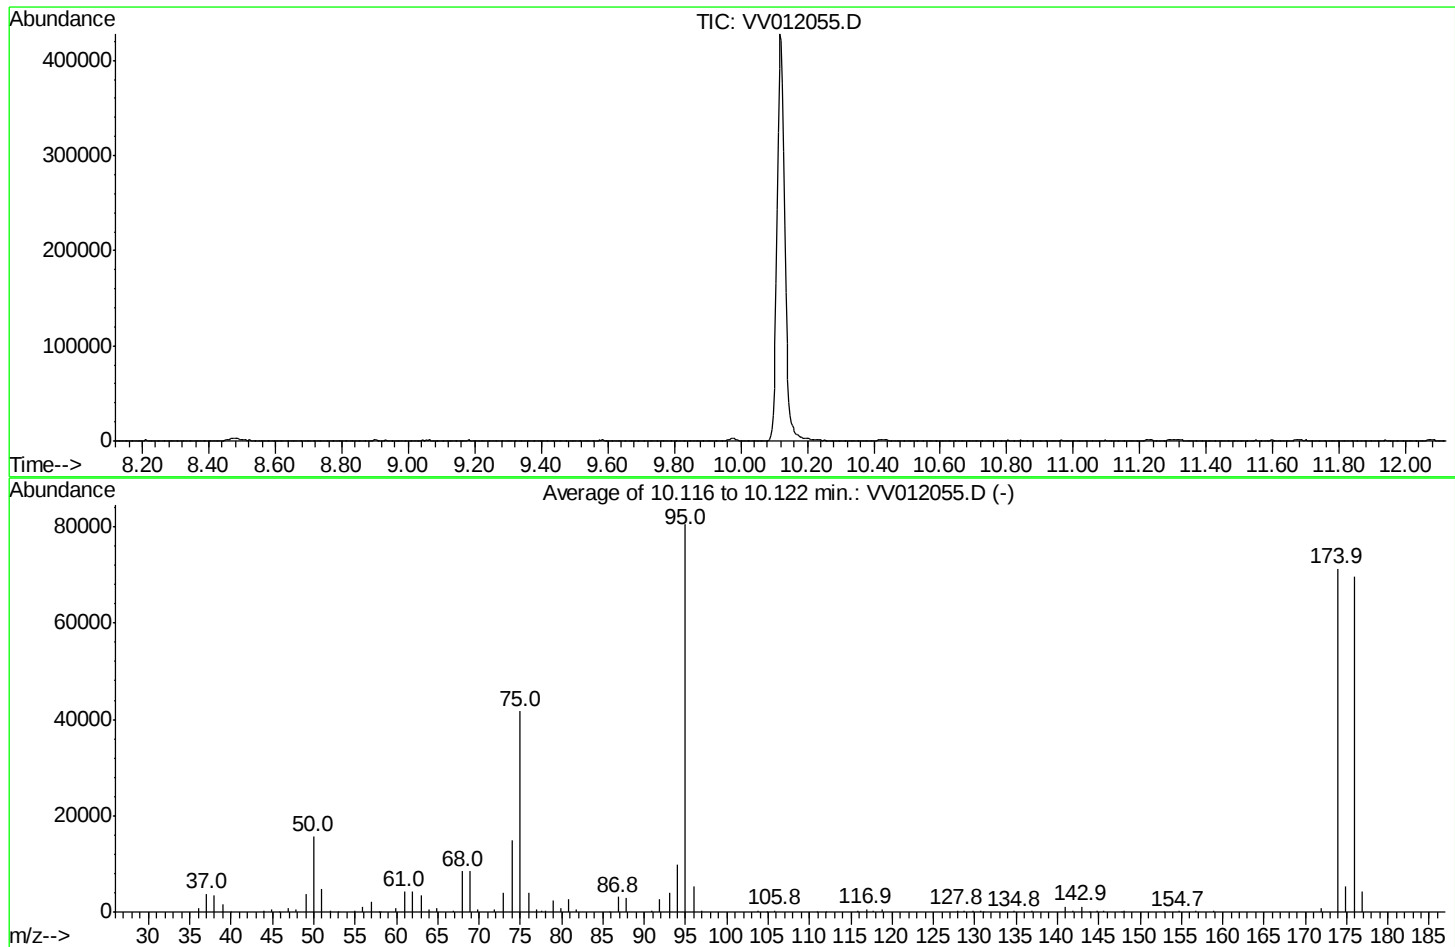

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2793

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.4	15646	PASS
75	95	30	80	51.8	41682	PASS
95	95	100	100	100.0	80514	PASS
96	95	5	9	6.7	5369	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	88.6	71373	PASS
175	174	5	9	7.5	5382	PASS
176	174	95	101	97.5	69616	PASS
177	176	5	9	6.1	4278	PASS

m/z	Abundance
39.90	206.0
43.80	341.0

Instrument :
MSVOA_V
ClientSampleId :
BFB400

m/z	Abundance
36.00	711.0
37.00	3791.0
38.00	3283.0
39.00	1361.0
39.80	195.0
43.90	639.0
44.90	583.0
45.90	123.0
47.00	725.0
47.90	598.0
49.00	3638.0
50.00	14889.0
51.00	4750.0
51.90	216.0
53.00	108.0
54.90	232.0
55.90	1147.0
56.90	2063.0
57.90	132.0
59.80	643.0
60.90	3996.0
61.90	4036.0
63.00	3383.0
63.90	382.0
64.90	782.0
66.80	262.0
68.00	8293.0
68.90	8042.0
69.90	693.0
71.80	454.0
72.90	3905.0
73.90	14125.0
75.00	39920.0
76.00	3728.0
76.90	519.0
77.60	262.0
78.00	291.0
78.90	2278.0
79.90	760.0
80.80	2558.0
81.80	546.0
85.80	137.0
86.80	2846.0
87.90	2576.0
90.90	313.0
91.90	2420.0
93.00	4042.0
94.00	9344.0
95.00	76272.0
95.90	5011.0
96.90	172.0
103.70	382.0
104.90	131.0
105.80	396.0
110.90	124.0
111.90	102.0
115.80	388.0
116.90	572.0
117.70	340.0
118.90	491.0
127.90	278.0
128.70	131.0
129.80	294.0
130.70	179.0
134.80	170.0
136.80	153.0
140.90	964.0
141.90	195.0
142.90	1064.0
143.90	113.0
144.80	279.0
145.70	213.0
148.00	262.0
154.70	246.0
156.80	142.0
158.80	231.0
171.90	882.0
173.90	66856.0
174.90	5017.0
175.90	64704.0
176.90	4117.0

Instrument :
MSVOA_V
ClientSampleId :
BFB400

m/z	Abundance
36.00	735.0
37.00	3830.0
38.00	3485.0
39.00	1593.0
39.80	168.0
44.00	629.0
44.90	655.0
45.90	118.0
46.90	754.0
47.90	592.0
49.00	3876.0
50.00	16314.0
51.00	4957.0
52.00	259.0
52.90	109.0
54.90	223.0
56.00	1188.0
56.90	2068.0
57.90	117.0
59.90	723.0
60.90	4407.0
61.90	4377.0
63.00	3548.0
63.90	426.0
64.90	752.0
66.90	227.0
68.00	8734.0
69.00	8888.0
69.90	668.0
71.90	433.0
72.90	4229.0
73.90	15447.0
75.00	43096.0
76.00	4057.0
76.90	575.0
77.60	270.0
78.00	336.0
78.90	2523.0
79.90	919.0
80.80	2653.0
81.80	635.0
85.80	129.0
86.80	3219.0
87.80	3065.0
90.90	345.0
91.90	2738.0
93.00	4106.0
94.00	10207.0
95.00	83128.0
96.00	5524.0
96.90	221.0
103.70	382.0
104.90	130.0
105.80	417.0
111.00	109.0
112.00	114.0
115.80	439.0
116.90	630.0
117.70	365.0
118.80	588.0
127.90	343.0
128.70	171.0
129.90	293.0
130.70	165.0
131.00	177.0
134.80	191.0
136.80	172.0
140.90	1003.0
141.90	206.0
142.90	1163.0
143.90	112.0
144.80	328.0
145.60	211.0
147.70	209.0
148.00	248.0
152.90	113.0
154.70	255.0
156.80	167.0
158.80	245.0
171.90	926.0
173.90	73792.0
174.90	5536.0
175.90	72048.0
176.90	4324.0

Instrument :
MSVOA_V
ClientSampleId :
BFB400

m/z	Abundance
36.00	685.0
37.00	3690.0
38.00	3373.0
39.00	1537.0
40.00	167.0
44.10	617.0
44.90	681.0
46.90	866.0
47.90	541.0
49.00	3553.0
50.00	15735.0
51.00	4671.0
52.00	255.0
52.80	124.0
55.00	211.0
56.00	1133.0
56.90	1988.0
58.10	111.0
59.90	763.0
61.00	4273.0
61.90	4236.0
63.00	3245.0
63.90	453.0
64.90	594.0
66.90	224.0
68.00	8438.0
69.00	8711.0
69.90	632.0
71.90	424.0
72.90	4077.0
74.00	14899.0
75.00	42032.0
76.00	3904.0
77.00	569.0
78.00	308.0
78.90	2576.0
79.90	1001.0
80.80	2572.0
81.80	693.0
85.90	134.0
86.90	3176.0
87.80	3337.0
90.90	328.0
91.90	2702.0
93.00	3968.0
94.00	9993.0
95.00	82144.0
96.00	5574.0
97.00	218.0
103.80	380.0
104.80	135.0
105.90	373.0
111.00	117.0
115.90	383.0
116.90	651.0
117.70	346.0
118.80	630.0
127.80	350.0
128.70	164.0
129.90	266.0
130.70	120.0
131.00	150.0
134.70	202.0
136.90	187.0
140.90	1012.0
141.80	194.0
142.90	1220.0
144.80	311.0
145.60	204.0
147.70	176.0
148.00	193.0
152.90	123.0
154.60	241.0
156.80	142.0
158.90	215.0
171.80	931.0
173.90	73472.0
174.90	5593.0
175.90	72096.0
177.00	4393.0

Instrument :
MSVOA_V
ClientSampleId :
BFB400