




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
Data File : VV027089.D
Acq On : 29 Jul 2022 16:55
Operator : SY/MD
Sample : N3880-18 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUH4

Manual IntegrationsAPPROVED

Quant Time: Jul 30 00:08:39 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Jul 30 00:04:45 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 08/01/2022
Supervised By :Mahesh Dadoda 08/02/2022

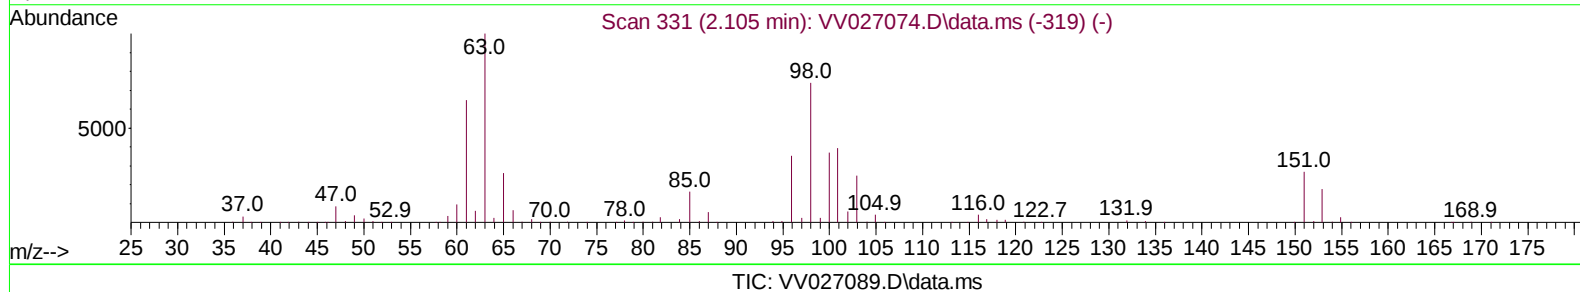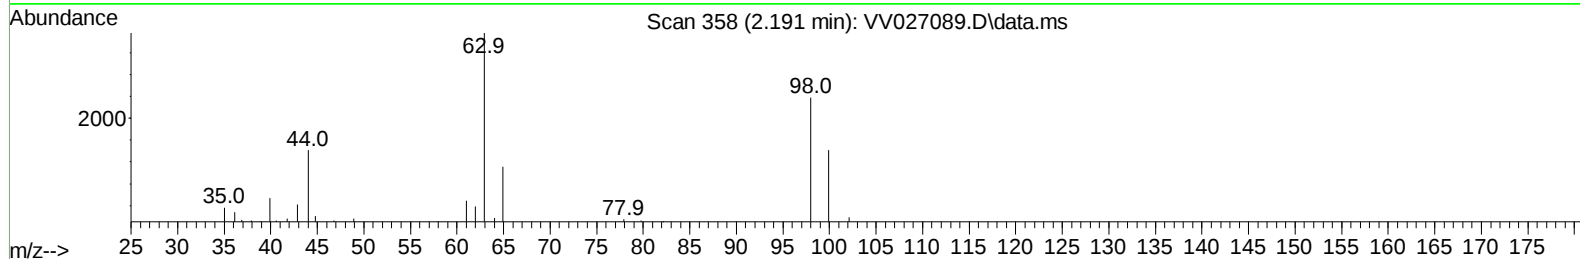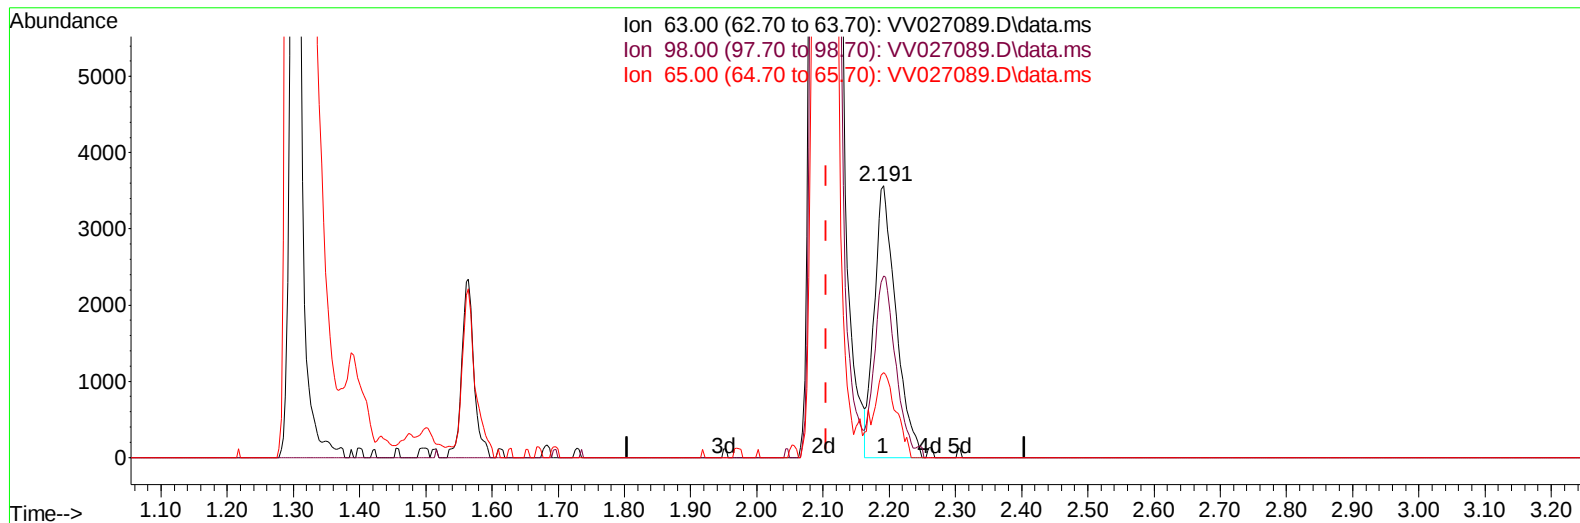

(11) 1,1-Dichloroethene-d2 (S)

2.191min (+ 0.087) 0.95 ug/L

response 8117

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	77.30	65.54
65.00	24.20	29.11
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
 Data File : VV027089.D
 Acq On : 29 Jul 2022 16:55
 Operator : SY/MD
 Sample : N3880-18 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUH4

Manual IntegrationsAPPROVED

Quant Time: Jul 30 00:08:39 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jul 30 00:04:45 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 08/01/2022
 Supervised By :Mahesh Dadoda 08/02/2022

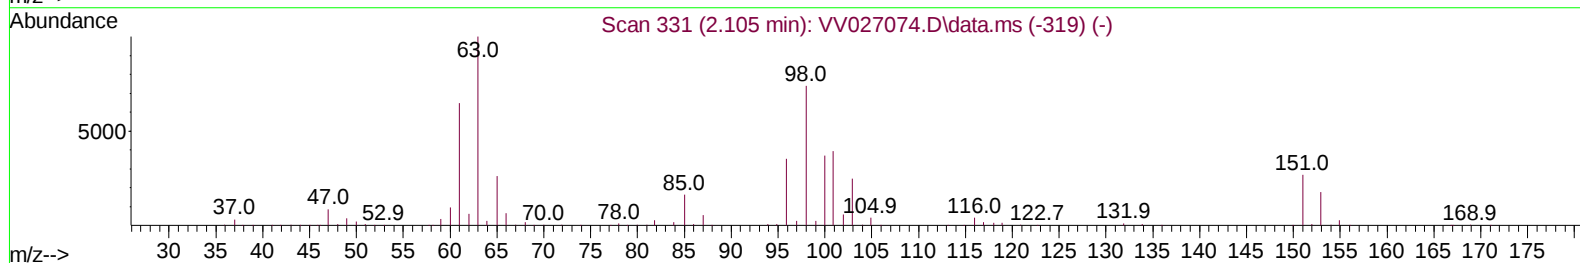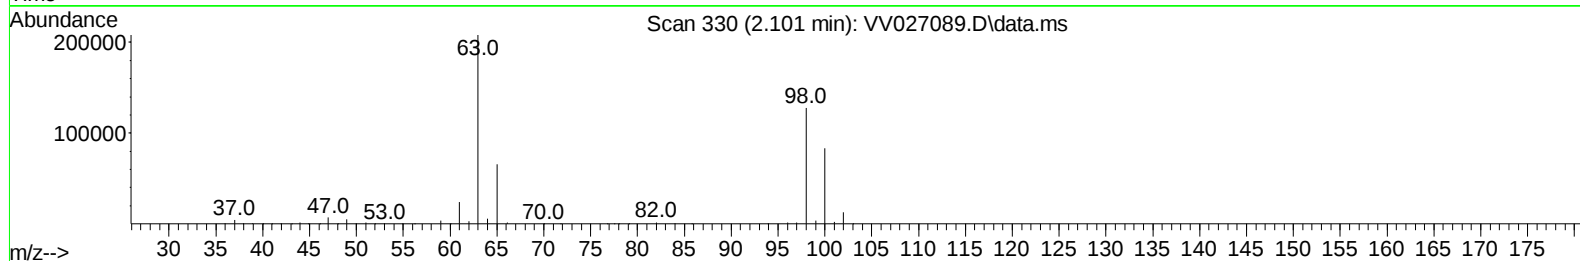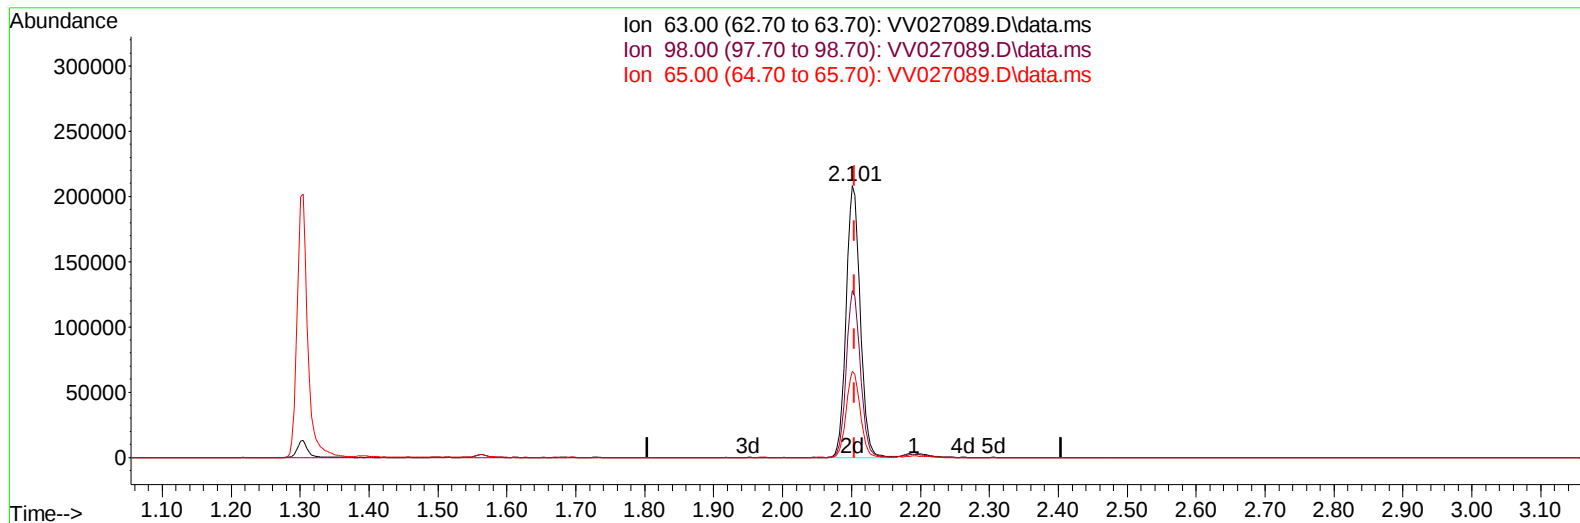

TIC: VV027089.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

2.101min (-0.003) 34.63 ug/L m

response 294771

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	77.30	1.80#
65.00	24.20	0.80#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
 Data File : VV027089.D
 Acq On : 29 Jul 2022 16:55
 Operator : SY/MD
 Sample : N3880-18 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUH4

Manual IntegrationsAPPROVED

Quant Time: Jul 30 00:08:39 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jul 30 00:04:45 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 08/01/2022
 Supervised By :Mahesh Dadoda 08/02/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.613	114	525485	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	522409	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	218030	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	217868	43.580	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	87.160%	
7) Chloroethane-d5	1.564	69	178544	45.075	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	90.160%	
11) 1,1-Dichloroethene-d2	2.101	63	294771m	34.634	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	69.260%	
21) 2-Butanone-d5	3.886	46	192620	67.571	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	67.570%	
24) Chloroform-d	4.342	84	397958	44.198	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	88.400%	
26) 1,2-Dichloroethane-d4	5.027	65	236521	46.274	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	92.540%	
32) Benzene-d6	5.047	84	832951	45.405	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	90.800%	
36) 1,2-Dichloropropane-d6	6.066	67	267327	47.610	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	95.220%	
41) Toluene-d8	7.313	98	675782	40.755	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	81.500%	
43) trans-1,3-Dichloroprop...	7.619	79	100158	40.381	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	80.760%	
47) 2-Hexanone-d5	8.092	63	189043	78.318	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	78.320%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	363383	42.923	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	85.840%	
66) 1,2-Dichlorobenzene-d4	11.622	152	239559	48.877	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	97.760%	
Target Compounds						
46) Tetrachloroethene	7.976	164	40463	11.939	ug/L	Qvalue 98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
Data File : VV027089.D
Acq On : 29 Jul 2022 16:55
Operator : SY/MD
Sample : N3880-18 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 3

Instrument :
MSVOA_V
ClientSampleId :
DBUH4

Manual IntegrationsAPPROVED

Quant Time: Jul 30 00:08:39 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Jul 30 00:04:45 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 08/01/2022
Supervised By :Mahesh Dadoda 08/02/2022

