




Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV072922\  
 Data File : VV027096.D  
 Acq On : 29 Jul 2022 19:47  
 Operator : SY/MD  
 Sample : N3899-03  
 Misc : 5.0mL/MSVOA\_V/WATER  
 ALS Vial : 24 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 DBUR2

Manual IntegrationsAPPROVED

Quant Time: Jul 30 00:10:20 2022  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVLM072822WMA.M  
 Quant Title : VOC Analysis  
 QLast Update : Sat Jul 30 00:04:45 2022  
 Response via : Initial Calibration

Reviewed By :Krupa Patel 08/01/2022  
 Supervised By :Mahesh Dadoda 08/02/2022

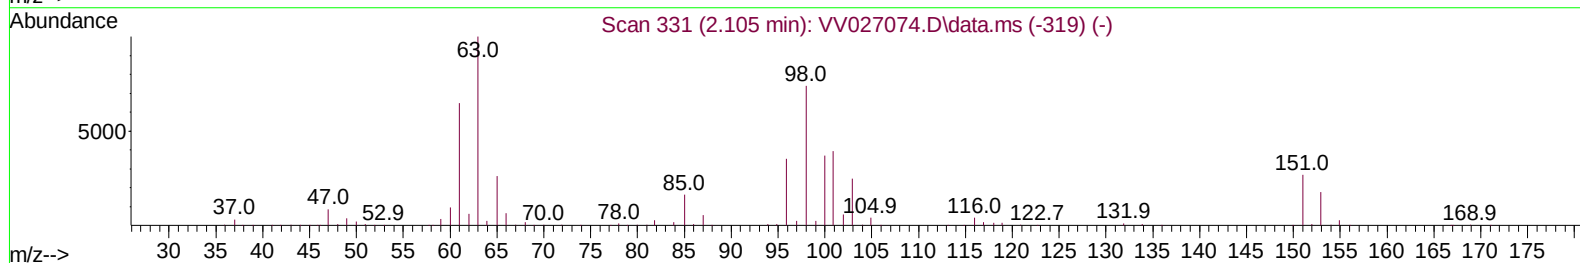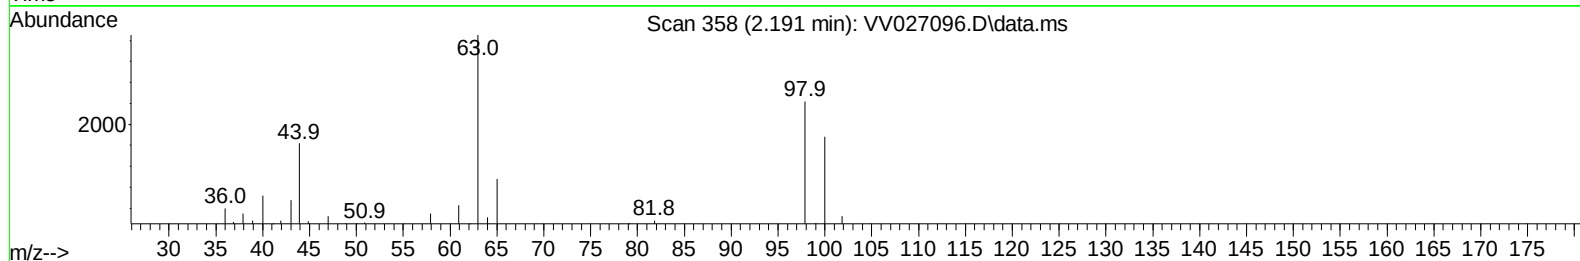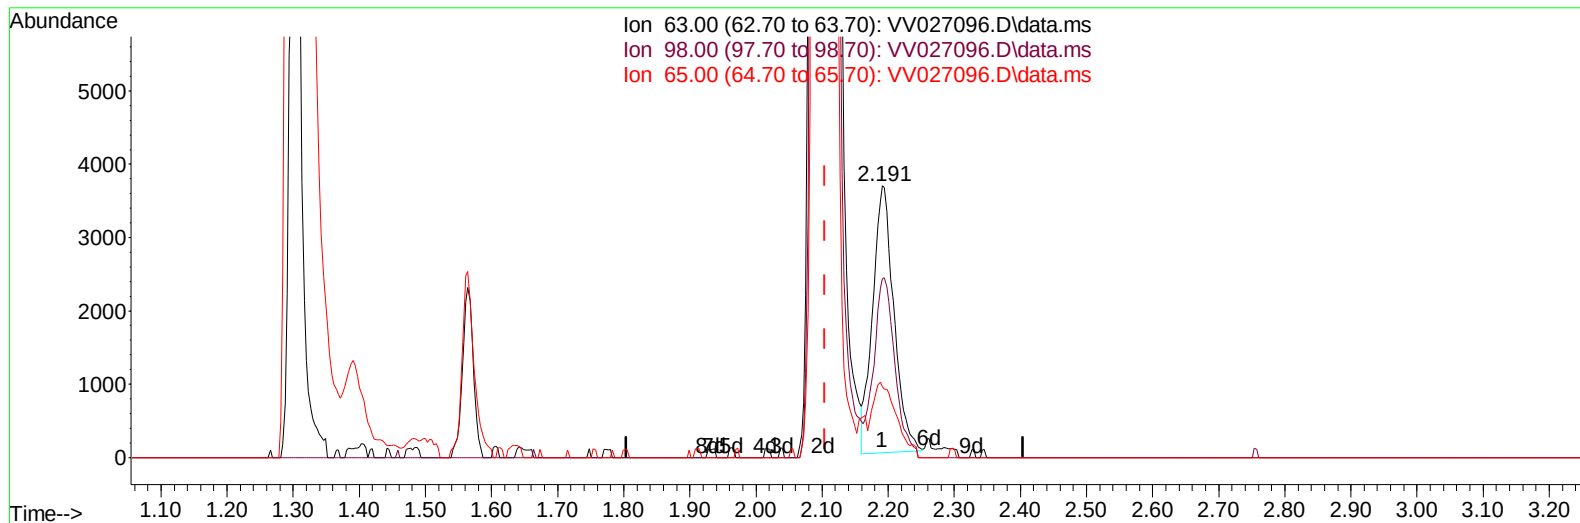

TIC: VV027096.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

2.191min (+ 0.087) 0.89 ug/L

response 8088

| Ion   | Exp%   | Act%   |
|-------|--------|--------|
| 63.00 | 100.00 | 100.00 |
| 98.00 | 77.30  | 67.10  |
| 65.00 | 24.20  | 24.06  |
| 0.00  | 0.00   | 0.00   |




Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV072922\  
 Data File : VV027096.D  
 Acq On : 29 Jul 2022 19:47  
 Operator : SY/MD  
 Sample : N3899-03  
 Misc : 5.0mL/MSVOA\_V/WATER  
 ALS Vial : 24 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 DBUR2

Manual IntegrationsAPPROVED

Quant Time: Jul 30 00:10:20 2022  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVLM072822WMA.M  
 Quant Title : VOC Analysis  
 QLast Update : Sat Jul 30 00:04:45 2022  
 Response via : Initial Calibration

Reviewed By :Krupa Patel 08/01/2022  
 Supervised By :Mahesh Dadoda 08/02/2022

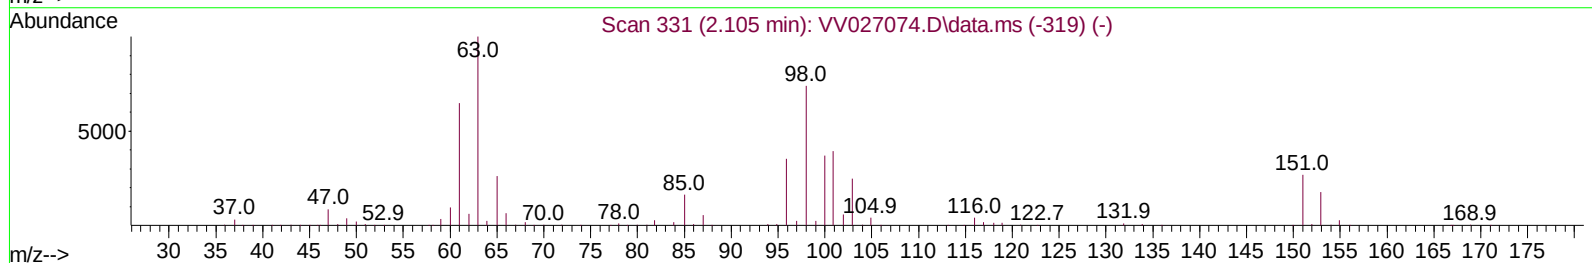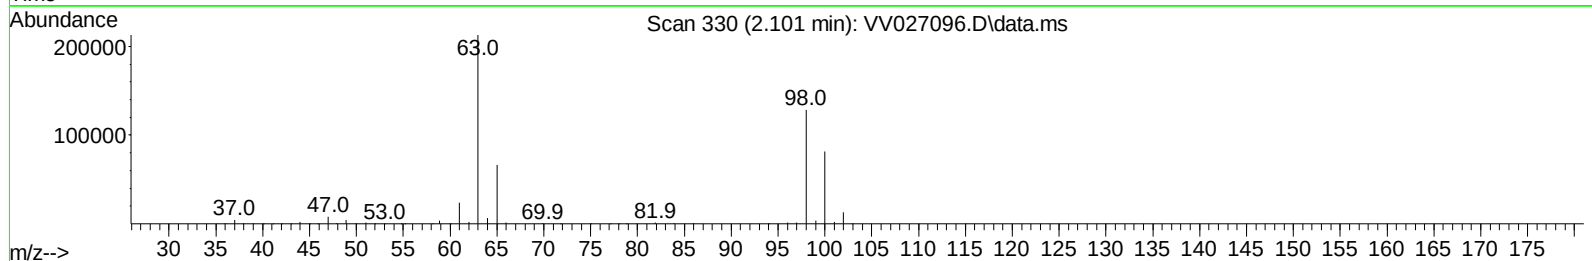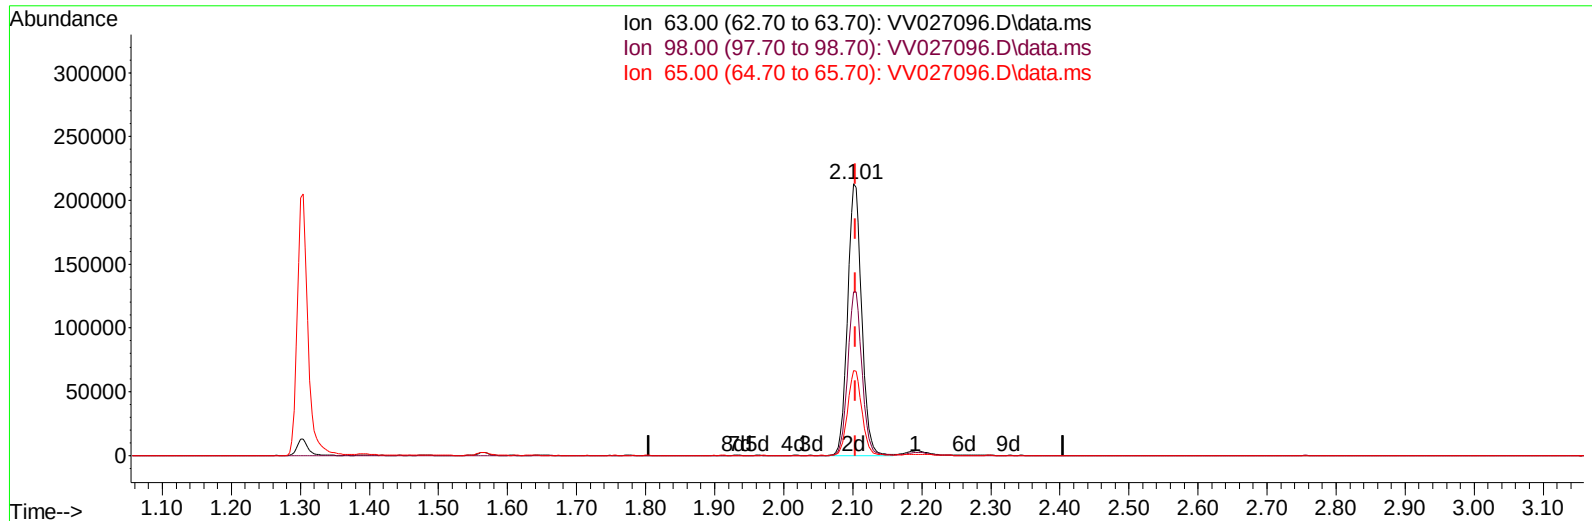

TIC: VV027096.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

2.101min (-0.003) 33.24 ug/L m

response 301899

| Ion   | Exp%   | Act%   |
|-------|--------|--------|
| 63.00 | 100.00 | 100.00 |
| 98.00 | 77.30  | 1.80#  |
| 65.00 | 24.20  | 0.64#  |
| 0.00  | 0.00   | 0.00   |

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV072922\  
 Data File : VV027096.D  
 Acq On : 29 Jul 2022 19:47  
 Operator : SY/MD  
 Sample : N3899-03  
 Misc : 5.0mL/MSVOA\_V/WATER  
 ALS Vial : 24 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 DBUR2

Manual IntegrationsAPPROVED

Quant Time: Jul 30 00:10:20 2022  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVLM072822WMA.M  
 Quant Title : VOC Analysis  
 QLast Update : Sat Jul 30 00:04:45 2022  
 Response via : Initial Calibration

Reviewed By :Krupa Patel 08/01/2022  
 Supervised By :Mahesh Dadoda 08/02/2022

| Compound                      | R.T.     | QIon  | Response | Conc   | Units   | Dev(Min) |
|-------------------------------|----------|-------|----------|--------|---------|----------|
| -----                         |          |       |          |        |         |          |
| Internal Standards            |          |       |          |        |         |          |
| 1) 1,4-Difluorobenzene        | 5.612    | 114   | 560715   | 50.000 | ug/L    | 0.00     |
| 28) Chlorobenzene-d5          | 8.850    | 117   | 556857   | 50.000 | ug/L    | 0.00     |
| 58) 1,4-Dichlorobenzene-d4    | 11.249   | 152   | 241317   | 50.000 | ug/L    | 0.00     |
| System Monitoring Compounds   |          |       |          |        |         |          |
| 4) Vinyl Chloride-d3          | 1.304    | 65    | 218756   | 41.008 | ug/L    | 0.00     |
| Spiked Amount 50.000          | Range 60 | - 135 | Recovery | =      | 82.020% |          |
| 7) Chloroethane-d5            | 1.564    | 69    | 182153   | 43.097 | ug/L    | 0.00     |
| Spiked Amount 50.000          | Range 70 | - 130 | Recovery | =      | 86.200% |          |
| 11) 1,1-Dichloroethene-d2     | 2.101    | 63    | 301899m  | 33.243 | ug/L    | 0.00     |
| Spiked Amount 50.000          | Range 60 | - 125 | Recovery | =      | 66.480% |          |
| 21) 2-Butanone-d5             | 3.889    | 46    | 185487   | 60.980 | ug/L    | 0.00     |
| Spiked Amount 100.000         | Range 40 | - 130 | Recovery | =      | 60.980% |          |
| 24) Chloroform-d              | 4.342    | 84    | 402398   | 41.883 | ug/L    | 0.00     |
| Spiked Amount 50.000          | Range 70 | - 125 | Recovery | =      | 83.760% |          |
| 26) 1,2-Dichloroethane-d4     | 5.027    | 65    | 236658   | 43.392 | ug/L    | 0.00     |
| Spiked Amount 50.000          | Range 70 | - 125 | Recovery | =      | 86.780% |          |
| 32) Benzene-d6                | 5.046    | 84    | 835040   | 42.703 | ug/L    | 0.00     |
| Spiked Amount 50.000          | Range 70 | - 125 | Recovery | =      | 85.400% |          |
| 36) 1,2-Dichloropropane-d6    | 6.066    | 67    | 264533   | 44.198 | ug/L    | 0.00     |
| Spiked Amount 50.000          | Range 70 | - 120 | Recovery | =      | 88.400% |          |
| 41) Toluene-d8                | 7.313    | 98    | 708188   | 40.067 | ug/L    | 0.00     |
| Spiked Amount 50.000          | Range 80 | - 120 | Recovery | =      | 80.140% |          |
| 43) trans-1,3-Dichloroprop... | 7.619    | 79    | 101401   | 38.353 | ug/L    | 0.00     |
| Spiked Amount 50.000          | Range 60 | - 125 | Recovery | =      | 76.700% |          |
| 47) 2-Hexanone-d5             | 8.091    | 63    | 207222   | 80.539 | ug/L    | 0.00     |
| Spiked Amount 100.000         | Range 45 | - 130 | Recovery | =      | 80.540% |          |
| 56) 1,1,2,2-Tetrachloroeth... | 10.213   | 84    | 377349   | 41.816 | ug/L    | 0.00     |
| Spiked Amount 50.000          | Range 65 | - 120 | Recovery | =      | 83.640% |          |
| 66) 1,2-Dichlorobenzene-d4    | 11.622   | 152   | 260548   | 48.029 | ug/L    | 0.00     |
| Spiked Amount 50.000          | Range 80 | - 120 | Recovery | =      | 96.060% |          |

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV072922\  
Data File : VV027096.D  
Acq On : 29 Jul 2022 19:47  
Operator : SY/MD  
Sample : N3899-03  
Misc : 5.0mL/MSVOA\_V/WATER  
ALS Vial : 24 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
DBUR2

Manual IntegrationsAPPROVED

Quant Time: Jul 30 00:10:20 2022  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVLM072822WMA.M  
Quant Title : VOC Analysis  
QLast Update : Sat Jul 30 00:04:45 2022  
Response via : Initial Calibration

Reviewed By :Krupa Patel 08/01/2022  
Supervised By :Mahesh Dadoda 08/02/2022

