




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
Data File : VV027102.D
Acq On : 29 Jul 2022 23:03
Operator : SY/MD
Sample : N3955-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0ZD7

Manual IntegrationsAPPROVED

Quant Time: Jul 30 04:28:02 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Jul 30 01:28:32 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 08/01/2022
Supervised By :Mahesh Dadoda 08/02/2022

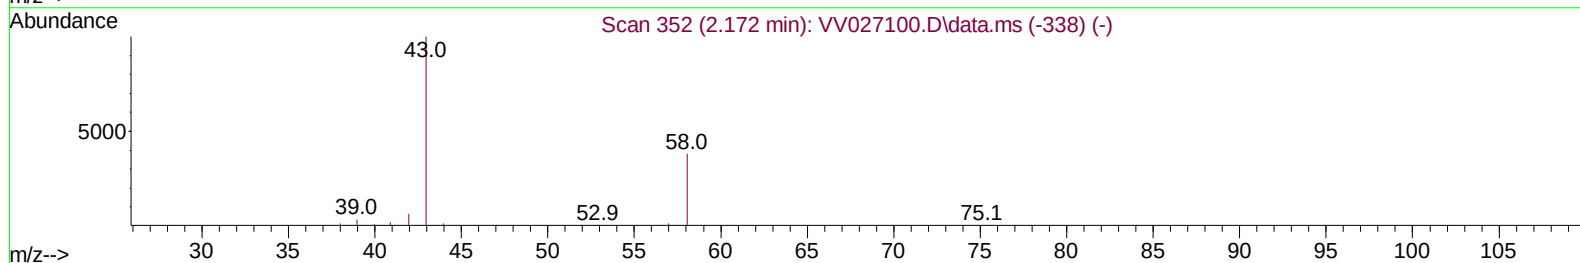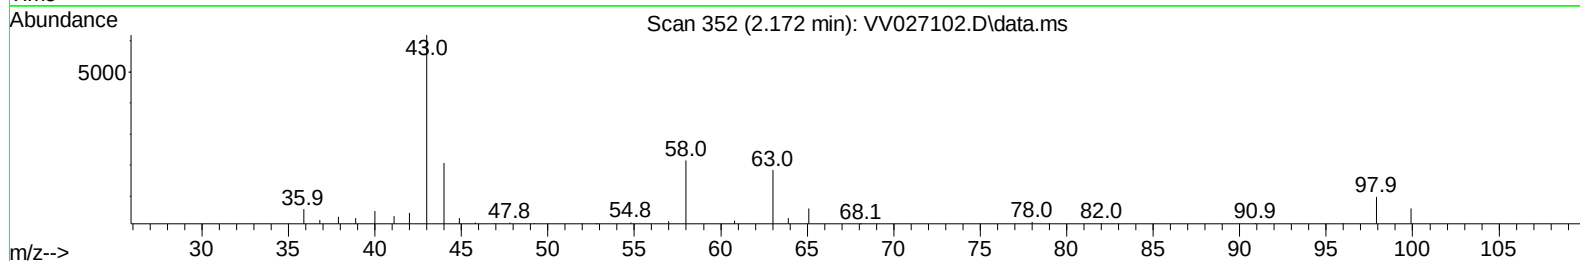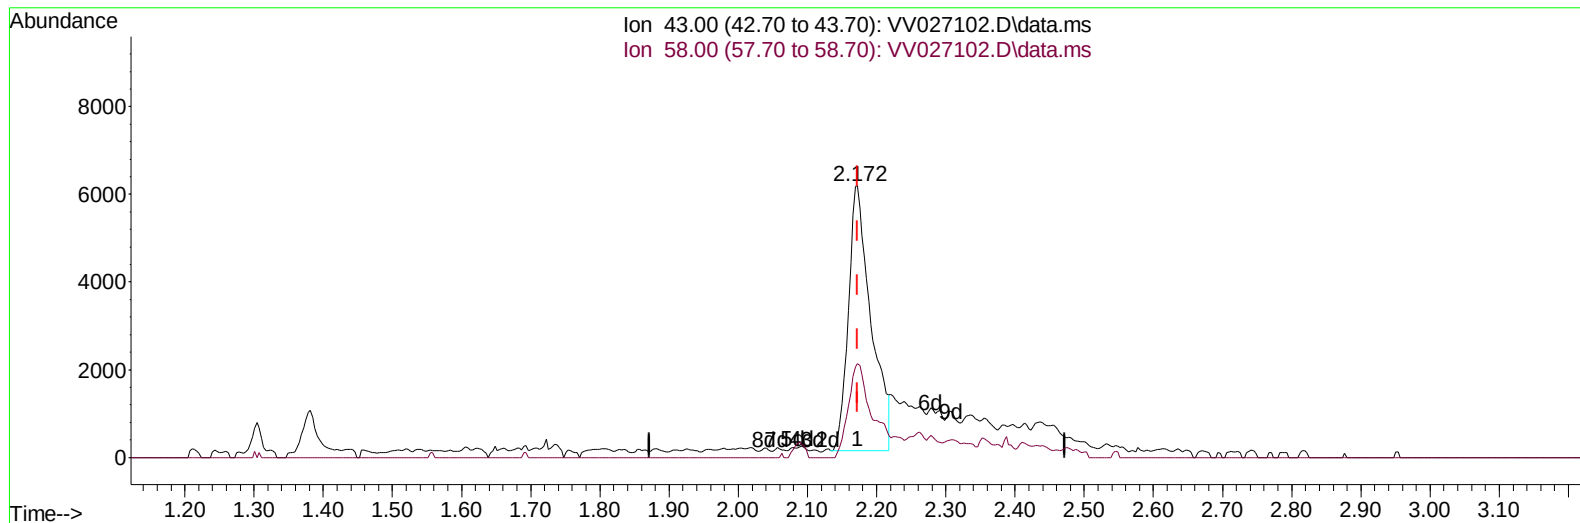

TIC: VV027102.D\data.ms

(13) Acetone (T)

2.172min (+ 0.000) 6.32 ug/L

response 13633

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	24.80	37.49
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
 Data File : VV027102.D
 Acq On : 29 Jul 2022 23:03
 Operator : SY/MD
 Sample : N3955-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0ZD7

Manual IntegrationsAPPROVED

Quant Time: Jul 30 04:28:02 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jul 30 01:28:32 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 08/01/2022
 Supervised By :Mahesh Dadoda 08/02/2022

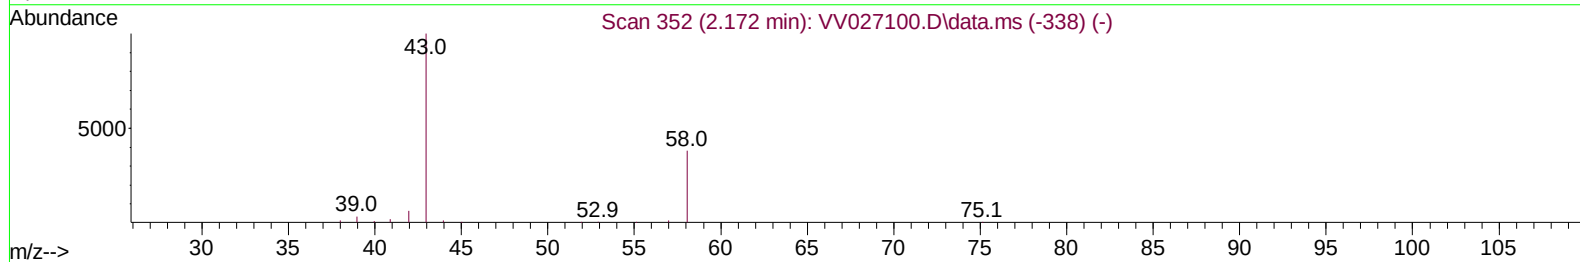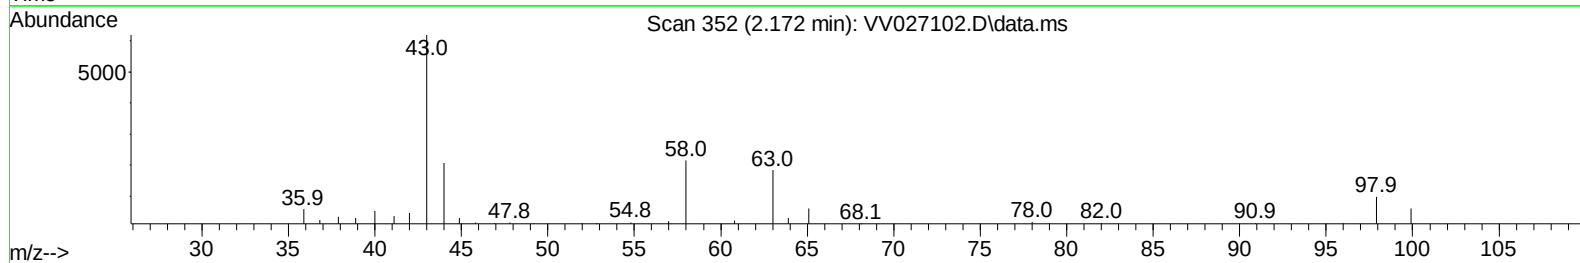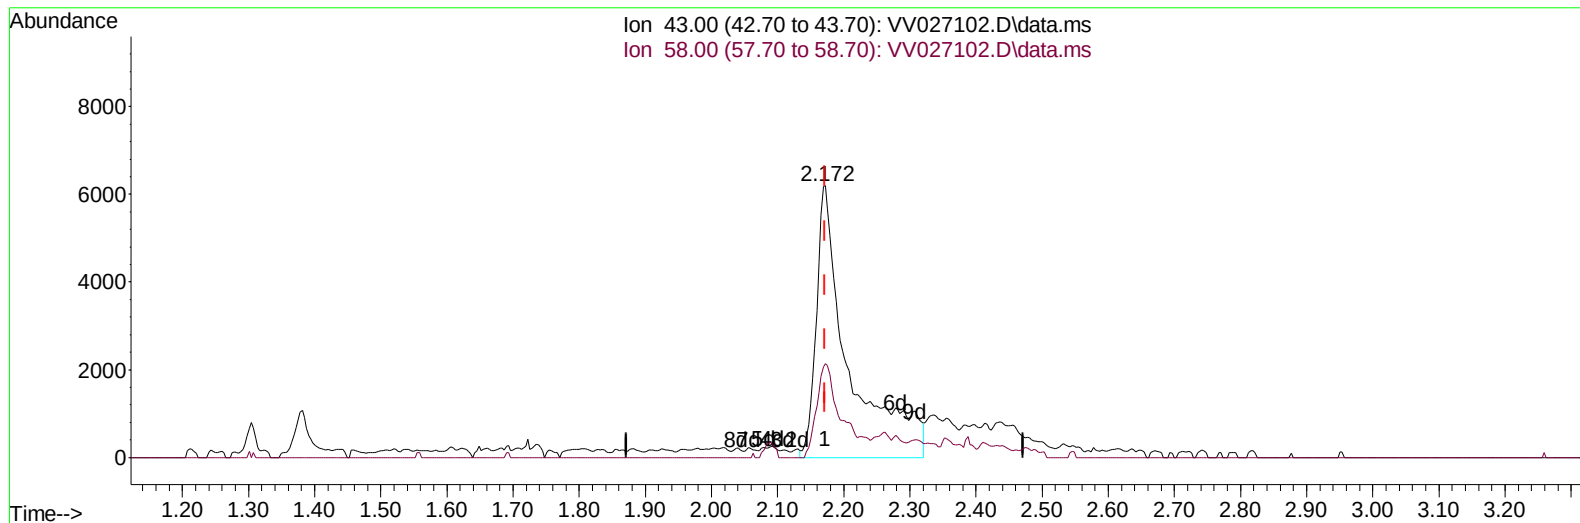

TIC: VV027102.D\data.ms

(13) Acetone (T)

2.172min (+ 0.000) 9.82 ug/L m

response 21178

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	24.80	24.13
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
 Data File : VV072102.D
 Acq On : 29 Jul 2022 23:03
 Operator : SY/MD
 Sample : N3955-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0ZD7

Manual IntegrationsAPPROVED

Quant Time: Jul 30 04:28:02 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jul 30 01:28:32 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 08/01/2022
 Supervised By :Mahesh Dadoda 08/02/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.613	114	536783	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	527473	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	233270	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	196092	38.398	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	76.800%	
7) Chloroethane-d5	1.565	69	169645	41.927	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	83.860%	
11) 1,1-Dichloroethene-d2	2.102	63	280913	32.311	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	64.620%	
21) 2-Butanone-d5	3.886	46	175696	60.337	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	60.340%	
24) Chloroform-d	4.343	84	386045	41.972	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	83.940%	
26) 1,2-Dichloroethane-d4	5.027	65	232542	44.538	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	89.080%	
32) Benzene-d6	5.047	84	805077	43.464	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	86.920%	
36) 1,2-Dichloropropane-d6	6.066	67	256216	45.193	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	90.380%	
41) Toluene-d8	7.314	98	673878	40.250	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	80.500%	
43) trans-1,3-Dichloroprop...	7.619	79	98749	39.431	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	78.860%	
47) 2-Hexanone-d5	8.092	63	186501	76.523	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	76.520%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	346918	40.585	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	81.160%	
66) 1,2-Dichlorobenzene-d4	11.622	152	245052	46.731	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	93.460%	
Target Compounds						
13) Acetone	2.172	43	21178m	9.819	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
Data File : VV027102.D
Acq On : 29 Jul 2022 23:03
Operator : SY/MD
Sample : N3955-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0ZD7

Manual IntegrationsAPPROVED

Quant Time: Jul 30 04:28:02 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Jul 30 01:28:32 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 08/01/2022
Supervised By :Mahesh Dadoda 08/02/2022

