

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
 Data File : VV027118.D
 Acq On : 30 Jul 2022 05:34
 Operator : SY/MD
 Sample : N3899-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUR6

Quant Time: Jul 30 06:09:44 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jul 30 01:28:32 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.613	114	602247	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	589454	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	254285	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	221412	38.644	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	77.280%
7) Chloroethane-d5	1.564	69	186106	40.996	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	82.000%
11) 1,1-Dichloroethene-d2	2.101	63	308253	31.602	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	63.200%
21) 2-Butanone-d5	3.886	46	200766	61.452	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	61.450%
24) Chloroform-d	4.342	84	424362	41.123	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	82.240%
26) 1,2-Dichloroethane-d4	5.027	65	248879	42.486	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	84.980%
32) Benzene-d6	5.043	84	896594	43.315	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	86.620%
36) 1,2-Dichloropropane-d6	6.066	67	273916	43.235	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	86.480%
41) Toluene-d8	7.313	98	759333	40.585	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	81.180%
43) trans-1,3-Dichloroprop...	7.619	79	104446	37.320	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	74.640%
47) 2-Hexanone-d5	8.088	63	212653	78.079	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	78.080%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	381918	39.981	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	79.960%
66) 1,2-Dichlorobenzene-d4	11.622	152	267139	46.733	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	93.460%
Target Compounds						
					Qvalue	
51) Chlorobenzene	8.879	112	11454	0.867	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
Data File : VV027118.D
Acq On : 30 Jul 2022 05:34
Operator : SY/MD
Sample : N3899-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUR6

Quant Time: Jul 30 06:09:44 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Jul 30 01:28:32 2022
Response via : Initial Calibration

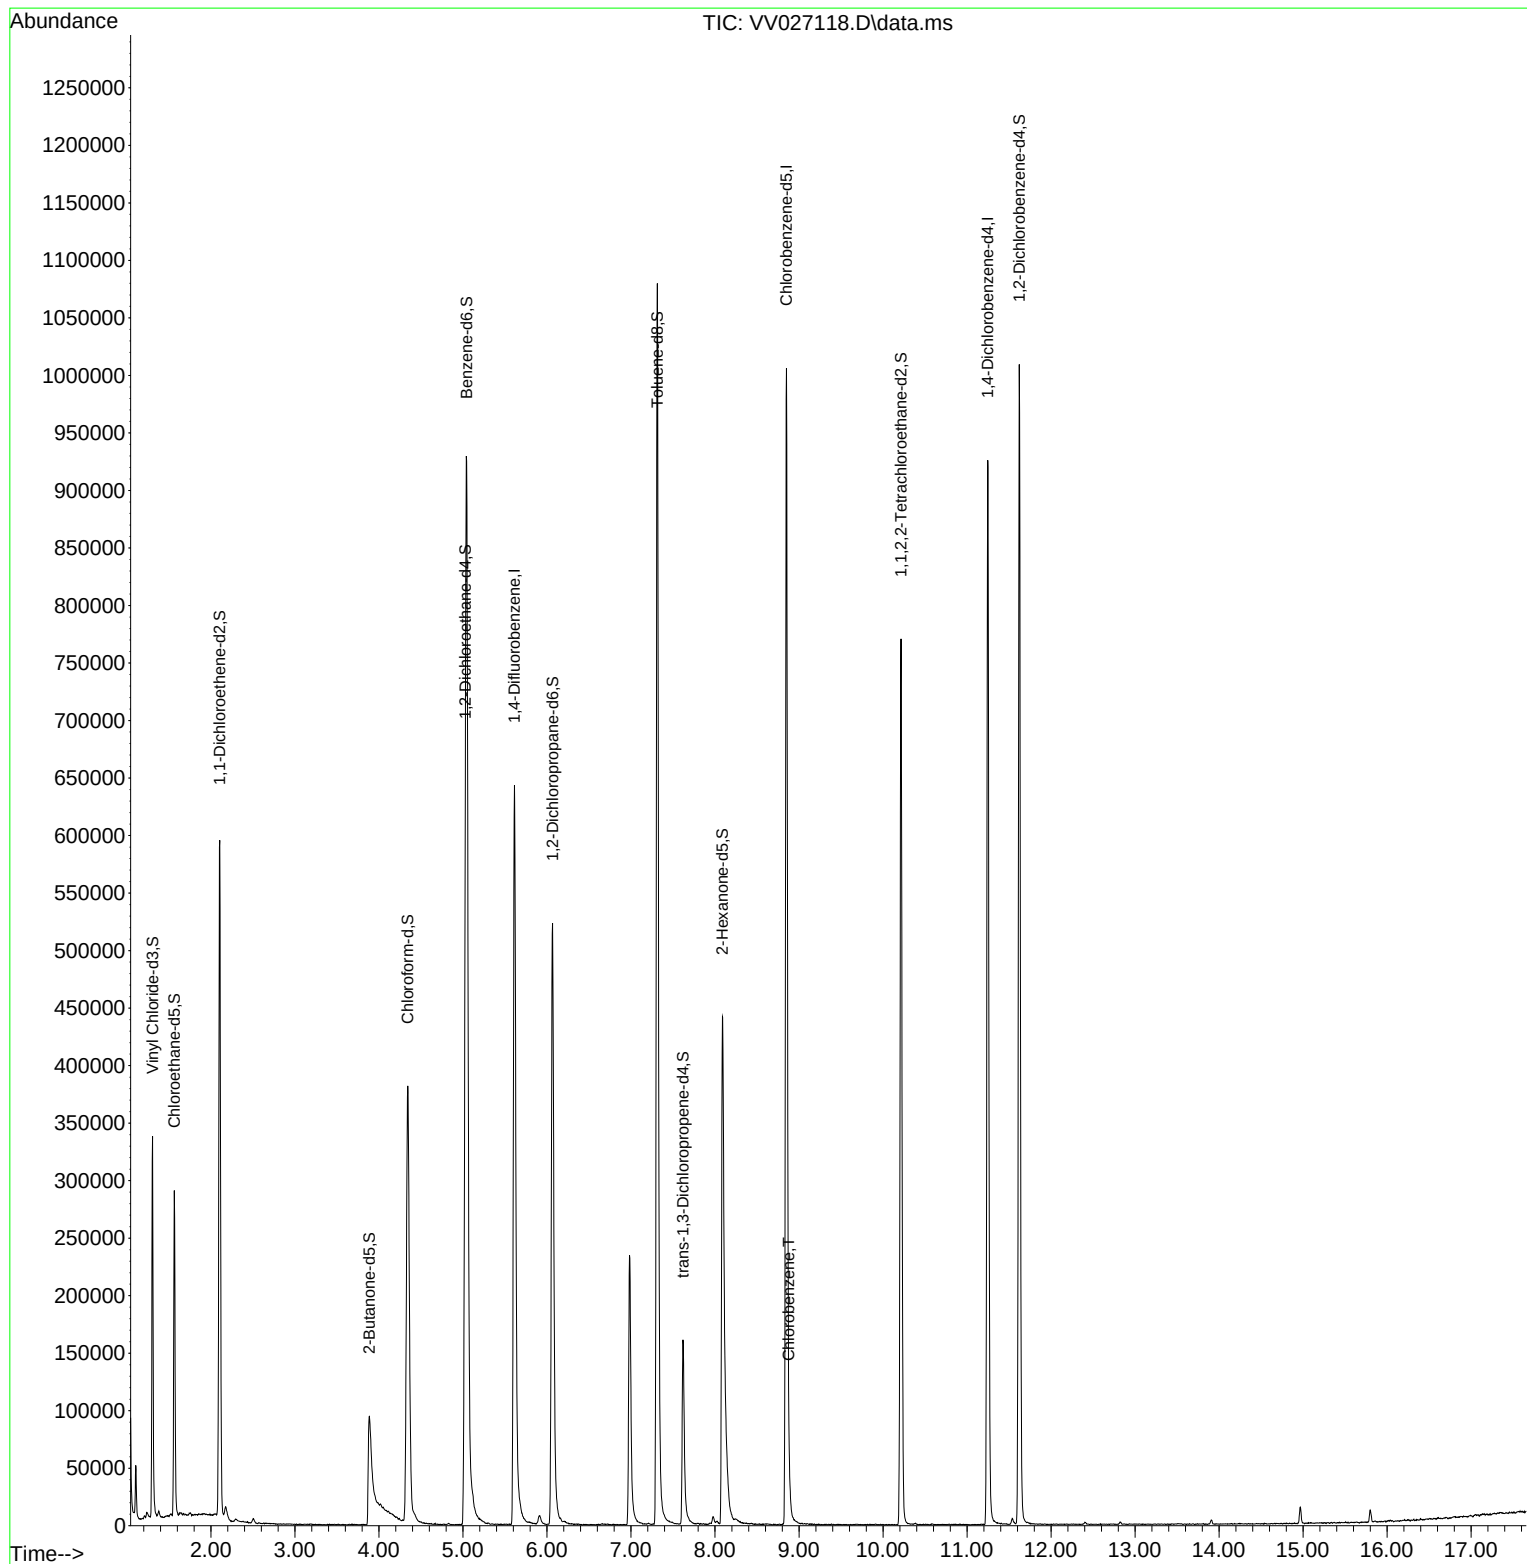

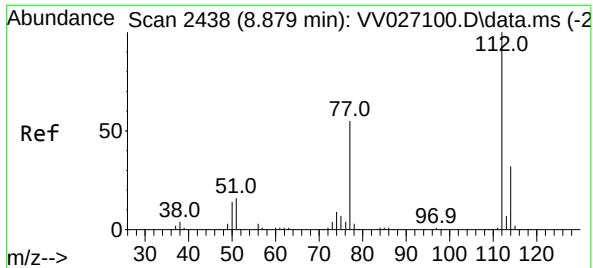

#51
 Chlorobenzene
 Concen: 0.867 ug/L
 RT: 8.879 min Scan# 24
 Delta R.T. 0.000 min
 Lab File: VV027118.D
 Acq: 30 Jul 2022 05:34

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUR6

Tgt Ion:112	Resp:	11454
Ion	Ratio	Lower Upper
112	100	
114	33.0	22.8 42.4
77	61.3	44.2 66.2

