

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW072922\
 Data File : VW027119.D
 Acq On : 30 Jul 2022 05:59
 Operator : SY/MD
 Sample : N3899-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUS3

Quant Time: Jul 30 06:28:18 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jul 30 01:28:32 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.613	114	607526	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	596594	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	267573	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	216754	37.502	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	75.000%		
7) Chloroethane-d5	1.565	69	185963	40.608	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	81.220%		
11) 1,1-Dichloroethene-d2	2.102	63	304931	30.989	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	61.980%		
21) 2-Butanone-d5	3.892	46	193873	58.826	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	58.830%		
24) Chloroform-d	4.343	84	428224	41.137	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	82.280%		
26) 1,2-Dichloroethane-d4	5.027	65	253943	42.973	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	85.940%		
32) Benzene-d6	5.044	84	903797	43.140	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	86.280%		
36) 1,2-Dichloropropane-d6	6.066	67	283633	44.233	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	88.460%		
41) Toluene-d8	7.314	98	761036	40.189	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	80.380%		
43) trans-1,3-Dichloroprop...	7.619	79	104025	36.725	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	73.460%		
47) 2-Hexanone-d5	8.088	63	212897	77.233	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	77.230%		
56) 1,1,2,2-Tetrachloroeth...	10.214	84	381368	39.446	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	78.900%		
66) 1,2-Dichlorobenzene-d4	11.622	152	273589	45.485	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	90.960%		
Target Compounds					Qvalue	
13) Acetone	2.179	43	10443	4.278	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
Data File : VV0727119.D
Acq On : 30 Jul 2022 05:59
Operator : SY/MD
Sample : N3899-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUS3

Quant Time: Jul 30 06:28:18 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Jul 30 01:28:32 2022
Response via : Initial Calibration

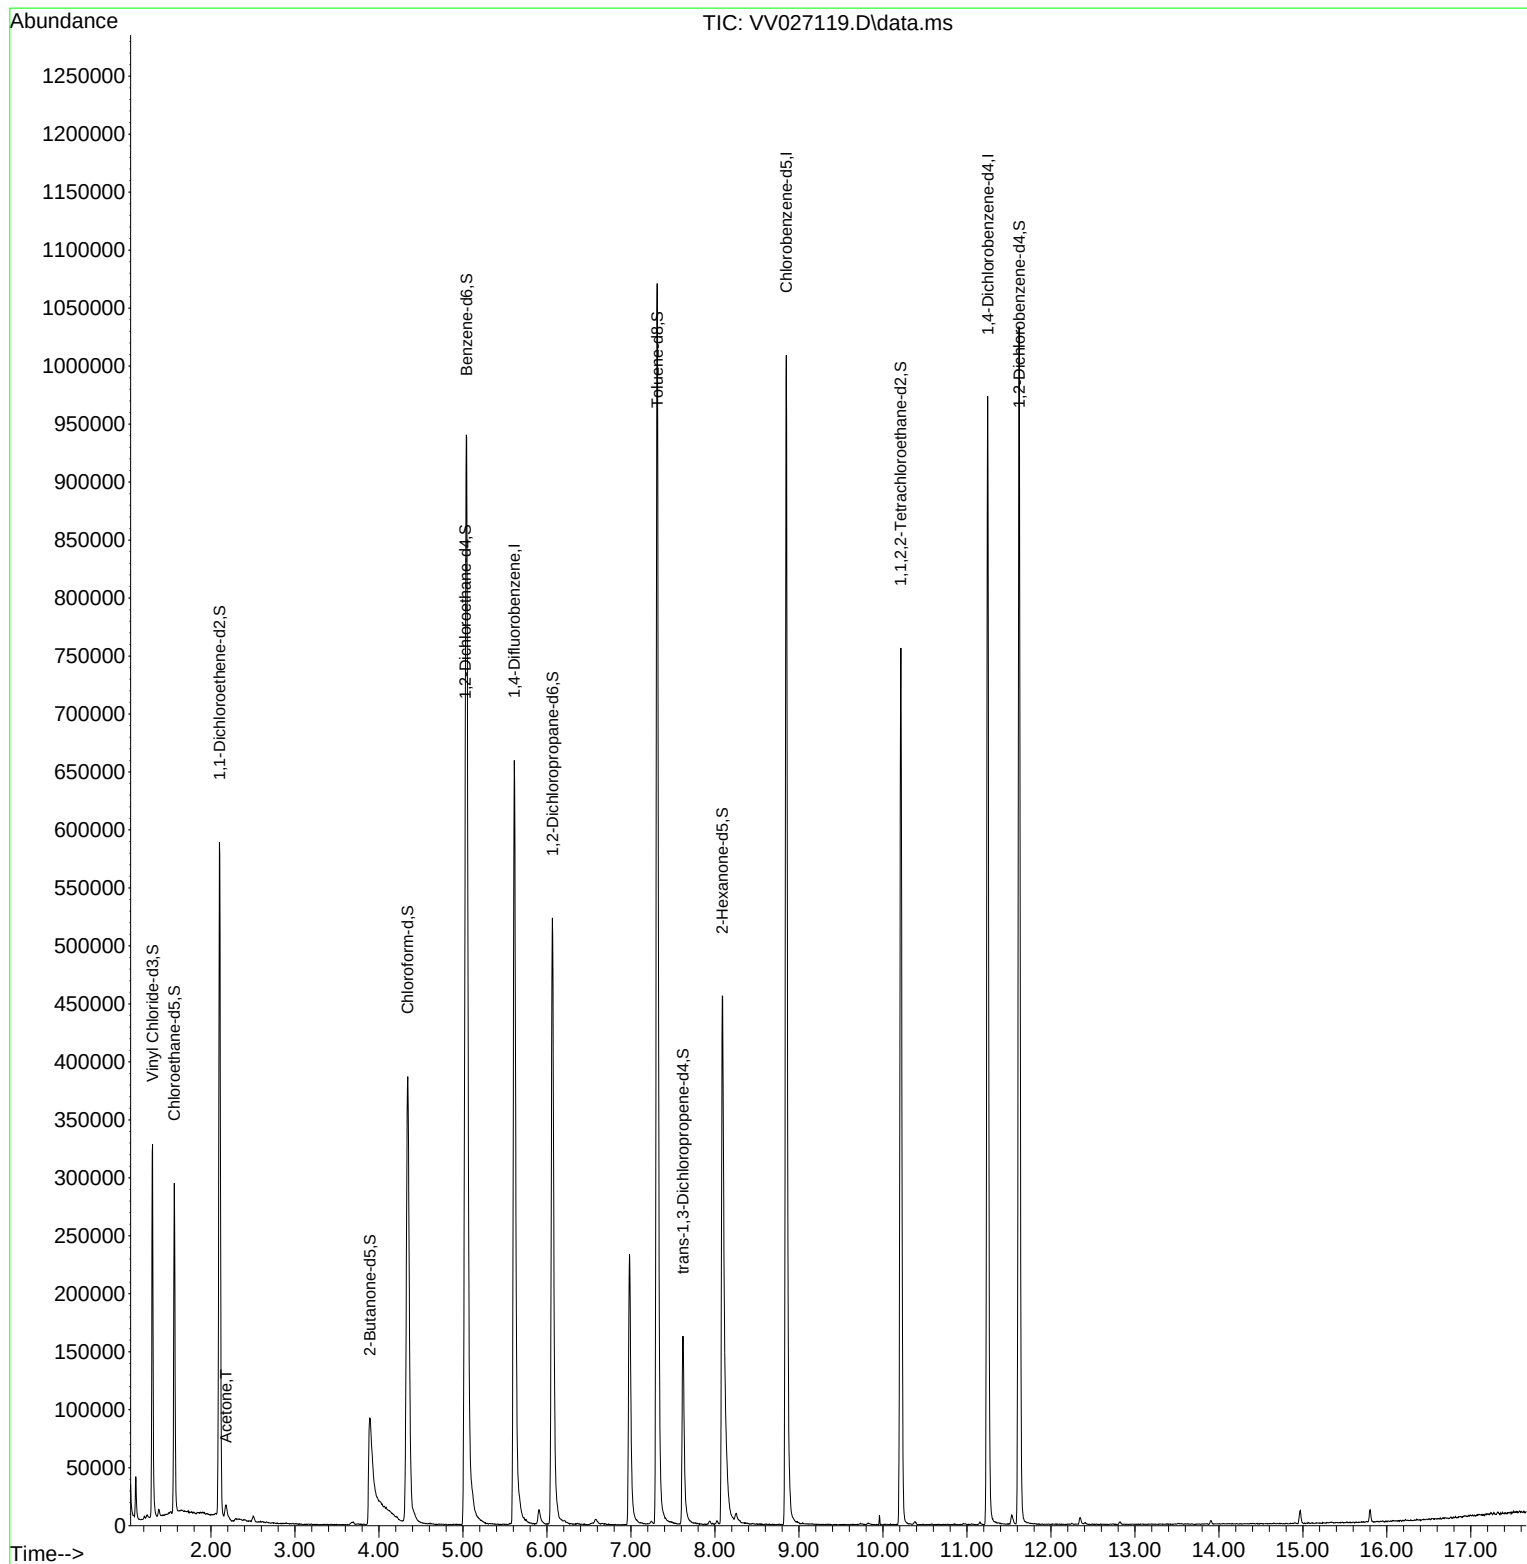

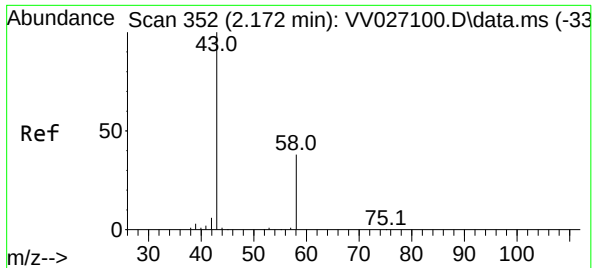

#13
 Acetone
 Concen: 4.278 ug/L
 RT: 2.179 min Scan# 31
 Delta R.T. 0.007 min
 Lab File: VV027119.D
 Acq: 30 Jul 2022 05:59

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUS3

Tgt Ion: 43 Resp: 10443
 Ion Ratio Lower Upper
 43 100
 58 28.0 0.0 49.6

