

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
 Data File : VV027076.D
 Acq On : 29 Jul 2022 11:37
 Operator : SY/MD
 Sample : VV0729WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK241

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
 Title : VOC Analysis

Signal : TIC: VV027076.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	98	rBV	371243	394212	14.61%	2.132%
2	1.564	156	163	179	rVB	325985	373941	13.86%	2.023%
3	2.101	321	330	345	rBV	664100	943736	34.98%	5.105%
4	2.863	566	567	568	rBV	430	116	0.00%	0.001%
5	2.902	575	579	582	rBV3	453	416	0.02%	0.002%
6	3.085	632	636	637	rBV	399	245	0.01%	0.001%
7	3.223	677	679	680	rBV	305	132	0.00%	0.001%
8	3.391	727	731	736	rBV2	498	492	0.02%	0.003%
9	3.416	736	739	743	rBV2	214	232	0.01%	0.001%
10	3.510	765	768	770	rVB	362	201	0.01%	0.001%
11	3.526	770	773	777	rBV2	405	254	0.01%	0.001%
12	3.548	777	780	781	rBV	287	177	0.01%	0.001%
13	3.587	789	792	798	rBV2	506	671	0.02%	0.004%
14	3.635	805	807	811	rBV	320	283	0.01%	0.002%
15	3.674	816	819	820	rBV	259	131	0.00%	0.001%
16	3.722	828	834	837	rBV2	352	427	0.02%	0.002%
17	3.760	840	846	847	rBV2	289	311	0.01%	0.002%
18	3.793	854	856	859	rBV2	166	82	0.00%	0.000%
19	3.886	874	885	927	rBV2	114690	496456	18.40%	2.685%
20	4.342	1012	1027	1068	rVB	432972	1070935	39.69%	5.793%
21	4.754	1152	1155	1156	rBV2	290	172	0.01%	0.001%
22	4.818	1171	1175	1179	rBV3	486	394	0.01%	0.002%
23	4.847	1183	1184	1185	rBV3	239	67	0.00%	0.000%
24	4.931	1207	1210	1212	rBV2	363	218	0.01%	0.001%
25	5.040	1223	1244	1289	rBV2	1027609	2698239	100.00%	14.595%
26	5.394	1351	1354	1355	rBV2	998	520	0.02%	0.003%
27	5.545	1398	1401	1404	rBV4	473	237	0.01%	0.001%
28	5.612	1410	1422	1461	rBV	569654	1200272	44.48%	6.493%
29	5.905	1502	1513	1538	rBV2	20785	46610	1.73%	0.252%
30	6.066	1549	1563	1598	rBV	579618	1221880	45.28%	6.609%
31	6.352	1648	1652	1655	rBV4	839	767	0.03%	0.004%
32	6.390	1660	1664	1665	rBV3	556	422	0.02%	0.002%
33	6.452	1681	1683	1687	rVB	427	232	0.01%	0.001%
34	6.474	1687	1690	1693	rBV2	658	382	0.01%	0.002%
35	6.513	1697	1702	1706	rVB5	494	578	0.02%	0.003%
36	6.532	1706	1708	1710	rBV2	533	370	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
 Data File : VV027076.D
 Acq On : 29 Jul 2022 11:37
 Operator : SY/MD
 Sample : VV0729WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK241

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
 Title : VOC Analysis

37	6.554	1713	1715	1717	rVB	276	128	0.00%	0.001%
38	6.580	1721	1723	1725	rVB	239	100	0.00%	0.001%
39	6.593	1725	1727	1730	rBV2	214	119	0.00%	0.001%
40	6.609	1730	1732	1736	rVB3	426	323	0.01%	0.002%
41	6.651	1736	1745	1748	rBV6	1245	1696	0.06%	0.009%
42	6.699	1759	1760	1764	rVB2	661	306	0.01%	0.002%
43	6.760	1775	1779	1784	rVB3	531	559	0.02%	0.003%
44	6.792	1787	1789	1792	rVB2	249	120	0.00%	0.001%
45	6.812	1792	1795	1799	rBV3	331	277	0.01%	0.001%
46	6.834	1800	1802	1803	rBV	255	72	0.00%	0.000%
47	6.889	1818	1819	1820	rBV	134	30	0.00%	0.000%
48	6.899	1820	1822	1826	rVB2	395	224	0.01%	0.001%
49	6.918	1826	1828	1830	rBV	145	82	0.00%	0.000%
50	6.982	1836	1848	1885	rBV	265732	517845	19.19%	2.801%
51	7.313	1938	1951	1986	rBV	1178955	2055962	76.20%	11.121%
52	7.619	2036	2046	2075	rBV	190159	354508	13.14%	1.918%
53	7.828	2108	2111	2114	rBV3	652	458	0.02%	0.002%
54	7.908	2134	2136	2139	rBV2	516	370	0.01%	0.002%
55	7.979	2152	2158	2166	rVB6	1658	2048	0.08%	0.011%
56	8.091	2181	2193	2230	rBV	512371	1213499	44.97%	6.564%
57	8.500	2319	2320	2321	rBV	463	164	0.01%	0.001%
58	8.590	2346	2348	2350	rBV	413	264	0.01%	0.001%
59	8.850	2417	2429	2457	rBV	906489	1505780	55.81%	8.145%
60	9.368	2588	2590	2593	rBV2	283	142	0.01%	0.001%
61	9.490	2626	2628	2632	rVB2	485	307	0.01%	0.002%
62	9.509	2632	2634	2639	rVB3	248	168	0.01%	0.001%
63	9.548	2639	2646	2649	rBV3	481	586	0.02%	0.003%
64	9.583	2656	2657	2658	rBV3	268	66	0.00%	0.000%
65	9.612	2664	2666	2668	rBV	265	162	0.01%	0.001%
66	9.728	2699	2702	2703	rBV	270	127	0.00%	0.001%
67	9.738	2703	2705	2707	rVV	197	96	0.00%	0.001%
68	9.783	2716	2719	2721	rBV2	406	243	0.01%	0.001%
69	9.815	2725	2729	2732	rBV3	251	212	0.01%	0.001%
70	9.844	2736	2738	2741	rBV2	355	171	0.01%	0.001%
71	9.869	2745	2746	2747	rVB	356	70	0.00%	0.000%
72	9.931	2761	2765	2766	rBV2	547	323	0.01%	0.002%
73	9.966	2774	2776	2778	rBV2	419	122	0.00%	0.001%
74	10.001	2781	2787	2792	rBV2	338	517	0.02%	0.003%
75	10.062	2803	2806	2809	rBV3	310	218	0.01%	0.001%
76	10.130	2824	2827	2831	rBV2	248	250	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
 Data File : VV072076.D
 Acq On : 29 Jul 2022 11:37
 Operator : SY/MD
 Sample : VV0729WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK241

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M

Title : VOC Analysis

77	10.213	2840	2853	2885	rBV	858931	1361536	50.46%	7.365%
78	10.545	2954	2956	2958	rBV2	370	220	0.01%	0.001%
79	10.577	2963	2966	2970	rBV4	659	526	0.02%	0.003%
80	10.644	2985	2987	2991	rBV2	276	171	0.01%	0.001%
81	10.725	3010	3012	3013	rBV	336	133	0.00%	0.001%
82	10.779	3026	3029	3030	rBV2	185	94	0.00%	0.001%
83	10.857	3049	3053	3060	rVB3	843	672	0.02%	0.004%
84	10.927	3071	3075	3083	rVB3	646	711	0.03%	0.004%
85	10.966	3083	3087	3091	rVB2	445	349	0.01%	0.002%
86	10.988	3091	3094	3096	rBV2	412	279	0.01%	0.002%
87	11.249	3163	3175	3200	rBV	815801	1293635	47.94%	6.998%
88	11.622	3279	3291	3315	rBV	1081681	1704979	63.19%	9.223%
89	12.053	3424	3425	3426	rVB	555	107	0.00%	0.001%
90	12.554	3579	3581	3584	rVB	460	137	0.01%	0.001%
91	12.799	3654	3657	3663	rBV2	482	437	0.02%	0.002%
92	13.271	3797	3804	3810	rVB5	1667	2218	0.08%	0.012%
93	13.509	3872	3878	3887	rVB2	4591	6781	0.25%	0.037%
94	13.882	3991	3994	3998	rBV2	710	479	0.02%	0.003%




Sum of corrected areas: 18486988

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
Data File : VV027076.D
Acq On : 29 Jul 2022 11:37
Operator : SY/MD
Sample : VV0729WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK241

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

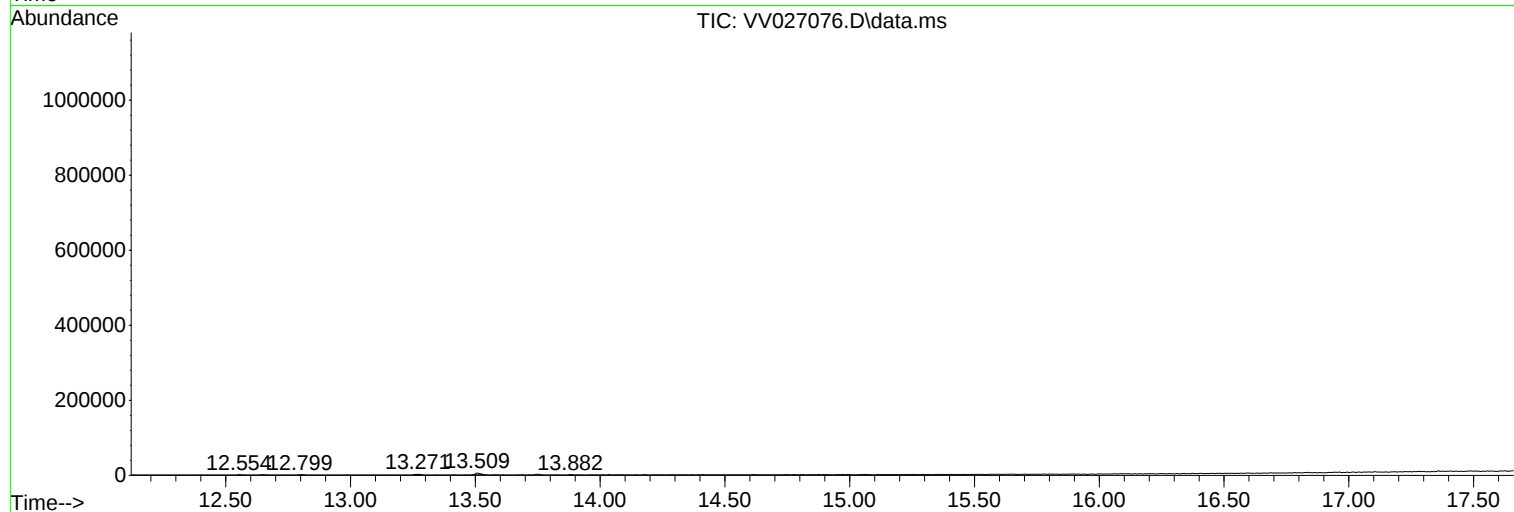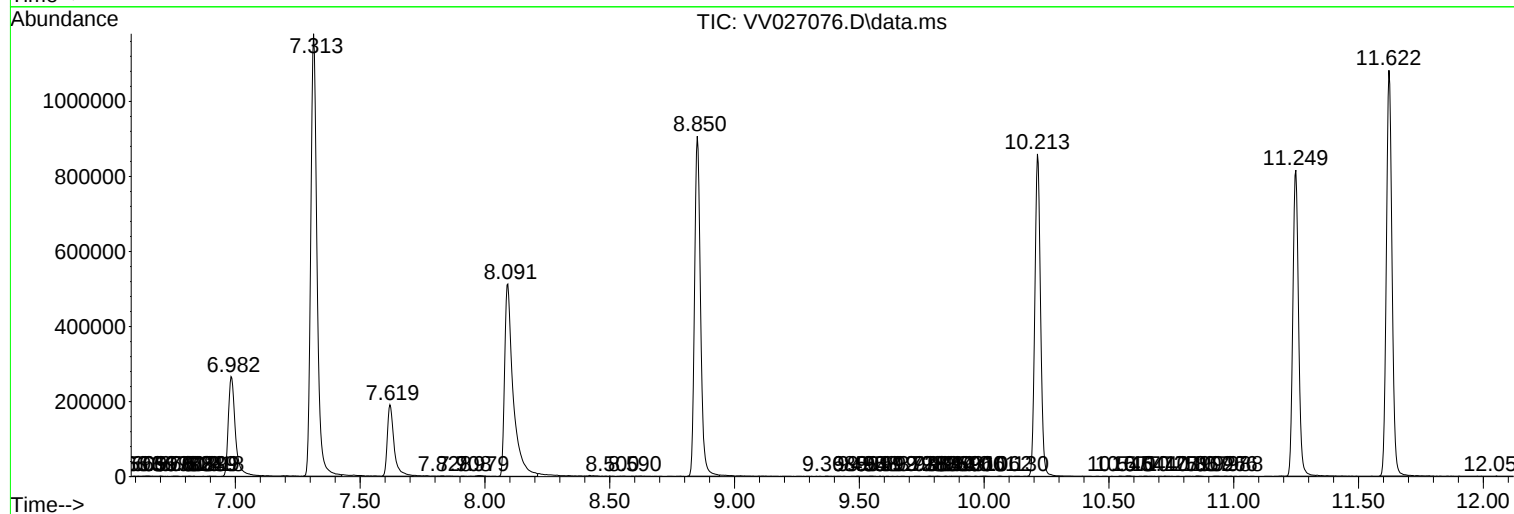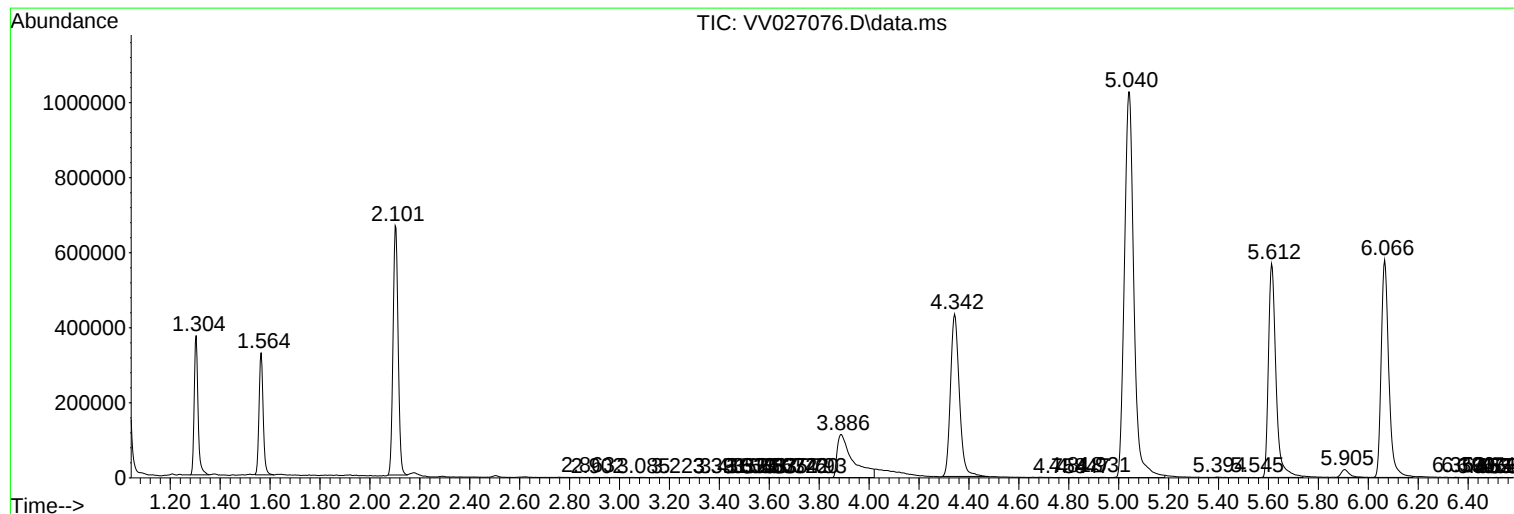

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
Data File : VV027076.D
Acq On : 29 Jul 2022 11:37
Operator : SY/MD
Sample : VV0729WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK241

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
Data File : VV027076.D
Acq On : 29 Jul 2022 11:37
Operator : SY/MD
Sample : VV0729WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK241

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc