

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
 Data File : VV027078.D
 Acq On : 29 Jul 2022 12:26
 Operator : SY/MD
 Sample : N3821-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXEZ9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M

Title : VOC Analysis

Signal : TIC: VV027078.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	74	81	103	rVB	351449	372830	15.25%	2.196%
2	1.564	155	163	174	rBV	293646	336629	13.77%	1.983%
3	2.101	319	330	346	rBV	632054	895589	36.64%	5.275%
4	2.433	431	433	438	rVB2	741	523	0.02%	0.003%
5	2.500	447	454	464	rVV4	5976	9062	0.37%	0.053%
6	2.558	469	472	476	rVB2	464	334	0.01%	0.002%
7	2.764	533	536	538	rVB2	637	293	0.01%	0.002%
8	2.941	585	591	594	rBV2	319	304	0.01%	0.002%
9	3.127	646	649	656	rBV2	292	349	0.01%	0.002%
10	3.172	658	663	666	rBV3	493	355	0.01%	0.002%
11	3.227	677	680	685	rVB	403	335	0.01%	0.002%
12	3.288	694	699	704	rVB3	274	329	0.01%	0.002%
13	3.384	725	729	732	rBV2	449	314	0.01%	0.002%
14	3.474	753	757	761	rBV3	306	302	0.01%	0.002%
15	3.532	772	775	782	rVB2	390	454	0.02%	0.003%
16	3.622	800	803	808	rVB2	313	258	0.01%	0.002%
17	3.802	855	859	862	rBV2	429	342	0.01%	0.002%
18	3.896	877	888	936	rBV	85816	404249	16.54%	2.381%
19	4.342	1011	1027	1049	rBV2	391437	981660	40.16%	5.782%
20	4.809	1167	1172	1175	rBV3	505	511	0.02%	0.003%
21	4.889	1194	1197	1202	rVB2	588	485	0.02%	0.003%
22	5.043	1227	1245	1294	rBV2	928599	2444378	100.00%	14.396%
23	5.288	1319	1321	1325	rVB4	645	391	0.02%	0.002%
24	5.487	1380	1383	1384	rBV2	518	272	0.01%	0.002%
25	5.516	1390	1392	1397	rVB3	617	359	0.01%	0.002%
26	5.612	1406	1422	1459	rBV	560032	1179667	48.26%	6.948%
27	5.815	1484	1485	1488	rVB3	1279	348	0.01%	0.002%
28	5.905	1503	1513	1528	rBV3	22142	47999	1.96%	0.283%
29	6.066	1548	1563	1605	rBV	523439	1103525	45.15%	6.499%
30	6.294	1632	1634	1639	rVB3	495	309	0.01%	0.002%
31	6.339	1643	1648	1651	rBV3	567	575	0.02%	0.003%
32	6.355	1651	1653	1657	rVB2	692	501	0.02%	0.003%
33	6.403	1663	1668	1674	rVB4	541	704	0.03%	0.004%
34	6.439	1674	1679	1682	rBV4	556	526	0.02%	0.003%
35	6.503	1696	1699	1702	rBV2	357	286	0.01%	0.002%
36	6.564	1715	1718	1722	rVB3	658	398	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
 Data File : VV027078.D
 Acq On : 29 Jul 2022 12:26
 Operator : SY/MD
 Sample : N3821-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXEZ9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
 Title : VOC Analysis

37	6.638	1736	1741	1745	rBV3	652	827	0.03%	0.005%
38	6.657	1745	1747	1750	rVB2	513	309	0.01%	0.002%
39	6.796	1786	1790	1794	rBV	452	441	0.02%	0.003%
40	6.821	1794	1798	1801	rVB2	378	275	0.01%	0.002%
41	6.870	1807	1813	1817	rBV4	288	319	0.01%	0.002%
42	6.982	1837	1848	1884	rBV	239491	468255	19.16%	2.758%
43	7.201	1913	1916	1917	rBV4	476	276	0.01%	0.002%
44	7.313	1939	1951	1989	rBV	1035508	1864616	76.28%	10.982%
45	7.619	2036	2046	2071	rBV	173504	317656	13.00%	1.871%
46	7.834	2111	2113	2117	rVB2	843	573	0.02%	0.003%
47	7.866	2120	2123	2127	rBV4	328	264	0.01%	0.002%
48	7.908	2131	2136	2139	rVB4	705	664	0.03%	0.004%
49	7.979	2152	2158	2160	rBV5	1130	1248	0.05%	0.007%
50	8.091	2182	2193	2236	rBV	438646	1038648	42.49%	6.117%
51	8.477	2310	2313	2314	rBV	564	283	0.01%	0.002%
52	8.545	2332	2334	2340	rVB2	440	407	0.02%	0.002%
53	8.850	2414	2429	2457	rBV	896022	1479694	60.53%	8.715%
54	9.053	2490	2492	2494	rBV2	599	354	0.01%	0.002%
55	9.162	2524	2526	2529	rVB2	710	327	0.01%	0.002%
56	9.223	2543	2545	2550	rBB3	562	403	0.02%	0.002%
57	9.307	2569	2571	2576	rVB3	536	367	0.02%	0.002%
58	9.484	2622	2626	2629	rVB3	533	460	0.02%	0.003%
59	9.500	2629	2631	2636	rVB2	381	285	0.01%	0.002%
60	9.529	2636	2640	2644	rBV2	386	440	0.02%	0.003%
61	9.741	2704	2706	2711	rVB2	527	334	0.01%	0.002%
62	9.773	2711	2716	2719	rBV2	520	451	0.02%	0.003%
63	9.940	2765	2768	2771	rVV2	450	315	0.01%	0.002%
64	9.989	2780	2783	2787	rVB3	356	323	0.01%	0.002%
65	10.214	2835	2853	2875	rBV	740424	1187175	48.57%	6.992%
66	10.313	2882	2884	2890	rVB4	786	561	0.02%	0.003%
67	10.426	2917	2919	2923	rBV2	344	297	0.01%	0.002%
68	10.638	2982	2985	2993	rVB3	425	487	0.02%	0.003%
69	10.680	2993	2998	3000	rBV3	459	453	0.02%	0.003%
70	10.850	3049	3051	3056	rVV2	330	275	0.01%	0.002%
71	10.902	3063	3067	3072	rVB3	303	310	0.01%	0.002%
72	10.937	3072	3078	3081	rBV2	466	492	0.02%	0.003%
73	11.120	3128	3135	3137	rBV	536	651	0.03%	0.004%
74	11.165	3145	3149	3152	rVB3	464	378	0.02%	0.002%
75	11.191	3154	3157	3163	rBV4	934	881	0.04%	0.005%
76	11.249	3163	3175	3204	rBV	820575	1268850	51.91%	7.473%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
 Data File : VV027078.D
 Acq On : 29 Jul 2022 12:26
 Operator : SY/MD
 Sample : N3821-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXEZ9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
 Title : VOC Analysis

77	11.538	3253	3265	3275	rBV4	7415	14662	0.60%	0.086%
78	11.622	3279	3291	3312	rBV	977370	1522139	62.27%	8.965%
79	11.796	3342	3345	3349	rBV3	726	673	0.03%	0.004%
80	11.850	3360	3362	3369	rVB2	543	533	0.02%	0.003%
81	11.886	3369	3373	3377	rBV4	593	598	0.02%	0.004%
82	12.030	3415	3418	3421	rBV2	452	300	0.01%	0.002%
83	12.069	3426	3430	3432	rBV2	407	290	0.01%	0.002%
84	12.291	3497	3499	3504	rVB2	531	353	0.01%	0.002%
85	12.355	3513	3519	3524	rBV5	1973	2288	0.09%	0.013%
86	12.487	3557	3560	3564	rBV	443	365	0.01%	0.002%
87	12.651	3604	3611	3617	rBV7	822	1032	0.04%	0.006%
88	12.943	3695	3702	3704	rBV4	532	683	0.03%	0.004%
89	13.265	3799	3802	3803	rBV2	654	431	0.02%	0.003%
90	13.522	3876	3882	3883	rBV3	740	698	0.03%	0.004%
91	13.686	3930	3933	3937	rBV4	551	438	0.02%	0.003%
92	13.728	3941	3946	3948	rBV2	594	557	0.02%	0.003%
93	13.750	3950	3953	3955	rBV3	569	454	0.02%	0.003%
94	14.580	4205	4211	4215	rBV2	700	1019	0.04%	0.006%
95	14.660	4234	4236	4240	rBV3	509	375	0.02%	0.002%
96	14.683	4240	4243	4246	rBV3	487	467	0.02%	0.003%
97	14.950	4323	4326	4329	rBV2	659	459	0.02%	0.003%
98	15.229	4411	4413	4415	rBV3	646	424	0.02%	0.002%
99	15.246	4415	4418	4423	rVB	7064	3927	0.16%	0.023%
100	15.271	4423	4426	4429	rBV	816	514	0.02%	0.003%




Sum of corrected areas: 16979048

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
Data File : VV027078.D
Acq On : 29 Jul 2022 12:26
Operator : SY/MD
Sample : N3821-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXEZ9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

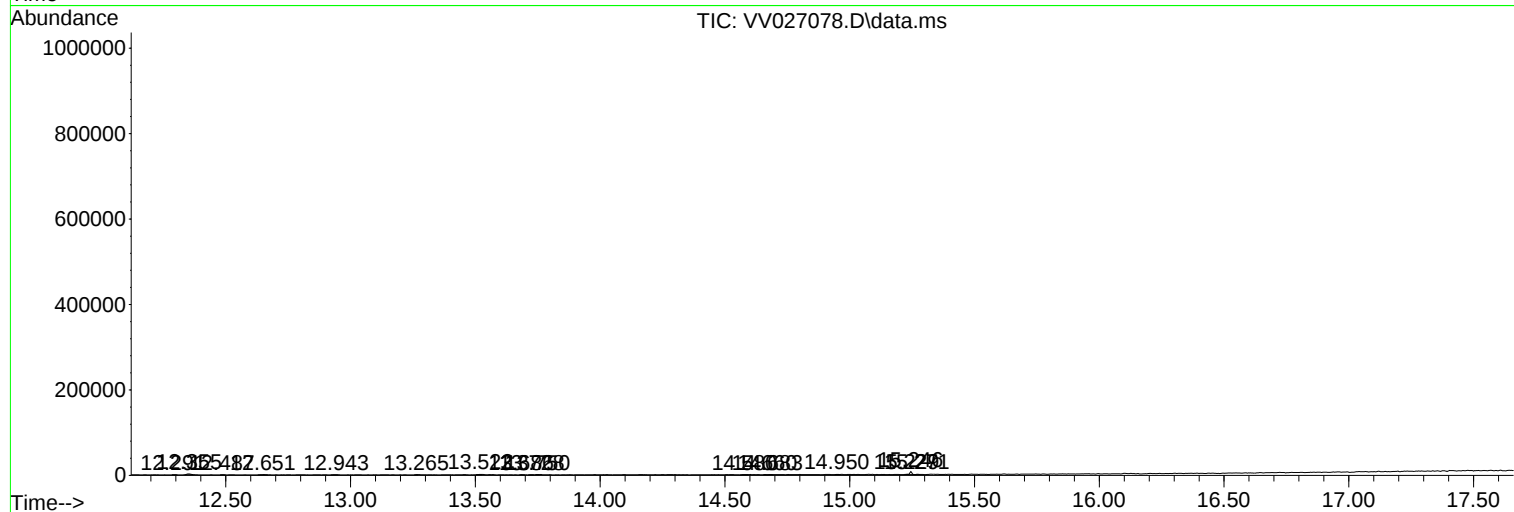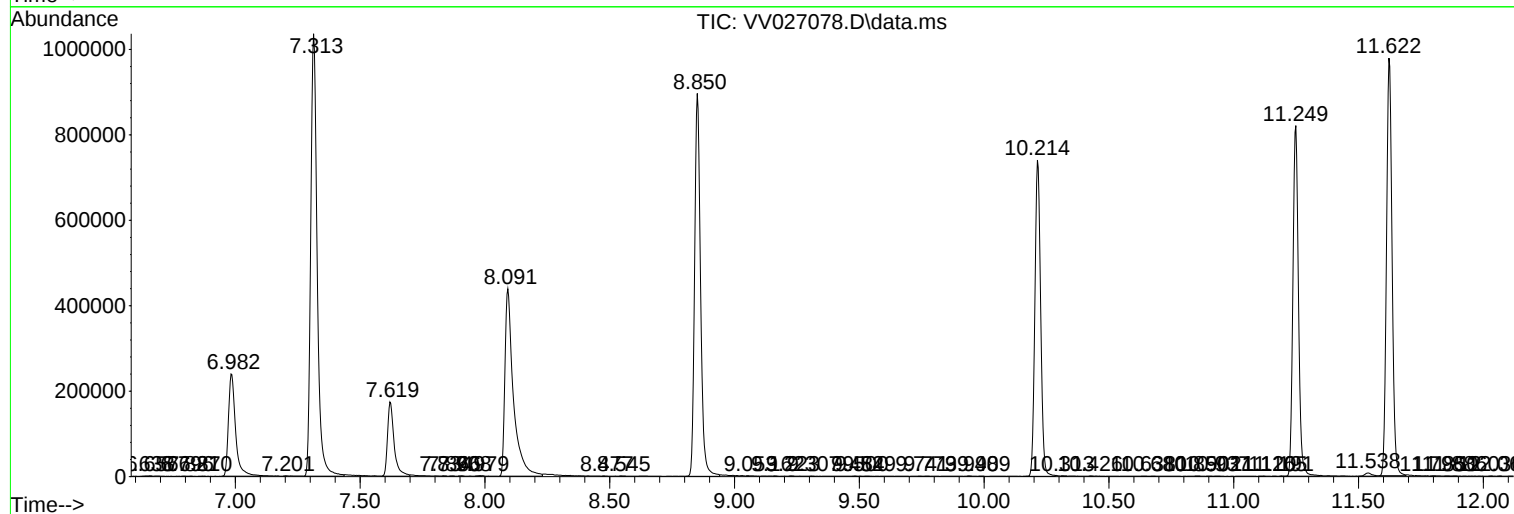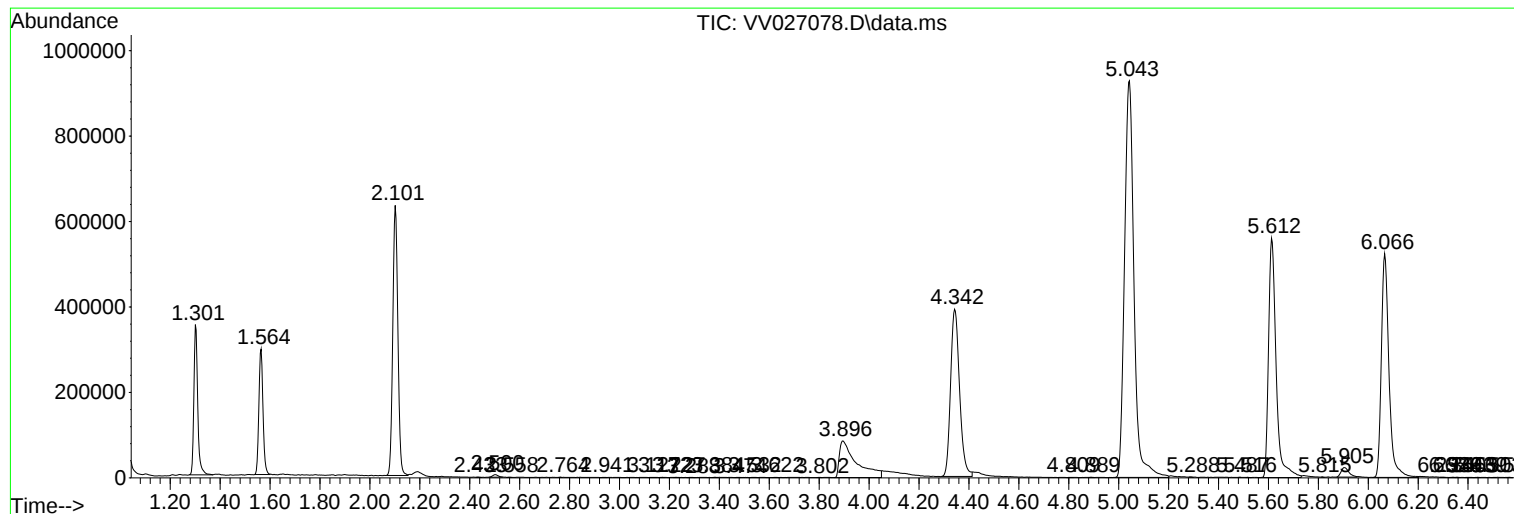

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
Data File : VV027078.D
Acq On : 29 Jul 2022 12:26
Operator : SY/MD
Sample : N3821-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXEZ9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
Data File : VV027078.D
Acq On : 29 Jul 2022 12:26
Operator : SY/MD
Sample : N3821-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXEZ9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc