

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
 Data File : VV027079.D
 Acq On : 29 Jul 2022 12:50
 Operator : SY/MD
 Sample : N3820-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M

Title : VOC Analysis

Signal : TIC: VV027079.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	74	81	99	rVB	352801	380434	14.51%	2.071%
2	1.564	155	163	180	rVB	312936	359209	13.70%	1.955%
3	2.101	319	330	346	rBV	646582	918664	35.03%	5.001%
4	2.500	448	454	465	rVB3	5807	9563	0.36%	0.052%
5	2.770	534	538	540	rVV2	595	373	0.01%	0.002%
6	2.822	549	554	556	rBV2	457	400	0.02%	0.002%
7	2.908	576	581	583	rBV2	373	280	0.01%	0.002%
8	2.992	605	607	611	rVV	621	444	0.02%	0.002%
9	3.037	618	621	623	rVV2	502	296	0.01%	0.002%
10	3.143	649	654	658	rBV2	317	423	0.02%	0.002%
11	3.320	705	709	715	rBV2	410	424	0.02%	0.002%
12	3.381	724	728	732	rVB2	325	294	0.01%	0.002%
13	3.539	774	777	781	rBV2	295	323	0.01%	0.002%
14	3.561	781	784	788	rVB2	373	274	0.01%	0.001%
15	3.629	801	805	806	rBV3	378	290	0.01%	0.002%
16	3.715	827	832	836	rVB3	414	406	0.02%	0.002%
17	3.764	841	847	850	rBV	330	307	0.01%	0.002%
18	3.892	876	887	928	rBV2	116622	528831	20.16%	2.879%
19	4.342	1011	1027	1054	rBV	417948	1039356	39.63%	5.658%
20	4.658	1120	1125	1126	rBV3	742	695	0.03%	0.004%
21	4.963	1215	1220	1223	rBV2	264	261	0.01%	0.001%
22	5.040	1227	1244	1296	rBV2	999728	2622659	100.00%	14.277%
23	5.259	1310	1312	1313	rBV3	1191	479	0.02%	0.003%
24	5.400	1352	1356	1358	rBV2	622	496	0.02%	0.003%
25	5.471	1374	1378	1380	rBV2	715	550	0.02%	0.003%
26	5.612	1410	1422	1461	rBV	596629	1258545	47.99%	6.851%
27	5.834	1488	1491	1492	rBV2	527	273	0.01%	0.001%
28	5.905	1502	1513	1530	rBV2	18469	40216	1.53%	0.219%
29	6.011	1543	1546	1548	rBV	573	289	0.01%	0.002%
30	6.066	1548	1563	1602	rBV	571637	1198408	45.69%	6.524%
31	6.336	1643	1647	1651	rBV4	486	428	0.02%	0.002%
32	6.648	1735	1744	1746	rBV4	811	998	0.04%	0.005%
33	6.699	1756	1760	1762	rBV3	322	262	0.01%	0.001%
34	6.764	1777	1780	1784	rVB2	367	257	0.01%	0.001%
35	6.944	1828	1836	1838	rBV2	554	539	0.02%	0.003%
36	6.982	1838	1848	1884	rBV	254617	499063	19.03%	2.717%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
 Data File : VV027079.D
 Acq On : 29 Jul 2022 12:50
 Operator : SY/MD
 Sample : N3820-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
 Title : VOC Analysis

37	7.204	1912	1917	1922	rVV6	746	867	0.03%	0.005%
38	7.313	1938	1951	1978	rBV	1110270	1967406	75.02%	10.710%
39	7.619	2036	2046	2084	rBV	187465	350845	13.38%	1.910%
40	7.751	2085	2087	2089	rVB2	744	297	0.01%	0.002%
41	7.863	2120	2122	2128	rVB5	733	540	0.02%	0.003%
42	7.976	2147	2157	2159	rBV8	1003	1307	0.05%	0.007%
43	8.030	2172	2174	2179	rVB3	516	325	0.01%	0.002%
44	8.091	2182	2193	2244	rBV	521875	1200231	45.76%	6.534%
45	8.355	2272	2275	2277	rBV2	679	435	0.02%	0.002%
46	8.426	2290	2297	2302	rVB10	1877	2579	0.10%	0.014%
47	8.493	2314	2318	2321	rBV4	1143	806	0.03%	0.004%
48	8.516	2322	2325	2330	rVB2	705	523	0.02%	0.003%
49	8.542	2330	2333	2336	rBV	374	278	0.01%	0.002%
50	8.622	2355	2358	2364	rVB4	475	405	0.02%	0.002%
51	8.693	2374	2380	2382	rBV3	291	260	0.01%	0.001%
52	8.850	2417	2429	2458	rBV	959198	1575144	60.06%	8.575%
53	9.127	2513	2515	2519	rVB2	551	398	0.02%	0.002%
54	9.156	2519	2524	2527	rVB4	776	673	0.03%	0.004%
55	9.178	2527	2531	2532	rBV3	413	262	0.01%	0.001%
56	9.194	2534	2536	2543	rVB3	566	544	0.02%	0.003%
57	9.226	2543	2546	2550	rBV2	427	315	0.01%	0.002%
58	9.558	2647	2649	2654	rVB4	350	257	0.01%	0.001%
59	9.837	2731	2736	2737	rBV2	352	275	0.01%	0.001%
60	9.892	2748	2753	2756	rBV2	387	346	0.01%	0.002%
61	9.927	2760	2764	2767	rBV3	388	307	0.01%	0.002%
62	10.001	2784	2787	2796	rVB2	257	357	0.01%	0.002%
63	10.214	2841	2853	2876	rBV	846737	1346205	51.33%	7.328%
64	10.371	2899	2902	2906	rBV2	694	517	0.02%	0.003%
65	10.471	2928	2933	2935	rBV	391	269	0.01%	0.001%
66	10.538	2948	2954	2958	rBV3	373	431	0.02%	0.002%
67	10.702	3001	3005	3008	rBV2	364	311	0.01%	0.002%
68	10.824	3039	3043	3046	rBV	464	336	0.01%	0.002%
69	10.853	3046	3052	3055	rVV3	762	670	0.03%	0.004%
70	10.924	3071	3074	3081	rVB3	508	576	0.02%	0.003%
71	10.959	3081	3085	3089	rBV2	392	372	0.01%	0.002%
72	11.040	3105	3110	3114	rBV3	329	382	0.01%	0.002%
73	11.098	3123	3128	3134	rBV3	367	528	0.02%	0.003%
74	11.249	3163	3175	3198	rBV	874222	1364922	52.04%	7.430%
75	11.622	3278	3291	3313	rBV	1069625	1673162	63.80%	9.108%
76	11.828	3353	3355	3358	rVB2	762	283	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
 Data File : VV027079.D
 Acq On : 29 Jul 2022 12:50
 Operator : SY/MD
 Sample : N3820-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
 Title : VOC Analysis

77	11.844	3358	3360	3361	rBV	1091	371	0.01%	0.002%
78	12.004	3406	3410	3414	rBV3	420	454	0.02%	0.002%
79	12.255	3485	3488	3493	rBV2	458	372	0.01%	0.002%
80	12.631	3601	3605	3607	rBV	380	297	0.01%	0.002%
81	12.657	3607	3613	3614	rVV5	450	425	0.02%	0.002%
82	12.725	3630	3634	3638	rBV2	351	346	0.01%	0.002%
83	12.908	3687	3691	3693	rBV2	318	270	0.01%	0.001%
84	12.950	3701	3704	3707	rVB3	474	319	0.01%	0.002%
85	13.066	3737	3740	3743	rBV2	466	296	0.01%	0.002%
86	13.085	3743	3746	3749	rBV2	484	342	0.01%	0.002%
87	13.143	3758	3764	3767	rBV4	608	538	0.02%	0.003%
88	13.242	3793	3795	3799	rVB3	492	281	0.01%	0.002%
89	13.278	3801	3806	3810	rVB4	662	640	0.02%	0.003%
90	13.467	3860	3865	3867	rBV2	467	402	0.02%	0.002%
91	13.853	3980	3985	3989	rBV	538	651	0.02%	0.004%
92	13.892	3994	3997	4002	rBV4	498	510	0.02%	0.003%
93	13.963	4015	4019	4020	rBV	612	340	0.01%	0.002%
94	14.020	4034	4037	4040	rBV	456	373	0.01%	0.002%
95	14.037	4040	4042	4046	rVB	690	391	0.01%	0.002%
96	14.477	4176	4179	4181	rBV3	558	288	0.01%	0.002%
97	14.528	4193	4195	4199	rVB2	632	360	0.01%	0.002%
98	14.914	4310	4315	4319	rBV5	627	579	0.02%	0.003%
99	15.281	4426	4429	4432	rBV3	472	454	0.02%	0.002%
100	15.545	4509	4511	4516	rVB3	1168	671	0.03%	0.004%




Sum of corrected areas: 18369925

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
Data File : VV027079.D
Acq On : 29 Jul 2022 12:50
Operator : SY/MD
Sample : N3820-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

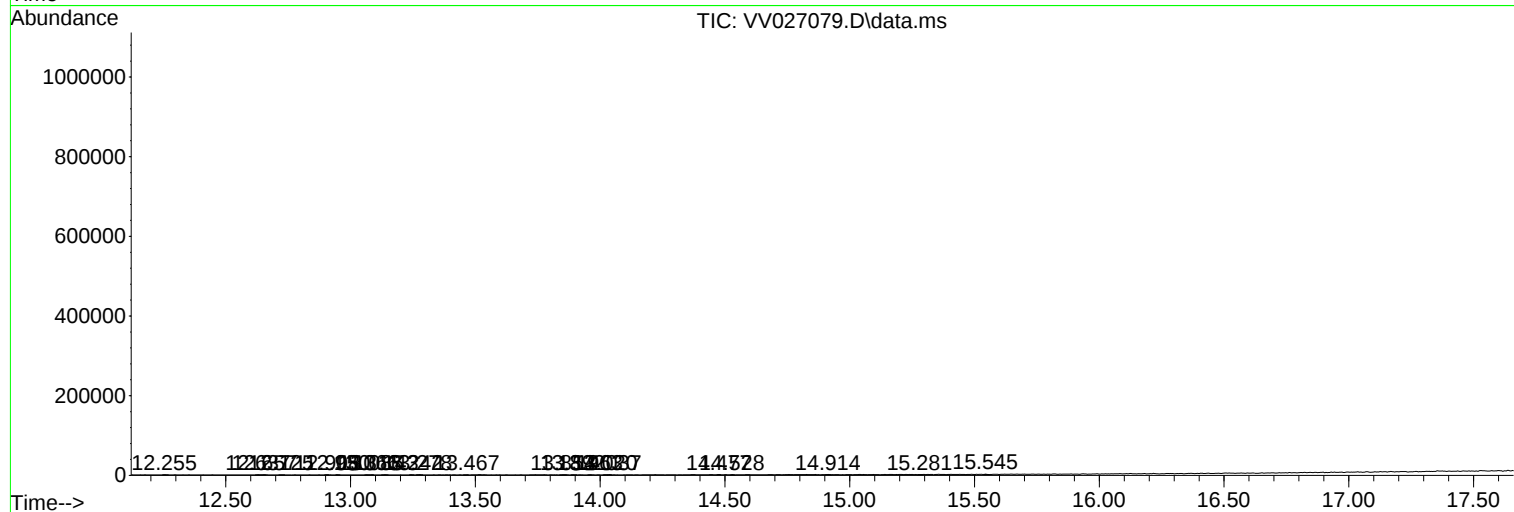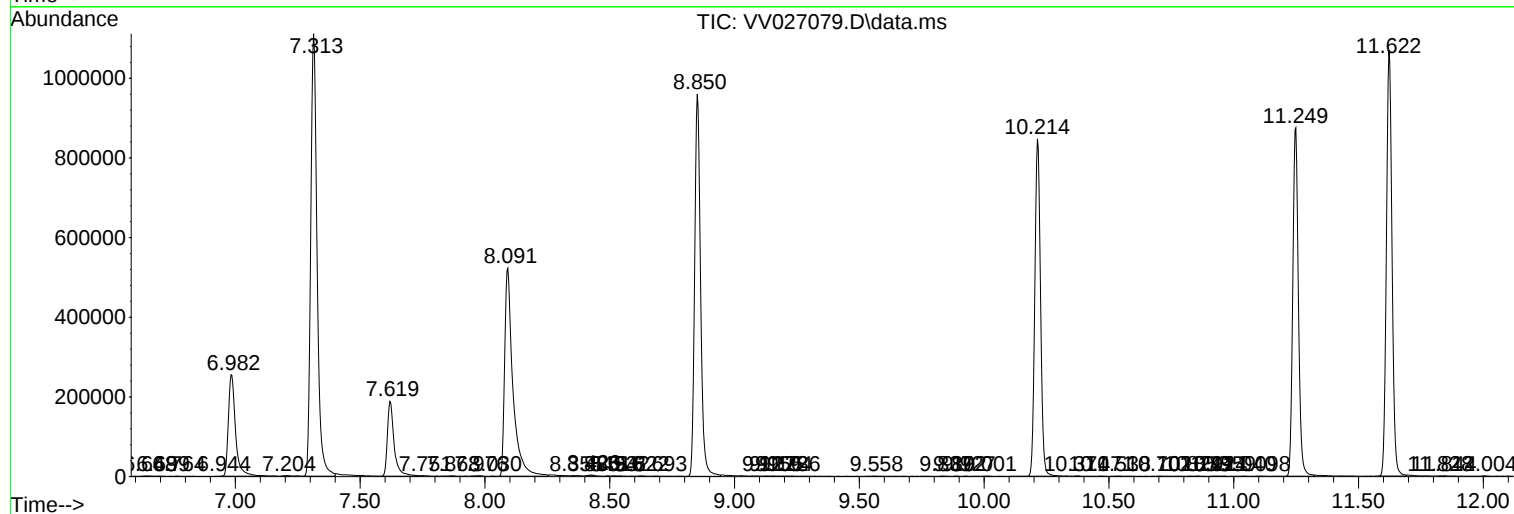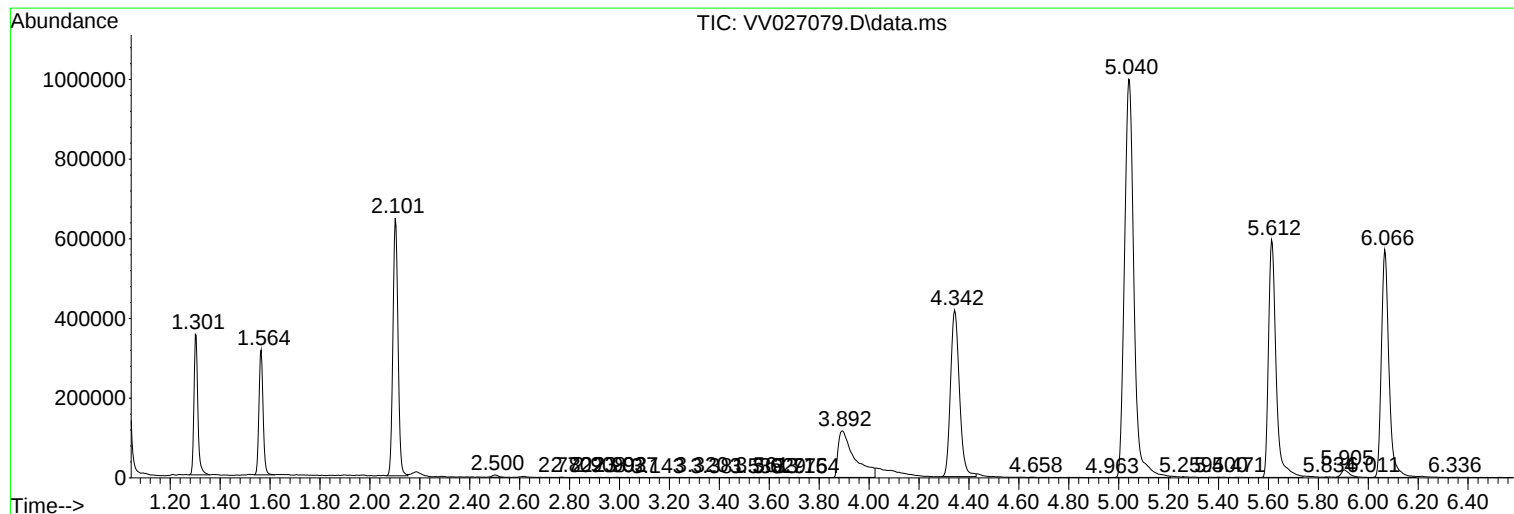

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
Data File : VV027079.D
Acq On : 29 Jul 2022 12:50
Operator : SY/MD
Sample : N3820-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
Data File : VV027079.D
Acq On : 29 Jul 2022 12:50
Operator : SY/MD
Sample : N3820-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc