

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
 Data File : VV027080.D
 Acq On : 29 Jul 2022 13:14
 Operator : SY/MD
 Sample : N3841-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
 Title : VOC Analysis

Signal : TIC: VV027080.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	74	81	100	rVB	354206	380524	14.43%	2.086%
2	1.564	155	163	181	rVB	314261	366011	13.88%	2.006%
3	2.101	320	330	346	rBV	649096	917394	34.79%	5.029%
4	2.281	383	386	390	rBV3	1306	1185	0.04%	0.006%
5	2.503	448	455	465	rVB3	6028	9205	0.35%	0.050%
6	2.571	474	476	479	rBV3	498	287	0.01%	0.002%
7	2.613	479	489	495	rBV4	2083	3864	0.15%	0.021%
8	2.661	502	504	511	rVB3	533	409	0.02%	0.002%
9	2.780	538	541	546	rVB3	440	432	0.02%	0.002%
10	3.024	615	617	621	rVV2	410	276	0.01%	0.002%
11	3.133	647	651	656	rBV3	228	295	0.01%	0.002%
12	3.162	657	660	666	rVB	347	317	0.01%	0.002%
13	3.410	732	737	743	rBV3	331	394	0.01%	0.002%
14	3.487	754	761	765	rBV2	468	604	0.02%	0.003%
15	3.593	788	794	795	rBV2	310	264	0.01%	0.001%
16	3.622	800	803	806	rBV	295	270	0.01%	0.001%
17	3.680	817	821	826	rVB2	350	258	0.01%	0.001%
18	3.709	826	830	834	rBV2	397	326	0.01%	0.002%
19	3.838	867	870	874	rBV	378	312	0.01%	0.002%
20	3.892	874	887	924	rBV2	116207	491852	18.65%	2.696%
21	4.342	1011	1027	1049	rBV	420244	1041007	39.48%	5.706%
22	4.564	1094	1096	1099	rBV3	565	251	0.01%	0.001%
23	4.596	1104	1106	1109	rVB3	859	459	0.02%	0.003%
24	4.709	1137	1141	1144	rBV2	323	292	0.01%	0.002%
25	4.741	1147	1151	1154	rBV3	570	429	0.02%	0.002%
26	4.963	1217	1220	1224	rBV3	337	298	0.01%	0.002%
27	5.043	1227	1245	1284	rBV2	1014171	2636914	100.00%	14.455%
28	5.284	1319	1320	1324	rVB3	955	503	0.02%	0.003%
29	5.397	1351	1355	1358	rBV2	590	450	0.02%	0.002%
30	5.410	1358	1359	1364	rVV2	565	433	0.02%	0.002%
31	5.490	1381	1384	1387	rBV2	390	309	0.01%	0.002%
32	5.612	1407	1422	1463	rBV	573549	1207641	45.80%	6.620%
33	5.863	1497	1500	1502	rBV4	741	451	0.02%	0.002%
34	5.908	1502	1514	1532	rVV3	18149	40268	1.53%	0.221%
35	6.066	1549	1563	1596	rBV	567718	1197957	45.43%	6.567%
36	6.278	1627	1629	1635	rVB4	722	634	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
 Data File : VV027080.D
 Acq On : 29 Jul 2022 13:14
 Operator : SY/MD
 Sample : N3841-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
 Title : VOC Analysis

37	6.378	1658	1660	1664	rBV3	374	251	0.01%	0.001%
38	6.632	1729	1739	1740	rBV2	632	715	0.03%	0.004%
39	6.680	1751	1754	1758	rVB3	595	450	0.02%	0.002%
40	6.821	1796	1798	1802	rVV4	386	323	0.01%	0.002%
41	6.847	1804	1806	1809	rVB	559	311	0.01%	0.002%
42	6.899	1818	1822	1825	rVB2	520	381	0.01%	0.002%
43	6.982	1835	1848	1871	rBV	263734	497505	18.87%	2.727%
44	7.255	1930	1933	1936	rVB3	736	392	0.01%	0.002%
45	7.313	1939	1951	1987	rBV	1108349	1987996	75.39%	10.897%
46	7.619	2035	2046	2078	rBV	188490	353186	13.39%	1.936%
47	7.982	2152	2159	2163	rBV6	1696	2206	0.08%	0.012%
48	8.091	2182	2193	2244	rBV	513907	1222983	46.38%	6.704%
49	8.403	2288	2290	2292	rBV3	860	486	0.02%	0.003%
50	8.506	2321	2322	2326	rVB2	396	253	0.01%	0.001%
51	8.593	2346	2349	2351	rVV2	393	300	0.01%	0.002%
52	8.615	2354	2356	2362	rVB2	486	412	0.02%	0.002%
53	8.773	2398	2405	2411	rVB3	534	661	0.03%	0.004%
54	8.802	2411	2414	2417	rBV2	560	414	0.02%	0.002%
55	8.850	2417	2429	2464	rBV	918530	1519199	57.61%	8.328%
56	9.088	2500	2503	2504	rBV	495	309	0.01%	0.002%
57	9.281	2560	2563	2566	rBV2	599	381	0.01%	0.002%
58	9.320	2572	2575	2578	rBV	336	256	0.01%	0.001%
59	9.455	2615	2617	2623	rVB3	496	281	0.01%	0.002%
60	9.638	2671	2674	2678	rVB2	374	295	0.01%	0.002%
61	9.718	2695	2699	2702	rBV2	349	315	0.01%	0.002%
62	9.908	2755	2758	2761	rVB2	349	269	0.01%	0.001%
63	10.059	2800	2805	2810	rBV3	393	421	0.02%	0.002%
64	10.114	2816	2822	2827	rVB2	301	373	0.01%	0.002%
65	10.162	2831	2837	2840	rBV2	393	390	0.01%	0.002%
66	10.213	2840	2853	2881	rBV	837624	1360323	51.59%	7.457%
67	10.394	2906	2909	2914	rBV2	563	468	0.02%	0.003%
68	10.586	2960	2969	2975	rVB3	929	1354	0.05%	0.007%
69	10.770	3021	3026	3032	rVB3	247	292	0.01%	0.002%
70	10.853	3049	3052	3059	rVB4	860	872	0.03%	0.005%
71	10.992	3090	3095	3100	rBV3	485	627	0.02%	0.003%
72	11.082	3118	3123	3127	rVB3	540	563	0.02%	0.003%
73	11.114	3127	3133	3135	rBV2	533	474	0.02%	0.003%
74	11.246	3163	3174	3197	rBV	821196	1297582	49.21%	7.113%
75	11.413	3224	3226	3229	rBV2	486	251	0.01%	0.001%
76	11.532	3259	3263	3269	rBV2	357	379	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
 Data File : VV027080.D
 Acq On : 29 Jul 2022 13:14
 Operator : SY/MD
 Sample : N3841-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
 Title : VOC Analysis

77	11.622	3279	3291	3315	rBV	1078708	1676499	63.58%	9.190%
78	11.844	3357	3360	3364	rVB3	472	301	0.01%	0.002%
79	12.011	3410	3412	3416	rVB3	384	266	0.01%	0.001%
80	12.651	3607	3611	3612	rBV2	446	329	0.01%	0.002%
81	12.696	3624	3625	3629	rVB3	489	270	0.01%	0.001%
82	12.728	3629	3635	3637	rBV	522	463	0.02%	0.003%
83	13.072	3739	3742	3745	rVB3	426	253	0.01%	0.001%
84	13.107	3750	3753	3759	rBV2	432	389	0.01%	0.002%
85	13.217	3782	3787	3790	rVB4	348	356	0.01%	0.002%
86	13.268	3799	3803	3808	rVV3	384	355	0.01%	0.002%
87	13.384	3835	3839	3842	rBV2	439	359	0.01%	0.002%
88	13.426	3849	3852	3862	rVB3	496	706	0.03%	0.004%
89	13.606	3905	3908	3910	rBV2	645	465	0.02%	0.003%
90	13.741	3947	3950	3952	rBV2	562	339	0.01%	0.002%
91	13.792	3963	3966	3970	rVV2	354	251	0.01%	0.001%
92	13.818	3971	3974	3979	rVB3	384	274	0.01%	0.002%
93	14.065	4047	4051	4053	rBV2	444	279	0.01%	0.002%
94	14.416	4157	4160	4164	rBV2	740	510	0.02%	0.003%
95	14.458	4169	4173	4176	rBV3	659	630	0.02%	0.003%
96	14.609	4218	4220	4223	rBV2	378	256	0.01%	0.001%
97	14.911	4311	4314	4316	rBV3	467	328	0.01%	0.002%
98	15.094	4368	4371	4374	rBV3	725	511	0.02%	0.003%
99	15.146	4385	4387	4390	rBV3	579	298	0.01%	0.002%
100	15.454	4480	4483	4485	rBV2	823	419	0.02%	0.002%




Sum of corrected areas: 18242780

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
Data File : VV027080.D
Acq On : 29 Jul 2022 13:14
Operator : SY/MD
Sample : N3841-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

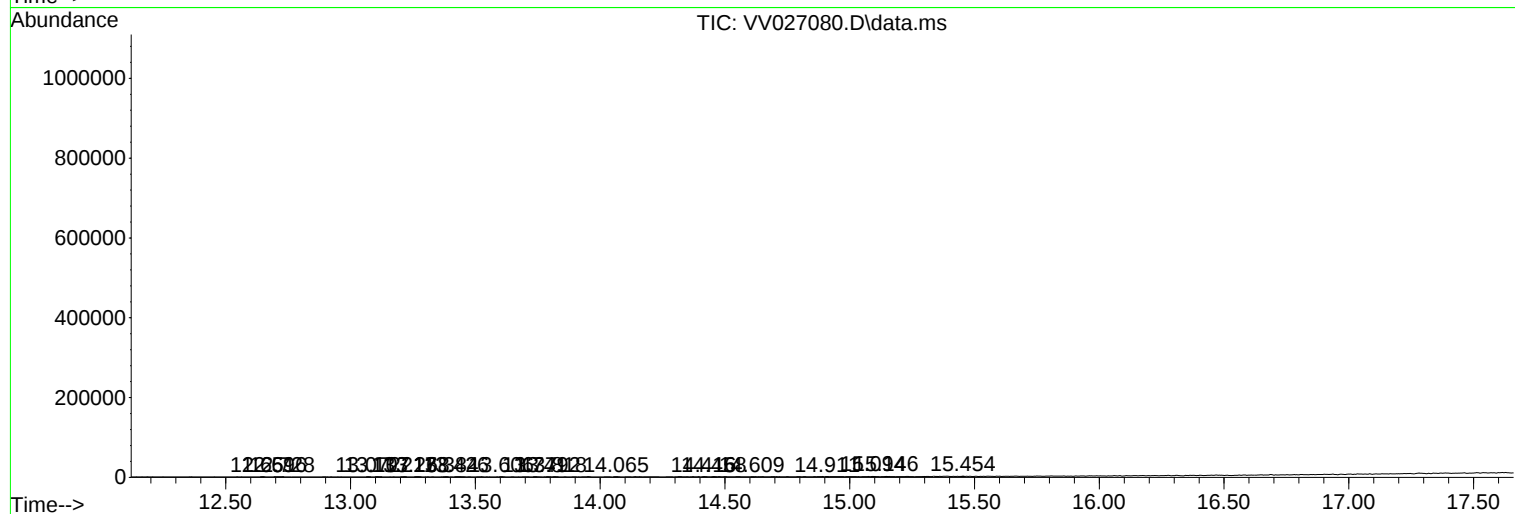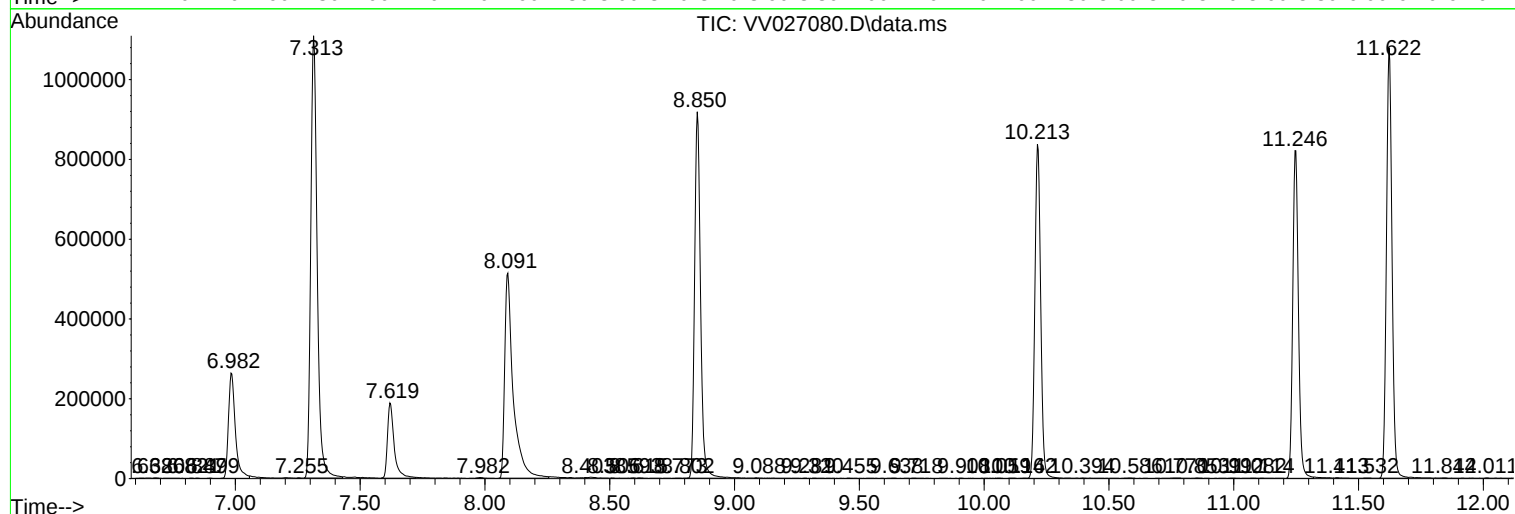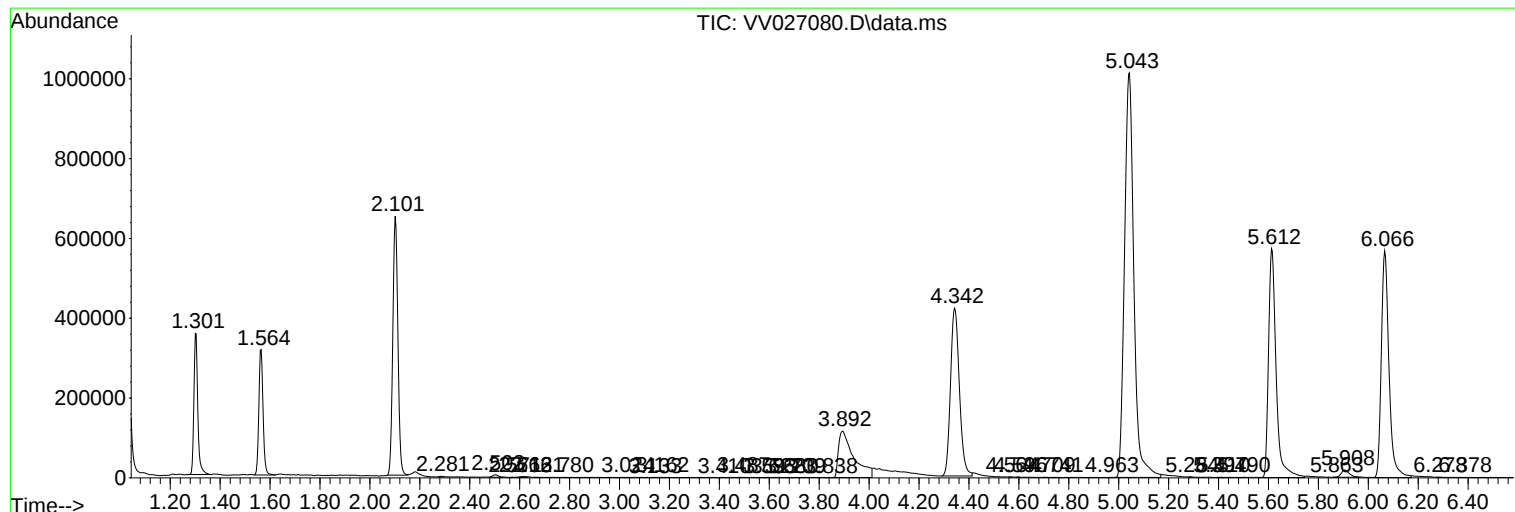

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
Data File : VV027080.D
Acq On : 29 Jul 2022 13:14
Operator : SY/MD
Sample : N3841-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
Data File : VV027080.D
Acq On : 29 Jul 2022 13:14
Operator : SY/MD
Sample : N3841-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc