

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
 Data File : VV027081.D
 Acq On : 29 Jul 2022 13:39
 Operator : SY/MD
 Sample : N3821-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
 Title : VOC Analysis

Signal : TIC: VV027081.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	98	rVB	347590	366123	14.26%	2.055%
2	1.565	155	163	179	rVB	303773	351944	13.70%	1.975%
3	2.102	320	330	346	rBV	626850	891161	34.70%	5.002%
4	2.503	443	455	466	rVB4	9553	16344	0.64%	0.092%
5	2.780	539	541	543	rBV2	336	157	0.01%	0.001%
6	2.912	579	582	585	rBV2	403	300	0.01%	0.002%
7	2.934	587	589	593	rVB2	376	264	0.01%	0.001%
8	3.056	622	627	633	rBV3	394	506	0.02%	0.003%
9	3.272	690	694	696	rBV	308	210	0.01%	0.001%
10	3.291	696	700	703	rBV2	350	300	0.01%	0.002%
11	3.320	707	709	717	rVB3	352	471	0.02%	0.003%
12	3.368	720	724	725	rBV3	174	122	0.00%	0.001%
13	3.442	744	747	750	rBV2	385	261	0.01%	0.001%
14	3.529	772	774	777	rVB2	345	203	0.01%	0.001%
15	3.555	779	782	785	rVB2	442	263	0.01%	0.001%
16	3.584	785	791	793	rBV2	337	294	0.01%	0.002%
17	3.626	797	804	807	rBV	489	405	0.02%	0.002%
18	3.642	807	809	812	rBV2	259	135	0.01%	0.001%
19	3.664	812	816	820	rBV2	297	299	0.01%	0.002%
20	3.680	820	821	824	rVB	429	101	0.00%	0.001%
21	3.712	829	831	832	rVB	133	36	0.00%	0.000%
22	3.725	832	835	837	rBV2	250	145	0.01%	0.001%
23	3.761	843	846	848	rBV	194	146	0.01%	0.001%
24	3.796	854	857	859	rBV	131	74	0.00%	0.000%
25	3.812	859	862	863	rBV2	252	152	0.01%	0.001%
26	3.828	863	867	874	rVB3	333	401	0.02%	0.002%
27	3.886	875	885	924	rBV2	111661	488726	19.03%	2.743%
28	4.343	1013	1027	1049	rBV2	410851	994173	38.71%	5.580%
29	4.696	1135	1137	1141	rVB2	461	224	0.01%	0.001%
30	4.716	1141	1143	1147	rBV3	512	305	0.01%	0.002%
31	4.741	1147	1151	1153	rBV2	535	385	0.01%	0.002%
32	4.780	1160	1163	1165	rBV2	397	238	0.01%	0.001%
33	4.828	1175	1178	1184	rVB5	668	656	0.03%	0.004%
34	4.860	1184	1188	1190	rBV2	344	236	0.01%	0.001%
35	4.892	1197	1198	1201	rBV3	262	88	0.00%	0.000%
36	4.976	1222	1224	1227	rBV2	269	210	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
 Data File : VV027081.D
 Acq On : 29 Jul 2022 13:39
 Operator : SY/MD
 Sample : N3821-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
 Title : VOC Analysis

37	5.044	1227	1245	1287	rBV2	966987	2568156	100.00%	14.414%
38	5.388	1350	1352	1353	rBV2	351	133	0.01%	0.001%
39	5.452	1370	1372	1378	rVB3	478	428	0.02%	0.002%
40	5.513	1389	1391	1396	rVB2	749	528	0.02%	0.003%
41	5.613	1410	1422	1461	rBV	579346	1214294	47.28%	6.815%
42	5.905	1502	1513	1538	rVB3	18622	42430	1.65%	0.238%
43	6.008	1544	1545	1547	rBV2	265	152	0.01%	0.001%
44	6.066	1549	1563	1599	rVV	556263	1167365	45.46%	6.552%
45	6.416	1670	1672	1673	rBV	209	107	0.00%	0.001%
46	6.429	1673	1676	1680	rVV4	471	443	0.02%	0.002%
47	6.510	1699	1701	1706	rBV2	251	208	0.01%	0.001%
48	6.545	1710	1712	1714	rBV	212	107	0.00%	0.001%
49	6.561	1714	1717	1722	rVB2	485	276	0.01%	0.002%
50	6.587	1722	1725	1727	rVB	194	105	0.00%	0.001%
51	6.597	1727	1728	1731	rBV	126	38	0.00%	0.000%
52	6.622	1731	1736	1738	rBV2	291	225	0.01%	0.001%
53	6.757	1774	1778	1781	rVB2	528	398	0.02%	0.002%
54	6.783	1782	1786	1790	rBV2	408	354	0.01%	0.002%
55	6.809	1790	1794	1798	rBV2	520	531	0.02%	0.003%
56	6.879	1812	1816	1817	rBV	282	172	0.01%	0.001%
57	6.928	1827	1831	1834	rBV2	329	271	0.01%	0.002%
58	6.982	1837	1848	1883	rBV	254381	490254	19.09%	2.752%
59	7.159	1902	1903	1905	rBV2	500	200	0.01%	0.001%
60	7.314	1939	1951	1985	rBV	1069142	1926044	75.00%	10.810%
61	7.619	2037	2046	2077	rBV	179633	336978	13.12%	1.891%
62	7.937	2143	2145	2150	rBV	371	200	0.01%	0.001%
63	8.011	2165	2168	2173	rBV3	221	195	0.01%	0.001%
64	8.037	2174	2176	2178	rVB2	582	197	0.01%	0.001%
65	8.092	2181	2193	2240	rBV	490050	1184407	46.12%	6.647%
66	8.703	2379	2383	2385	rBV2	449	377	0.01%	0.002%
67	8.757	2398	2400	2405	rVB4	549	398	0.02%	0.002%
68	8.789	2405	2410	2411	rBV2	404	292	0.01%	0.002%
69	8.850	2417	2429	2453	rBV	912260	1514556	58.97%	8.500%
70	9.349	2582	2584	2588	rVB	338	229	0.01%	0.001%
71	9.391	2594	2597	2599	rBV2	371	203	0.01%	0.001%
72	9.484	2622	2626	2629	rVB2	349	269	0.01%	0.002%
73	9.500	2629	2631	2632	rBV2	126	37	0.00%	0.000%
74	9.526	2633	2639	2640	rBV2	289	228	0.01%	0.001%
75	9.584	2654	2657	2658	rBV2	194	98	0.00%	0.001%
76	9.600	2658	2662	2665	rBV3	458	411	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
 Data File : VV027081.D
 Acq On : 29 Jul 2022 13:39
 Operator : SY/MD
 Sample : N3821-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
 Title : VOC Analysis

77	9.686	2687	2689	2691	rBV2	146	80	0.00%	0.000%
78	9.696	2691	2692	2694	rVV	464	106	0.00%	0.001%
79	9.776	2715	2717	2718	rVB	423	103	0.00%	0.001%
80	9.802	2724	2725	2726	rBV	183	54	0.00%	0.000%
81	9.828	2731	2733	2735	rBV2	282	125	0.00%	0.001%
82	10.050	2800	2802	2803	rBV	313	143	0.01%	0.001%
83	10.214	2841	2853	2881	rBV	823473	1316216	51.25%	7.387%
84	10.355	2895	2897	2901	rBV2	556	222	0.01%	0.001%
85	10.584	2961	2968	2971	rVB3	649	654	0.03%	0.004%
86	10.603	2971	2974	2975	rBV2	348	186	0.01%	0.001%
87	10.638	2983	2985	2987	rBV	235	138	0.01%	0.001%
88	10.773	3022	3027	3029	rBV2	425	398	0.02%	0.002%
89	10.850	3047	3051	3056	rBV3	948	777	0.03%	0.004%
90	10.908	3064	3069	3070	rBV	254	207	0.01%	0.001%
91	11.047	3108	3112	3113	rBV2	365	255	0.01%	0.001%
92	11.172	3148	3151	3152	rBV	368	204	0.01%	0.001%
93	11.249	3163	3175	3197	rBV	828658	1300048	50.62%	7.296%
94	11.622	3276	3291	3315	rBV	1037484	1627540	63.37%	9.134%
95	11.895	3373	3376	3378	rBV2	583	415	0.02%	0.002%
96	11.928	3385	3386	3387	rVB	571	110	0.00%	0.001%
97	11.940	3387	3390	3391	rBV2	339	189	0.01%	0.001%
98	12.760	3642	3645	3650	rBV3	543	499	0.02%	0.003%
99	13.767	3955	3958	3961	rBV	518	427	0.02%	0.002%
100	13.976	4020	4023	4024	rBV3	412	231	0.01%	0.001%




Sum of corrected areas: 17817679

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
Data File : VV027081.D
Acq On : 29 Jul 2022 13:39
Operator : SY/MD
Sample : N3821-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

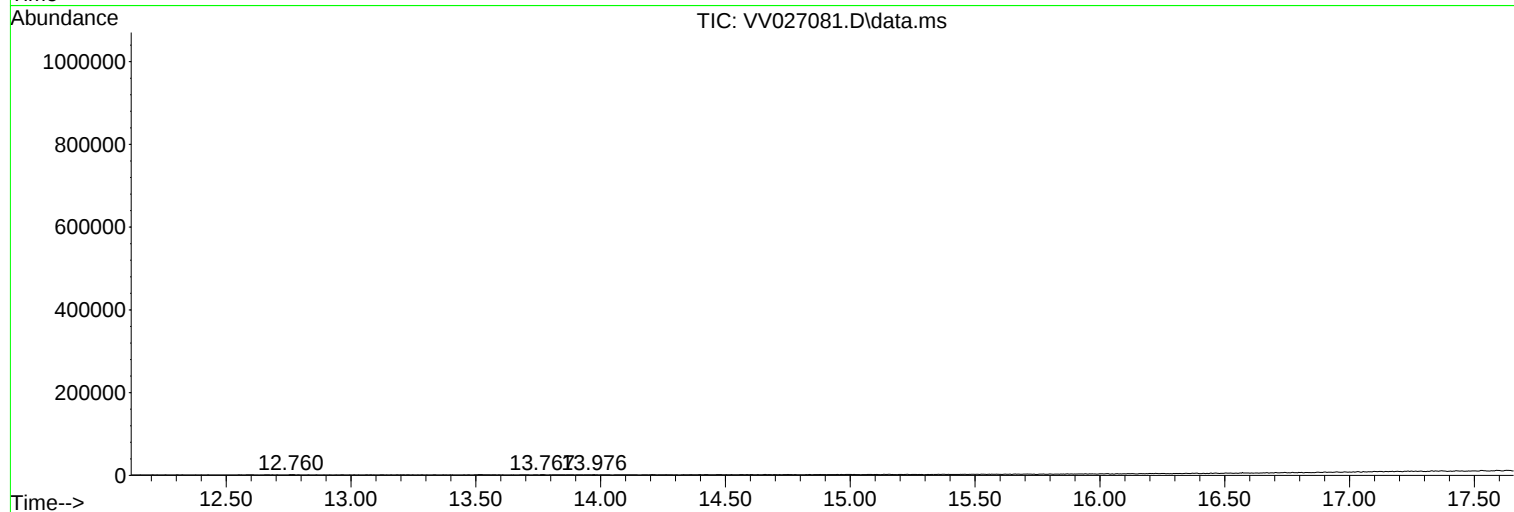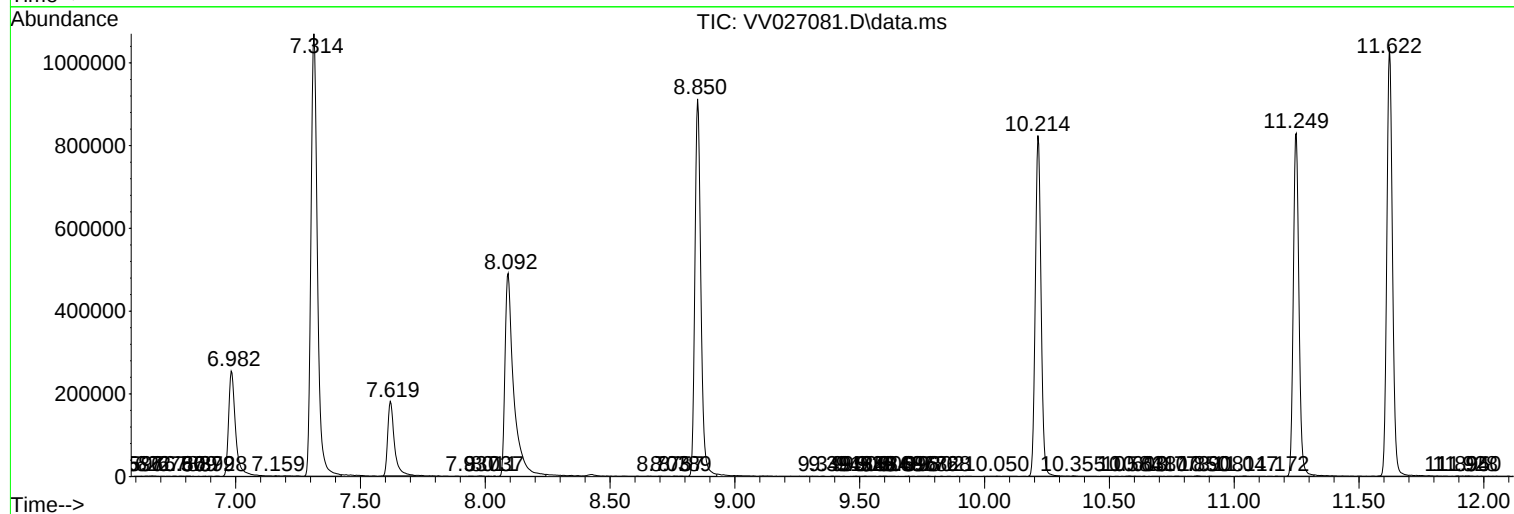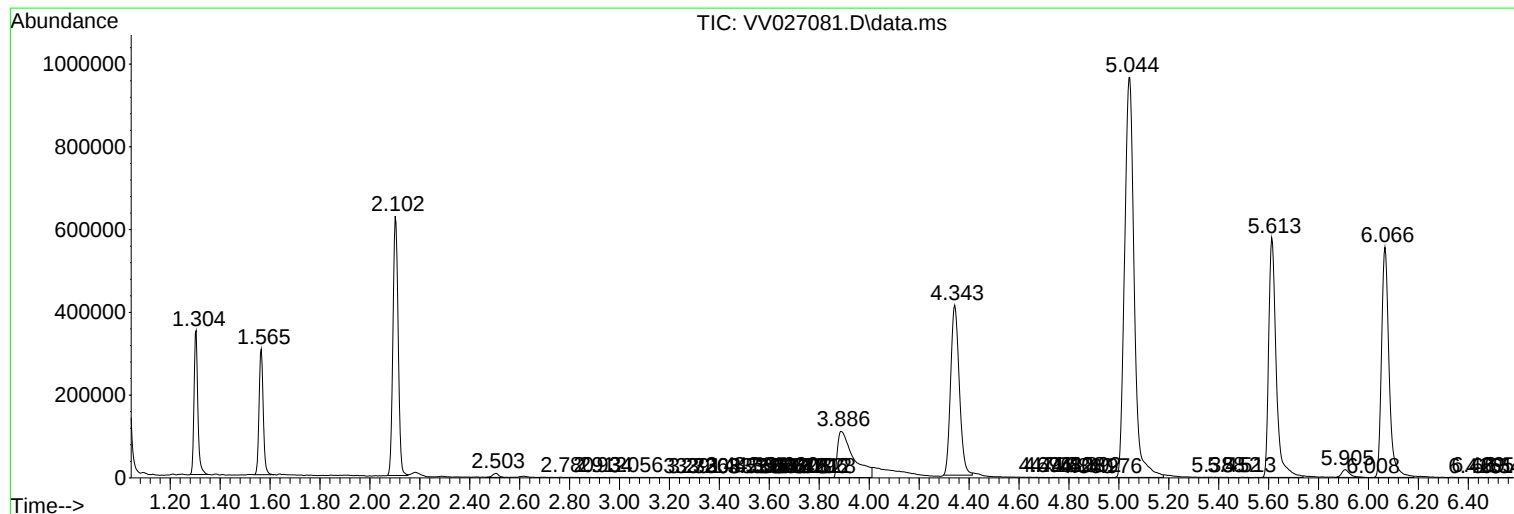

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
Data File : VV027081.D
Acq On : 29 Jul 2022 13:39
Operator : SY/MD
Sample : N3821-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
Data File : VV027081.D
Acq On : 29 Jul 2022 13:39
Operator : SY/MD
Sample : N3821-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc