

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
 Data File : VV027086.D
 Acq On : 29 Jul 2022 15:42
 Operator : SY/MD
 Sample : N3880-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUF8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
 Title : VOC Analysis

Signal : TIC: VV027086.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	102	rVB	348483	367395	9.27%	1.527%
2	1.564	155	163	178	rBV	281915	322945	8.15%	1.342%
3	2.101	320	330	346	rBV	593411	857980	21.65%	3.566%
4	2.291	384	389	396	rVB6	1383	1824	0.05%	0.008%
5	2.375	413	415	423	rVB5	1394	1383	0.03%	0.006%
6	2.500	447	454	466	rVB5	2498	4037	0.10%	0.017%
7	2.731	522	526	527	rBV2	561	398	0.01%	0.002%
8	2.764	527	536	545	rVB4	4838	8237	0.21%	0.034%
9	2.828	553	556	560	rVB3	428	280	0.01%	0.001%
10	2.860	560	566	569	rBV4	346	400	0.01%	0.002%
11	2.982	601	604	610	rVB2	288	287	0.01%	0.001%
12	3.104	637	642	643	rBV3	332	286	0.01%	0.001%
13	3.198	668	671	676	rVB3	623	550	0.01%	0.002%
14	3.236	676	683	686	rBV2	570	614	0.02%	0.003%
15	3.256	686	689	694	rVB2	388	328	0.01%	0.001%
16	3.336	710	714	716	rBV	392	278	0.01%	0.001%
17	3.455	748	751	754	rVV	504	360	0.01%	0.001%
18	3.481	757	759	763	rVB2	523	344	0.01%	0.001%
19	3.661	811	815	817	rBV	383	304	0.01%	0.001%
20	3.722	828	834	838	rBV3	438	413	0.01%	0.002%
21	3.741	838	840	848	rVB3	378	325	0.01%	0.001%
22	3.905	874	891	915	rBV2	1102229	2832059	71.47%	11.770%
23	4.342	1012	1027	1050	rBV	373245	909732	22.96%	3.781%
24	4.641	1115	1120	1121	rBV2	744	649	0.02%	0.003%
25	4.870	1189	1191	1195	rBV3	508	330	0.01%	0.001%
26	5.043	1227	1245	1282	rBV2	904378	2377613	60.00%	9.882%
27	5.407	1356	1358	1363	rVB4	518	341	0.01%	0.001%
28	5.461	1371	1375	1377	rBV2	372	296	0.01%	0.001%
29	5.519	1388	1393	1396	rBV4	572	510	0.01%	0.002%
30	5.612	1409	1422	1465	rBV	600626	1264435	31.91%	5.255%
31	5.911	1503	1515	1548	rBV2	339144	707853	17.86%	2.942%
32	6.066	1549	1563	1607	rVV	505686	1062114	26.80%	4.414%
33	6.345	1647	1650	1655	rVB4	744	752	0.02%	0.003%
34	6.368	1655	1657	1662	rBV3	428	395	0.01%	0.002%
35	6.423	1671	1674	1677	rBV3	391	335	0.01%	0.001%
36	6.481	1688	1692	1698	rBV3	483	499	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
 Data File : VV027086.D
 Acq On : 29 Jul 2022 15:42
 Operator : SY/MD
 Sample : N3880-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUF8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
 Title : VOC Analysis

37	6.561	1713	1717	1721	rVB2	486	303	0.01%	0.001%
38	6.596	1721	1728	1731	rBV4	476	646	0.02%	0.003%
39	6.664	1744	1749	1751	rBV2	508	458	0.01%	0.002%
40	6.757	1773	1778	1782	rBV2	555	471	0.01%	0.002%
41	6.882	1813	1817	1820	rBV3	457	385	0.01%	0.002%
42	6.902	1821	1823	1827	rVB2	417	273	0.01%	0.001%
43	6.921	1827	1829	1833	rBV2	446	387	0.01%	0.002%
44	6.985	1837	1849	1879	rBV	236211	462618	11.68%	1.923%
45	7.313	1939	1951	1969	rBV	1024316	1806814	45.60%	7.509%
46	7.554	2024	2026	2031	rVB4	924	736	0.02%	0.003%
47	7.622	2036	2047	2086	rVV	164017	309882	7.82%	1.288%
48	7.773	2092	2094	2098	rVB3	791	462	0.01%	0.002%
49	7.908	2132	2136	2137	rBV2	687	466	0.01%	0.002%
50	7.972	2142	2156	2182	rVV	2330434	3962390	100.00%	16.468%
51	8.091	2183	2193	2234	rVB	438323	1019902	25.74%	4.239%
52	8.500	2318	2320	2323	rVB2	565	271	0.01%	0.001%
53	8.580	2342	2345	2349	rBV4	469	460	0.01%	0.002%
54	8.628	2356	2360	2363	rBV4	720	645	0.02%	0.003%
55	8.792	2409	2411	2413	rBV	449	268	0.01%	0.001%
56	8.850	2417	2429	2463	rBV	939562	1559881	39.37%	6.483%
57	9.123	2510	2514	2515	rBV	463	271	0.01%	0.001%
58	9.136	2515	2518	2521	rBV4	718	658	0.02%	0.003%
59	9.249	2547	2553	2554	rBV5	528	464	0.01%	0.002%
60	9.377	2590	2593	2599	rBV3	595	594	0.01%	0.002%
61	9.477	2619	2624	2626	rBV	333	326	0.01%	0.001%
62	9.548	2641	2646	2647	rBV2	738	483	0.01%	0.002%
63	9.718	2695	2699	2703	rBV2	449	454	0.01%	0.002%
64	9.789	2717	2721	2723	rBV2	484	353	0.01%	0.001%
65	9.857	2738	2742	2747	rVB2	502	494	0.01%	0.002%
66	9.892	2747	2753	2754	rBV	408	340	0.01%	0.001%
67	9.921	2758	2762	2765	rBV3	305	282	0.01%	0.001%
68	10.213	2841	2853	2874	rBV	722165	1163711	29.37%	4.836%
69	10.384	2902	2906	2912	rVB5	1067	1267	0.03%	0.005%
70	10.410	2912	2914	2918	rVB2	399	265	0.01%	0.001%
71	10.484	2933	2937	2939	rBV2	476	306	0.01%	0.001%
72	10.548	2953	2957	2963	rVB4	431	352	0.01%	0.001%
73	10.577	2963	2966	2967	rBV	726	350	0.01%	0.001%
74	10.664	2991	2993	2996	rBV2	466	335	0.01%	0.001%
75	10.982	3089	3092	3099	rVB3	513	495	0.01%	0.002%
76	11.249	3162	3175	3201	rBV	886534	1371308	34.61%	5.699%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
 Data File : VV027086.D
 Acq On : 29 Jul 2022 15:42
 Operator : SY/MD
 Sample : N3880-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUF8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
 Title : VOC Analysis

77	11.474	3241	3245	3250	rBV3	614	582	0.01%	0.002%
78	11.535	3255	3264	3279	rBV10	4344	8950	0.23%	0.037%
79	11.622	3279	3291	3310	rBV	977218	1523306	38.44%	6.331%
80	11.799	3343	3346	3350	rBV3	658	588	0.01%	0.002%
81	12.300	3498	3502	3504	rBV	566	379	0.01%	0.002%
82	12.432	3541	3543	3548	rBV3	538	281	0.01%	0.001%
83	12.625	3598	3603	3607	rVV2	386	488	0.01%	0.002%
84	12.683	3619	3621	3625	rVV2	565	389	0.01%	0.002%
85	12.721	3629	3633	3636	rBV2	452	401	0.01%	0.002%
86	12.737	3636	3638	3646	rVB2	713	518	0.01%	0.002%
87	12.776	3647	3650	3654	rBV3	433	292	0.01%	0.001%
88	12.885	3681	3684	3691	rBV3	615	580	0.01%	0.002%
89	13.278	3804	3806	3813	rVB3	646	625	0.02%	0.003%
90	13.319	3813	3819	3821	rBV	527	555	0.01%	0.002%
91	13.509	3869	3878	3893	rVB	13632	22803	0.58%	0.095%
92	14.310	4124	4127	4131	rVB3	666	476	0.01%	0.002%
93	14.635	4218	4228	4244	rBV	13115	22220	0.56%	0.092%
94	14.712	4249	4252	4255	rBV2	581	348	0.01%	0.001%
95	14.818	4275	4285	4294	rBV2	16632	26003	0.66%	0.108%
96	14.908	4311	4313	4314	rBV2	735	296	0.01%	0.001%
97	15.040	4352	4354	4358	rBV4	589	346	0.01%	0.001%
98	15.663	4546	4548	4550	rBV	1244	635	0.02%	0.003%
99	15.815	4591	4595	4602	rVB6	3327	3619	0.09%	0.015%
100	16.483	4795	4803	4815	rVB	30634	48716	1.23%	0.202%




Sum of corrected areas: 24061103

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
Data File : VV027086.D
Acq On : 29 Jul 2022 15:42
Operator : SY/MD
Sample : N3880-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUF8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

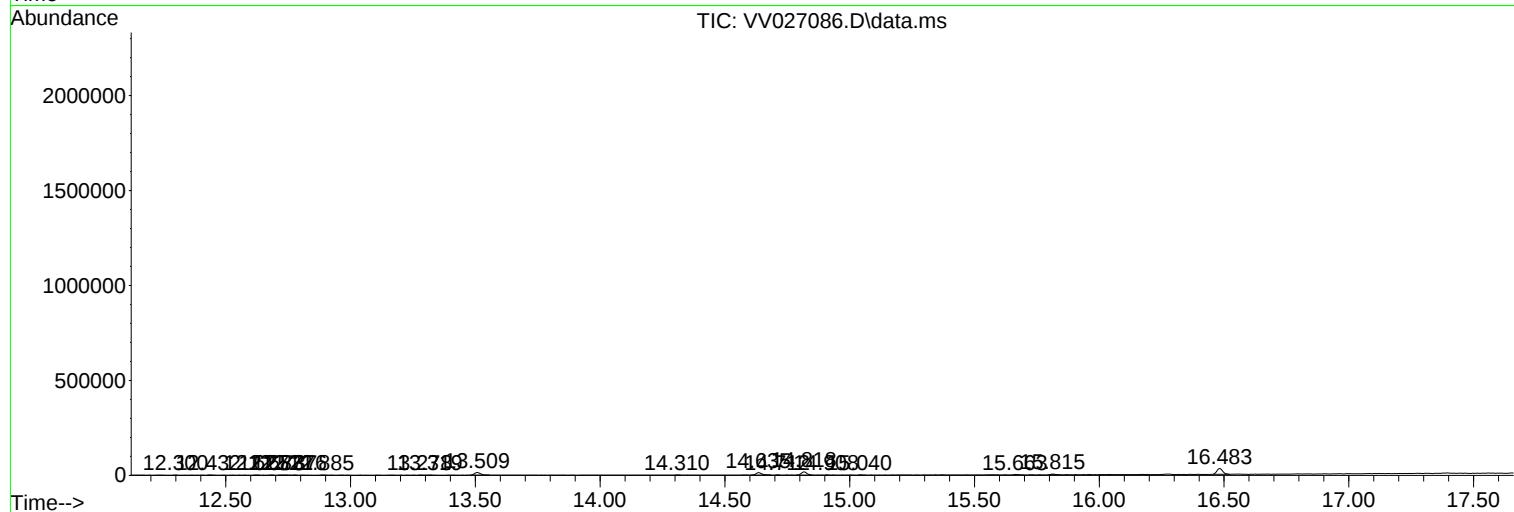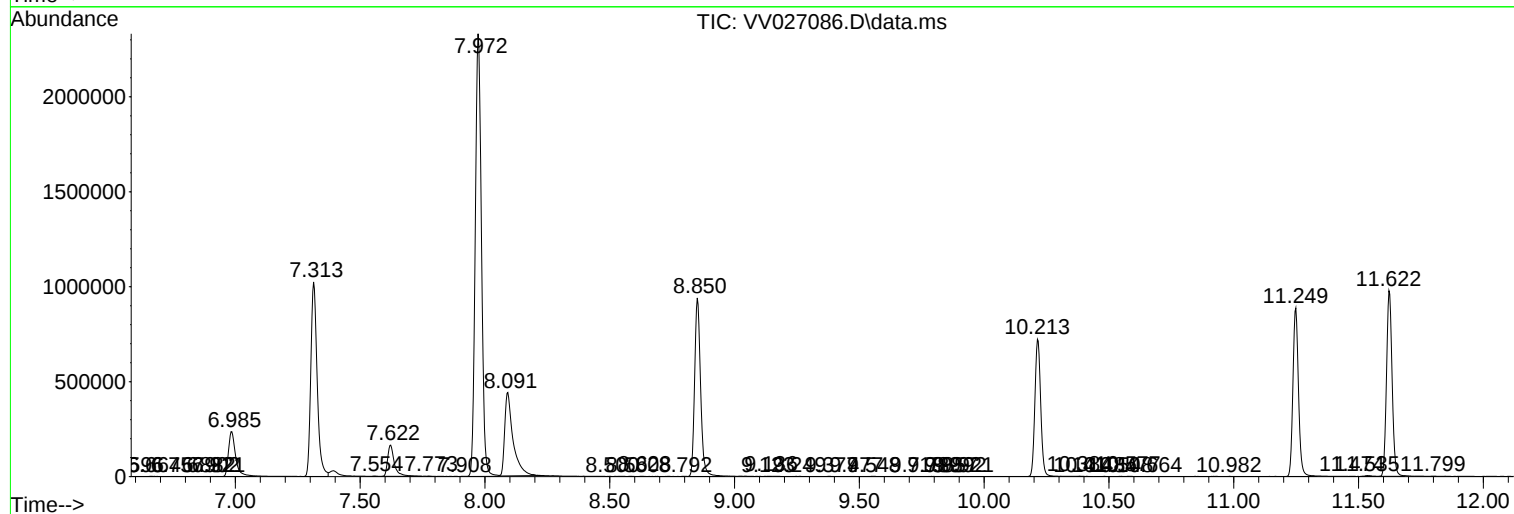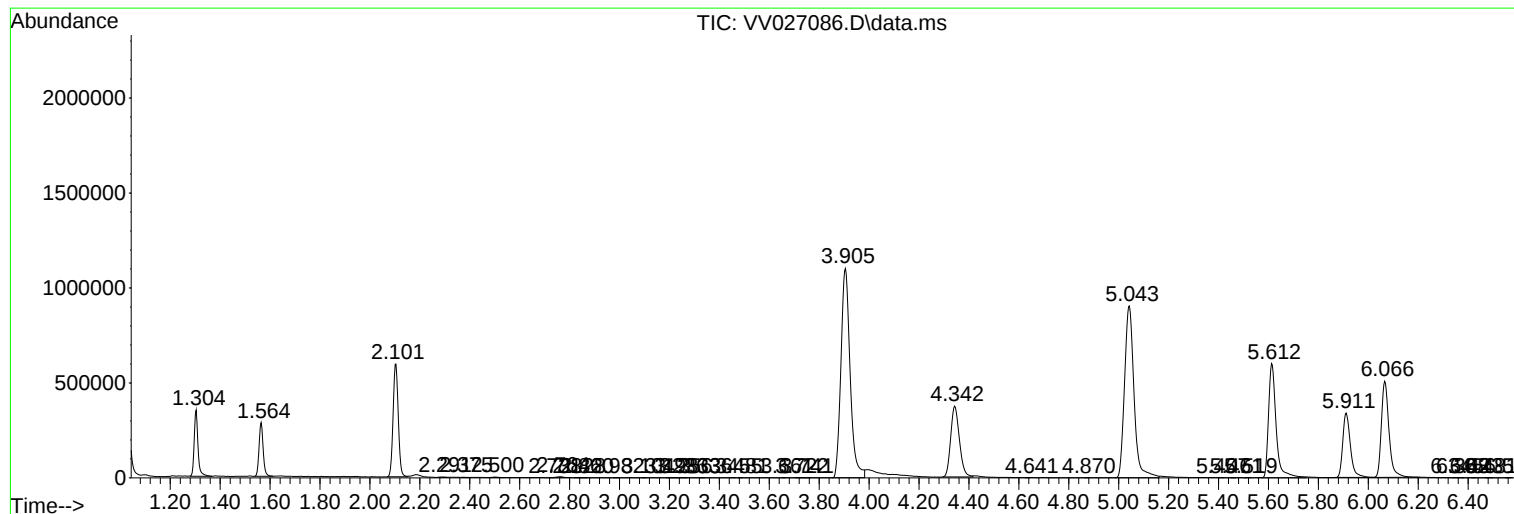

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
Data File : VV027086.D
Acq On : 29 Jul 2022 15:42
Operator : SY/MD
Sample : N3880-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUF8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
Data File : VV027086.D
Acq On : 29 Jul 2022 15:42
Operator : SY/MD
Sample : N3880-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUF8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc