

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
 Data File : VV027087.D
 Acq On : 29 Jul 2022 16:06
 Operator : SY/MD
 Sample : N3880-16 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUG9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M

Title : VOC Analysis

Signal : TIC: VV027087.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	74	81	98	rVB	330740	350720	14.73%	2.049%
2	1.561	155	162	175	rBV	271816	315179	13.24%	1.841%
3	2.101	319	330	347	rBV	595613	843657	35.44%	4.928%
4	2.333	399	402	406	rBV	18072	10038	0.42%	0.059%
5	2.500	446	454	466	rVB2	11398	18440	0.77%	0.108%
6	2.609	477	488	501	rBV2	4802	10712	0.45%	0.063%
7	2.748	529	531	534	rVB4	584	346	0.01%	0.002%
8	2.931	586	588	594	rBV2	380	386	0.02%	0.002%
9	3.153	652	657	659	rBV2	268	276	0.01%	0.002%
10	3.471	748	756	759	rBV3	328	386	0.02%	0.002%
11	3.529	767	774	778	rBV3	476	608	0.03%	0.004%
12	3.568	783	786	789	rBV3	411	283	0.01%	0.002%
13	3.677	817	820	823	rBV2	358	334	0.01%	0.002%
14	3.892	875	887	927	rBV2	111887	509812	21.41%	2.978%
15	4.342	1011	1027	1050	rBV	375066	923772	38.80%	5.396%
16	4.622	1111	1114	1117	rBV2	454	304	0.01%	0.002%
17	4.661	1122	1126	1131	rBV4	504	436	0.02%	0.003%
18	4.683	1131	1133	1139	rVB3	804	677	0.03%	0.004%
19	4.715	1139	1143	1145	rBV3	618	435	0.02%	0.003%
20	4.744	1150	1152	1157	rBV3	483	481	0.02%	0.003%
21	4.953	1211	1217	1219	rBV3	353	333	0.01%	0.002%
22	5.040	1227	1244	1305	rBV2	907472	2380744	100.00%	13.907%
23	5.291	1320	1322	1327	rVB3	758	534	0.02%	0.003%
24	5.368	1344	1346	1351	rBV2	376	334	0.01%	0.002%
25	5.410	1357	1359	1364	rVB2	621	471	0.02%	0.003%
26	5.477	1378	1380	1383	rBV	537	350	0.01%	0.002%
27	5.613	1410	1422	1460	rBV	589238	1243202	52.22%	7.262%
28	5.905	1502	1513	1535	rBV5	18952	45680	1.92%	0.267%
29	6.066	1549	1563	1598	rBV	506969	1074725	45.14%	6.278%
30	6.336	1644	1647	1650	rVB3	652	421	0.02%	0.002%
31	6.436	1676	1678	1683	rVB3	338	290	0.01%	0.002%
32	6.529	1703	1707	1711	rVB3	434	347	0.01%	0.002%
33	6.571	1716	1720	1725	rBV2	312	375	0.02%	0.002%
34	6.664	1743	1749	1753	rBV3	917	1074	0.05%	0.006%
35	6.719	1762	1766	1772	rBV5	415	497	0.02%	0.003%
36	6.760	1777	1779	1783	rVB3	478	352	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
 Data File : VV027087.D
 Acq On : 29 Jul 2022 16:06
 Operator : SY/MD
 Sample : N3880-16 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUG9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
 Title : VOC Analysis

37	6.812	1792	1795	1800	rBV3	459	408	0.02%	0.002%
38	6.985	1837	1849	1882	rBV	235996	456364	19.17%	2.666%
39	7.201	1912	1916	1918	rBV2	685	429	0.02%	0.003%
40	7.249	1928	1931	1934	rVB5	682	356	0.01%	0.002%
41	7.313	1939	1951	1986	rBV	1010063	1808882	75.98%	10.566%
42	7.558	2023	2027	2029	rBV3	686	435	0.02%	0.003%
43	7.619	2036	2046	2077	rBV	166179	305940	12.85%	1.787%
44	7.921	2136	2140	2142	rBV	584	386	0.02%	0.002%
45	7.976	2146	2157	2173	rBV	95797	164785	6.92%	0.963%
46	8.091	2182	2193	2238	rBV	457159	1039672	43.67%	6.073%
47	8.419	2292	2295	2304	rVB6	1884	2372	0.10%	0.014%
48	8.484	2312	2315	2319	rVB3	600	389	0.02%	0.002%
49	8.619	2354	2357	2359	rBV	689	421	0.02%	0.002%
50	8.850	2415	2429	2458	rBV	931068	1530097	64.27%	8.938%
51	9.018	2479	2481	2486	rVB4	1168	818	0.03%	0.005%
52	9.069	2492	2497	2500	rBV3	543	379	0.02%	0.002%
53	9.098	2503	2506	2510	rBV3	585	537	0.02%	0.003%
54	9.255	2551	2555	2558	rBV2	343	280	0.01%	0.002%
55	9.554	2643	2648	2650	rBV2	332	289	0.01%	0.002%
56	9.747	2705	2708	2712	rBV2	337	293	0.01%	0.002%
57	9.844	2735	2738	2742	rBV2	379	298	0.01%	0.002%
58	10.214	2841	2853	2875	rBV	748010	1168525	49.08%	6.826%
59	10.387	2905	2907	2914	rVB4	638	593	0.02%	0.003%
60	10.445	2922	2925	2927	rBV3	415	282	0.01%	0.002%
61	10.461	2927	2930	2935	rVB3	460	360	0.02%	0.002%
62	10.587	2964	2969	2975	rBV4	1076	1050	0.04%	0.006%
63	10.654	2986	2990	2991	rBV	510	326	0.01%	0.002%
64	10.902	3064	3067	3070	rVB2	383	286	0.01%	0.002%
65	11.037	3104	3109	3112	rBV	501	438	0.02%	0.003%
66	11.127	3129	3137	3139	rBV3	340	487	0.02%	0.003%
67	11.249	3163	3175	3204	rVV	847370	1340445	56.30%	7.830%
68	11.490	3246	3250	3252	rBV3	658	439	0.02%	0.003%
69	11.532	3255	3263	3265	rBV4	1003	1116	0.05%	0.007%
70	11.554	3268	3270	3275	rVB4	732	437	0.02%	0.003%
71	11.622	3278	3291	3314	rBV	969154	1501315	63.06%	8.770%
72	11.918	3380	3383	3387	rVB2	392	313	0.01%	0.002%
73	12.609	3593	3598	3602	rVB2	338	340	0.01%	0.002%
74	12.889	3682	3685	3690	rVB	586	446	0.02%	0.003%
75	12.982	3711	3714	3717	rBV2	358	317	0.01%	0.002%
76	13.027	3724	3728	3731	rBV2	324	303	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
 Data File : VV027087.D
 Acq On : 29 Jul 2022 16:06
 Operator : SY/MD
 Sample : N3880-16 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUG9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
 Title : VOC Analysis

77	13.098	3747	3750	3754	rBV3	372	292	0.01%	0.002%
78	13.217	3782	3787	3789	rBV2	586	561	0.02%	0.003%
79	13.429	3850	3853	3856	rBV3	515	350	0.01%	0.002%
80	13.513	3872	3879	3889	rBV2	4972	7705	0.32%	0.045%
81	13.593	3899	3904	3906	rBV3	531	444	0.02%	0.003%
82	13.670	3925	3928	3932	rVB2	280	277	0.01%	0.002%
83	13.857	3983	3986	3988	rBV	518	384	0.02%	0.002%
84	13.972	4019	4022	4024	rBV3	390	287	0.01%	0.002%
85	14.049	4044	4046	4050	rVB3	471	302	0.01%	0.002%
86	14.175	4082	4085	4089	rVB3	895	674	0.03%	0.004%
87	14.300	4119	4124	4128	rVB3	687	593	0.02%	0.003%
88	14.336	4131	4135	4139	rBV2	562	563	0.02%	0.003%
89	14.525	4191	4194	4198	rVB2	606	438	0.02%	0.003%
90	14.548	4199	4201	4205	rBV4	514	420	0.02%	0.002%
91	14.638	4221	4229	4243	rBV3	3966	7753	0.33%	0.045%
92	14.721	4252	4255	4258	rBV2	612	455	0.02%	0.003%
93	14.766	4266	4269	4272	rBV	585	387	0.02%	0.002%
94	14.824	4278	4287	4294	rVB4	4640	7213	0.30%	0.042%
95	14.889	4305	4307	4312	rVB3	486	352	0.01%	0.002%
96	14.950	4323	4326	4331	rVB3	686	620	0.03%	0.004%
97	14.998	4339	4341	4344	rBV4	599	410	0.02%	0.002%
98	15.384	4459	4461	4465	rBV4	652	401	0.02%	0.002%
99	15.429	4473	4475	4477	rBV3	781	368	0.02%	0.002%
100	16.483	4797	4803	4816	rVB3	12411	19615	0.82%	0.115%




Sum of corrected areas: 17119523

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
Data File : VV027087.D
Acq On : 29 Jul 2022 16:06
Operator : SY/MD
Sample : N3880-16 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUG9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

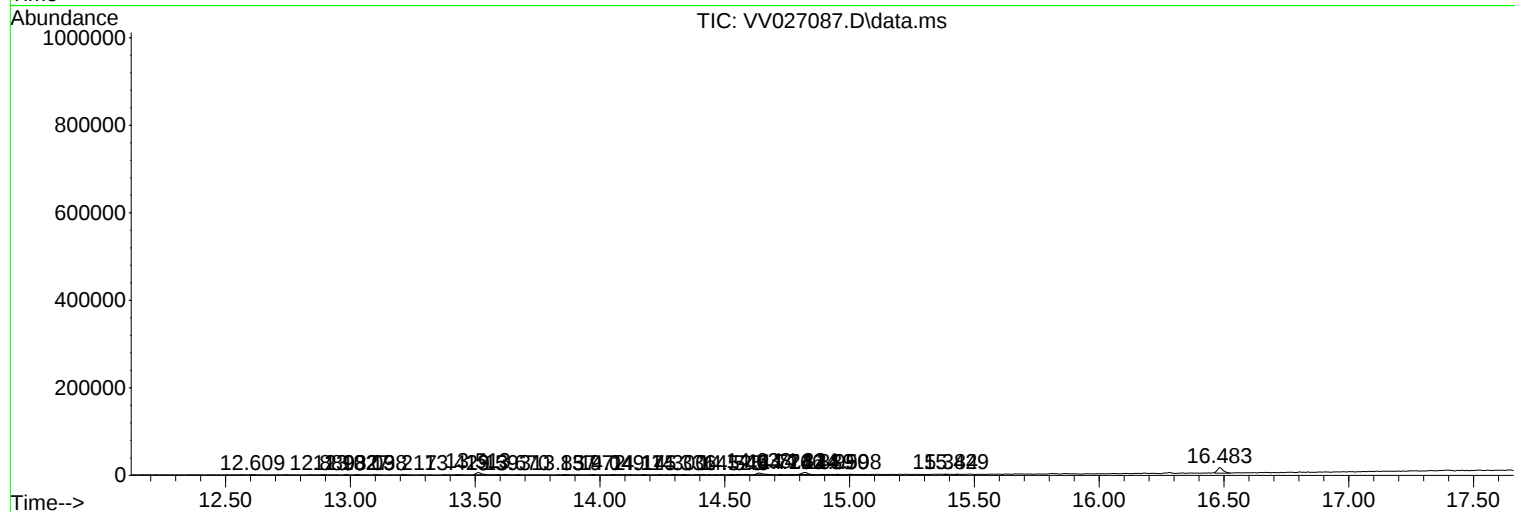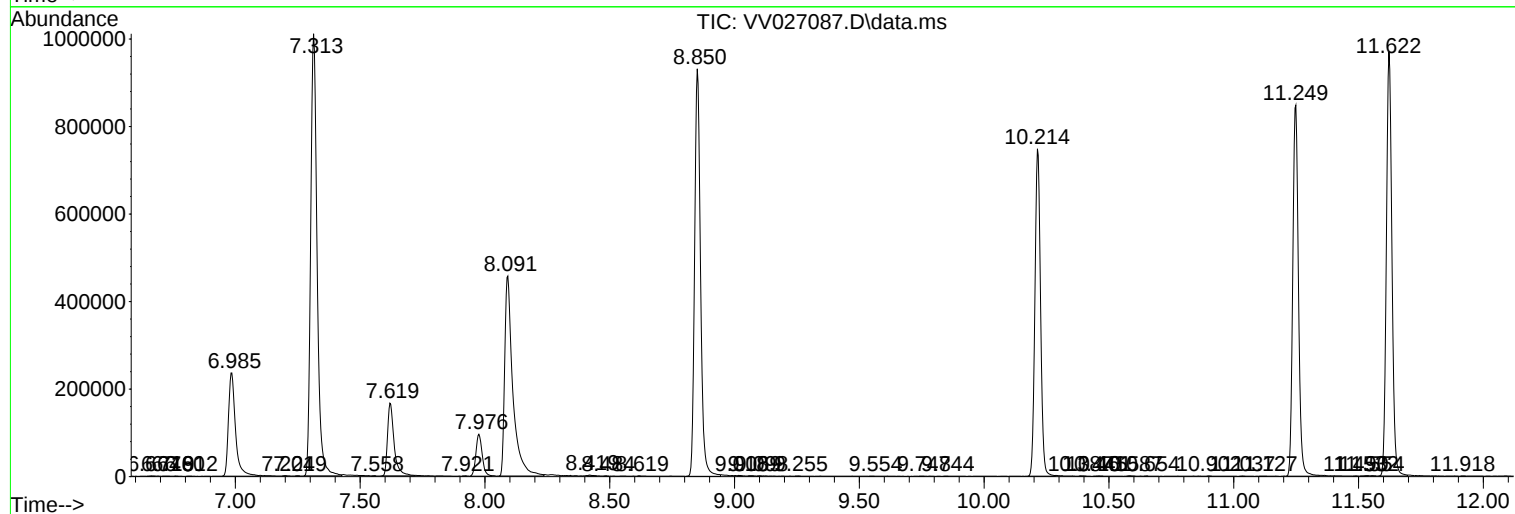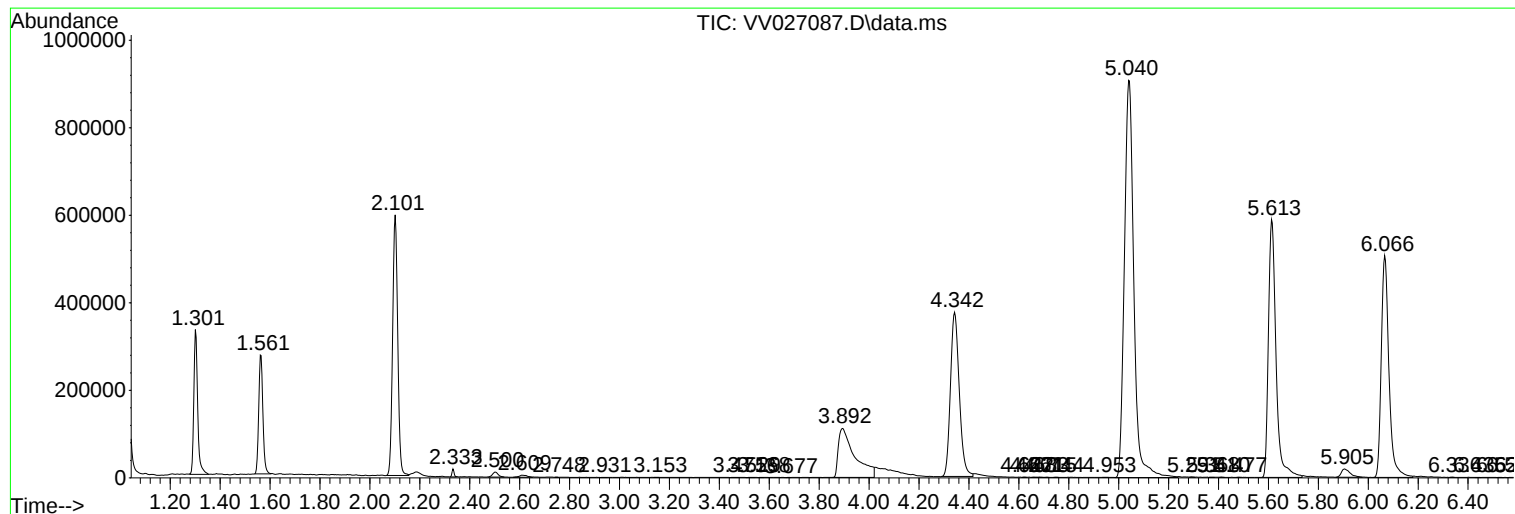

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
Data File : VV027087.D
Acq On : 29 Jul 2022 16:06
Operator : SY/MD
Sample : N3880-16 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUG9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
Data File : VV027087.D
Acq On : 29 Jul 2022 16:06
Operator : SY/MD
Sample : N3880-16 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUG9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------