

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
 Data File : VV027088.D
 Acq On : 29 Jul 2022 16:31
 Operator : SY/MD
 Sample : N3880-17 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUH1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M

Title : VOC Analysis

Signal : TIC: VV027088.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	74	81	101	rVB	322561	339386	14.79%	2.111%
2	1.561	155	162	173	rBV	268347	311138	13.56%	1.936%
3	2.101	320	330	347	rVB	568713	805152	35.09%	5.009%
4	2.503	445	455	467	rBV3	10506	17898	0.78%	0.111%
5	2.616	484	490	502	rVB4	2603	4784	0.21%	0.030%
6	2.677	507	509	511	rBV2	633	391	0.02%	0.002%
7	2.719	518	522	524	rBV	527	353	0.02%	0.002%
8	2.735	524	527	534	rVB2	677	697	0.03%	0.004%
9	2.818	551	553	557	rVB3	446	267	0.01%	0.002%
10	2.847	557	562	564	rBV2	425	472	0.02%	0.003%
11	3.175	657	664	669	rVB3	522	491	0.02%	0.003%
12	3.214	669	676	682	rBV2	374	614	0.03%	0.004%
13	3.387	724	730	731	rBV2	407	338	0.01%	0.002%
14	3.449	743	749	755	rVB3	439	559	0.02%	0.003%
15	3.484	755	760	762	rBV2	324	274	0.01%	0.002%
16	3.709	827	830	836	rBV2	300	372	0.02%	0.002%
17	3.757	842	845	849	rBV3	323	327	0.01%	0.002%
18	3.892	873	887	926	rBV2	108393	480151	20.92%	2.987%
19	4.342	1009	1027	1068	rBV	364557	923361	40.24%	5.745%
20	4.953	1214	1217	1221	rVB4	587	414	0.02%	0.003%
21	4.979	1221	1225	1228	rBV	425	340	0.01%	0.002%
22	5.043	1228	1245	1292	rBV2	877449	2294719	100.00%	14.276%
23	5.413	1358	1360	1363	rVB3	521	293	0.01%	0.002%
24	5.506	1385	1389	1392	rVB3	478	345	0.02%	0.002%
25	5.612	1407	1422	1463	rBV	549742	1163304	50.69%	7.237%
26	5.841	1491	1493	1494	rBV	906	354	0.02%	0.002%
27	5.908	1503	1514	1532	rVB3	15759	33581	1.46%	0.209%
28	6.066	1547	1563	1599	rBV	495961	1044264	45.51%	6.497%
29	6.288	1630	1632	1635	rVB2	591	312	0.01%	0.002%
30	6.326	1641	1644	1649	rVB3	749	746	0.03%	0.005%
31	6.352	1649	1652	1655	rVB2	583	279	0.01%	0.002%
32	6.371	1655	1658	1660	rBV	573	396	0.02%	0.002%
33	6.419	1671	1673	1676	rBV2	436	310	0.01%	0.002%
34	6.477	1687	1691	1693	rVB3	392	269	0.01%	0.002%
35	6.529	1704	1707	1711	rVB2	301	262	0.01%	0.002%
36	6.616	1730	1734	1738	rBV2	373	398	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
 Data File : VV027088.D
 Acq On : 29 Jul 2022 16:31
 Operator : SY/MD
 Sample : N3880-17 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUH1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
 Title : VOC Analysis

37	6.715	1762	1765	1768	rBV2	416	289	0.01%	0.002%
38	6.751	1773	1776	1783	rVB4	524	551	0.02%	0.003%
39	6.985	1837	1849	1880	rBV	222759	433204	18.88%	2.695%
40	7.198	1911	1915	1916	rBV2	621	411	0.02%	0.003%
41	7.239	1925	1928	1929	rBV3	499	272	0.01%	0.002%
42	7.313	1937	1951	1982	rBV	945912	1688170	73.57%	10.503%
43	7.558	2025	2027	2031	rVB3	654	372	0.02%	0.002%
44	7.619	2036	2046	2080	rVV	157020	294771	12.85%	1.834%
45	7.895	2129	2132	2136	rBV2	450	300	0.01%	0.002%
46	7.934	2141	2144	2146	rBV3	363	259	0.01%	0.002%
47	7.976	2148	2157	2176	rVB2	16775	30056	1.31%	0.187%
48	8.050	2176	2180	2182	rBV2	475	345	0.02%	0.002%
49	8.091	2182	2193	2231	rBV	440738	1012969	44.14%	6.302%
50	8.326	2264	2266	2272	rVB4	1074	641	0.03%	0.004%
51	8.423	2291	2296	2306	rVB5	2890	4281	0.19%	0.027%
52	8.490	2313	2317	2318	rBV3	793	566	0.02%	0.004%
53	8.529	2324	2329	2331	rVB4	386	299	0.01%	0.002%
54	8.548	2331	2335	2338	rBV3	474	325	0.01%	0.002%
55	8.651	2364	2367	2373	rVB4	492	305	0.01%	0.002%
56	8.735	2391	2393	2398	rVB4	322	276	0.01%	0.002%
57	8.760	2398	2401	2407	rBV3	746	594	0.03%	0.004%
58	8.850	2417	2429	2467	rBV	852948	1417110	61.76%	8.816%
59	9.101	2505	2507	2509	rBV3	720	319	0.01%	0.002%
60	9.329	2574	2578	2582	rBV2	529	516	0.02%	0.003%
61	9.522	2632	2638	2640	rBV2	353	305	0.01%	0.002%
62	9.564	2648	2651	2655	rVB2	386	294	0.01%	0.002%
63	9.689	2687	2690	2693	rBV2	340	262	0.01%	0.002%
64	9.763	2707	2713	2716	rVB2	353	344	0.01%	0.002%
65	10.133	2822	2828	2835	rBV3	493	798	0.03%	0.005%
66	10.214	2837	2853	2880	rBV	722698	1153366	50.26%	7.176%
67	10.310	2880	2883	2887	rVB3	666	503	0.02%	0.003%
68	10.397	2906	2910	2911	rBV2	429	302	0.01%	0.002%
69	10.455	2922	2928	2929	rBV	353	328	0.01%	0.002%
70	10.477	2933	2935	2938	rVV	386	264	0.01%	0.002%
71	10.532	2950	2952	2955	rVB	457	254	0.01%	0.002%
72	10.574	2959	2965	2966	rBV3	451	394	0.02%	0.002%
73	10.715	3006	3009	3013	rVB2	399	268	0.01%	0.002%
74	10.789	3028	3032	3034	rBV2	382	306	0.01%	0.002%
75	10.841	3043	3048	3049	rBV3	353	298	0.01%	0.002%
76	10.850	3049	3051	3054	rVV2	666	471	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
 Data File : VV027088.D
 Acq On : 29 Jul 2022 16:31
 Operator : SY/MD
 Sample : N3880-17 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUH1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
 Title : VOC Analysis

77	10.866	3054	3056	3062	rVB3	544	422	0.02%	0.003%
78	10.924	3070	3074	3077	rBV3	334	259	0.01%	0.002%
79	11.033	3104	3108	3110	rBV	354	288	0.01%	0.002%
80	11.120	3131	3135	3140	rBV	384	382	0.02%	0.002%
81	11.146	3140	3143	3147	rBV2	423	280	0.01%	0.002%
82	11.249	3163	3175	3200	rBV	765338	1202555	52.41%	7.482%
83	11.529	3259	3262	3267	rVB2	722	651	0.03%	0.004%
84	11.622	3278	3291	3316	rBV	874111	1384982	60.36%	8.617%
85	11.950	3391	3393	3400	rVB2	405	355	0.02%	0.002%
86	12.178	3462	3464	3469	rBV3	495	370	0.02%	0.002%
87	12.204	3470	3472	3477	rVB3	407	297	0.01%	0.002%
88	12.233	3478	3481	3484	rVB2	424	264	0.01%	0.002%
89	12.258	3485	3489	3492	rBV4	637	395	0.02%	0.002%
90	12.869	3676	3679	3681	rBV	485	351	0.02%	0.002%
91	12.911	3690	3692	3696	rBV2	488	347	0.02%	0.002%
92	13.213	3784	3786	3789	rBV3	506	308	0.01%	0.002%
93	13.516	3871	3880	3890	rBV5	2646	3981	0.17%	0.025%
94	13.641	3914	3919	3924	rBV2	839	820	0.04%	0.005%
95	14.291	4118	4121	4123	rBV2	590	272	0.01%	0.002%
96	14.319	4127	4130	4132	rBV2	469	289	0.01%	0.002%
97	14.631	4224	4227	4228	rBV3	1055	570	0.02%	0.004%
98	14.773	4267	4271	4273	rVB3	593	423	0.02%	0.003%
99	15.191	4399	4401	4406	rBV5	567	471	0.02%	0.003%
100	15.956	4637	4639	4643	rBV4	1053	617	0.03%	0.004%




Sum of corrected areas: 16073518

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
Data File : VV027088.D
Acq On : 29 Jul 2022 16:31
Operator : SY/MD
Sample : N3880-17 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUH1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

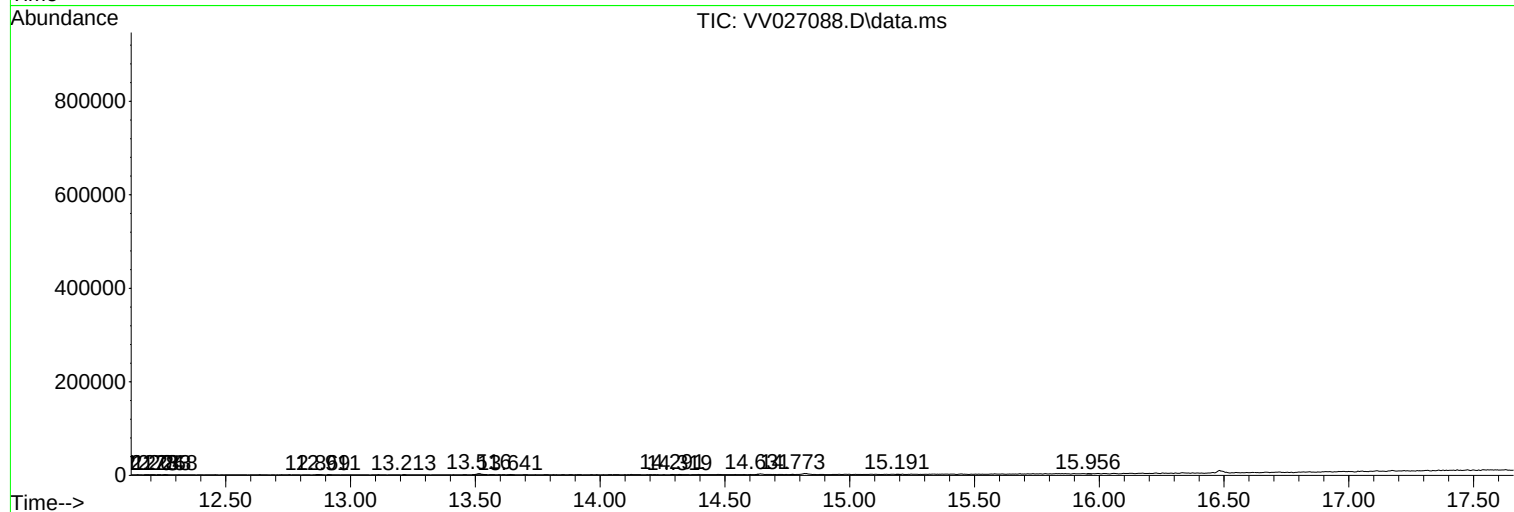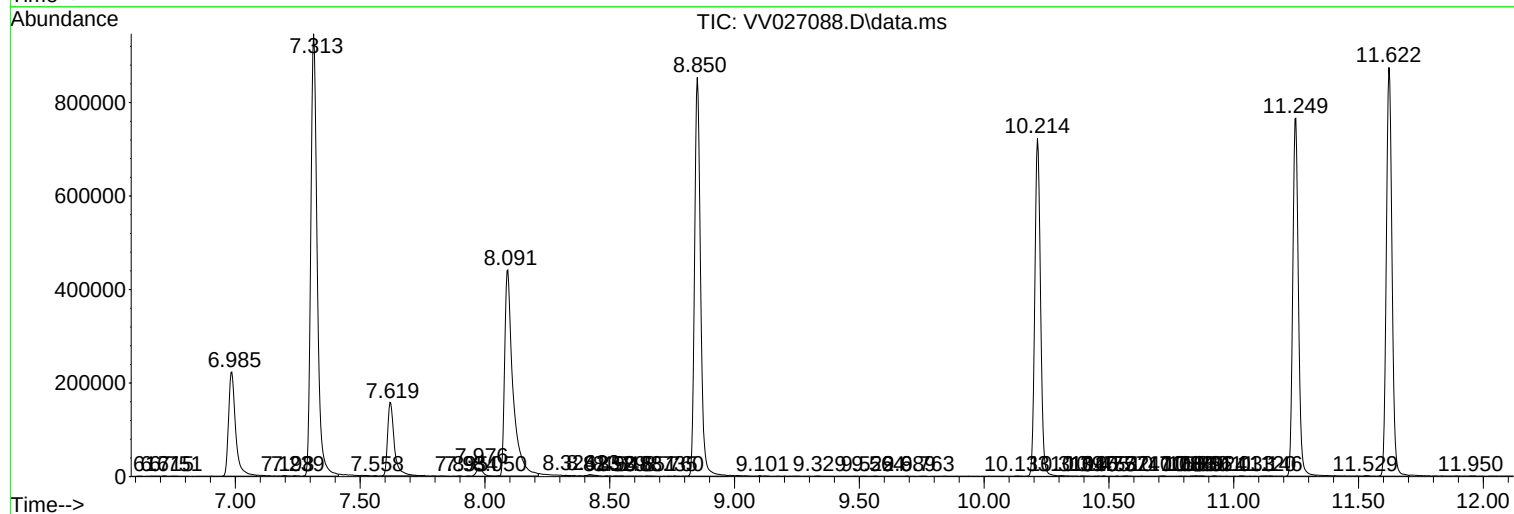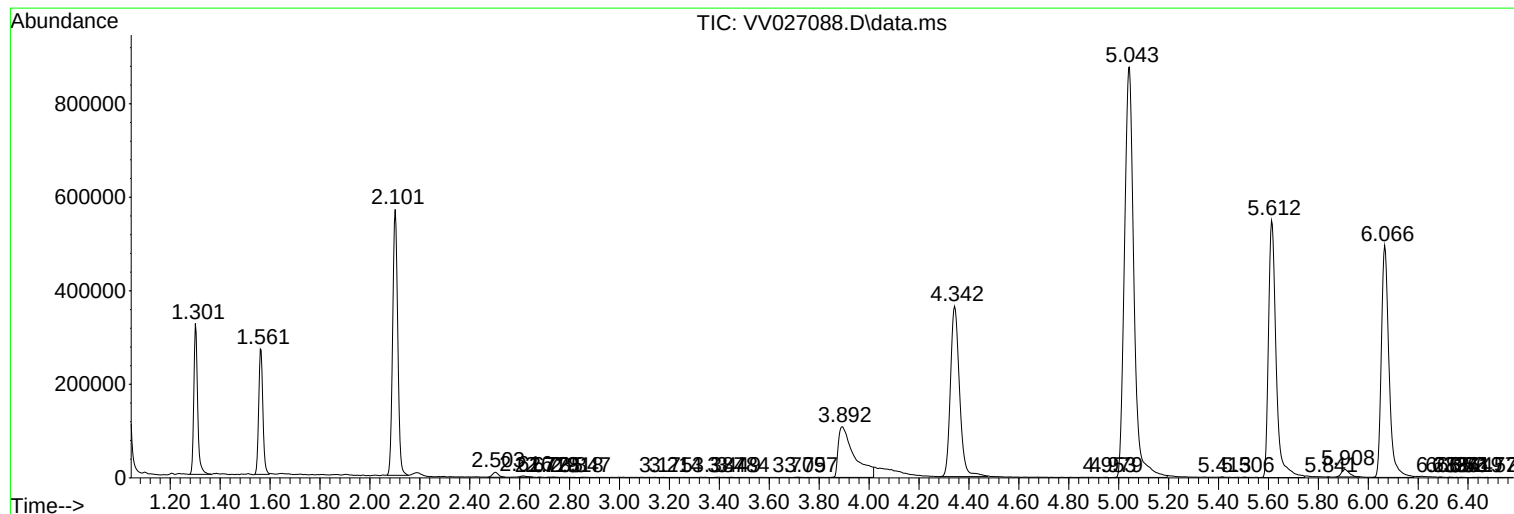

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
Data File : VV027088.D
Acq On : 29 Jul 2022 16:31
Operator : SY/MD
Sample : N3880-17 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUH1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
Data File : VV027088.D
Acq On : 29 Jul 2022 16:31
Operator : SY/MD
Sample : N3880-17 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUH1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc