

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
 Data File : VV027090.D
 Acq On : 29 Jul 2022 17:20
 Operator : SY/MD
 Sample : N3880-19 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUH8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
 Title : VOC Analysis

Signal : TIC: VV027090.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	74	81	102	rBV	325898	355962	15.18%	2.176%
2	1.564	155	163	176	rBV	276039	317249	13.53%	1.939%
3	2.101	320	330	347	rBV	591087	836518	35.68%	5.114%
4	2.503	445	455	470	rVB2	12220	21976	0.94%	0.134%
5	2.590	480	482	483	rVV2	702	367	0.02%	0.002%
6	2.616	483	490	501	rVB3	2349	4531	0.19%	0.028%
7	2.696	511	515	518	rVV4	447	451	0.02%	0.003%
8	2.831	554	557	560	rBV2	369	304	0.01%	0.002%
9	3.047	619	624	629	rVB3	282	318	0.01%	0.002%
10	3.204	669	673	676	rBV2	429	340	0.01%	0.002%
11	3.355	714	720	725	rVB2	410	523	0.02%	0.003%
12	3.394	725	732	736	rBV3	493	723	0.03%	0.004%
13	3.564	781	785	789	rBV2	271	304	0.01%	0.002%
14	3.786	851	854	860	rVB2	331	271	0.01%	0.002%
15	3.818	860	864	868	rBV2	298	306	0.01%	0.002%
16	3.889	875	886	915	rBV2	100499	386956	16.51%	2.365%
17	4.342	1010	1027	1052	rBV	367410	910723	38.85%	5.567%
18	4.574	1097	1099	1103	rBV2	439	369	0.02%	0.002%
19	4.696	1133	1137	1142	rBV2	519	433	0.02%	0.003%
20	4.757	1154	1156	1162	rVB3	701	556	0.02%	0.003%
21	4.786	1162	1165	1170	rBV4	383	353	0.02%	0.002%
22	4.928	1202	1209	1212	rBV3	585	654	0.03%	0.004%
23	4.960	1216	1219	1225	rVB2	643	621	0.03%	0.004%
24	5.040	1225	1244	1313	rBV2	883302	2344474	100.00%	14.332%
25	5.268	1313	1315	1319	rVB4	542	291	0.01%	0.002%
26	5.490	1376	1384	1385	rBV3	464	495	0.02%	0.003%
27	5.612	1410	1422	1464	rBV	566461	1203523	51.33%	7.357%
28	5.908	1502	1514	1531	rBV3	16303	37124	1.58%	0.227%
29	6.066	1550	1563	1599	rBV	498978	1045248	44.58%	6.390%
30	6.256	1620	1622	1627	rVB3	1130	972	0.04%	0.006%
31	6.320	1640	1642	1649	rVB3	592	488	0.02%	0.003%
32	6.371	1654	1658	1660	rVV4	410	279	0.01%	0.002%
33	6.452	1679	1683	1687	rVB3	401	359	0.02%	0.002%
34	6.481	1687	1692	1697	rBV3	416	484	0.02%	0.003%
35	6.571	1717	1720	1724	rVV3	412	337	0.01%	0.002%
36	6.593	1724	1727	1731	rVB2	408	321	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
 Data File : VV027090.D
 Acq On : 29 Jul 2022 17:20
 Operator : SY/MD
 Sample : N3880-19 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUH8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
 Title : VOC Analysis

37	6.657	1744	1747	1751	rBV3	434	406	0.02%	0.002%
38	6.693	1755	1758	1762	rBV3	324	271	0.01%	0.002%
39	6.747	1771	1775	1779	rBV3	381	293	0.01%	0.002%
40	6.783	1779	1786	1788	rBV2	299	308	0.01%	0.002%
41	6.982	1837	1848	1875	rBV	223465	433018	18.47%	2.647%
42	7.201	1913	1916	1918	rBV3	653	403	0.02%	0.002%
43	7.239	1924	1928	1936	rVB5	800	941	0.04%	0.006%
44	7.313	1938	1951	1989	rBV	970611	1768477	75.43%	10.811%
45	7.619	2036	2046	2077	rBV	159155	296809	12.66%	1.814%
46	7.805	2101	2104	2107	rBV3	473	286	0.01%	0.002%
47	7.924	2138	2141	2143	rBV2	515	378	0.02%	0.002%
48	7.937	2143	2145	2146	rVV2	610	314	0.01%	0.002%
49	7.947	2146	2148	2151	rVB2	729	322	0.01%	0.002%
50	7.982	2151	2159	2167	rBV5	2996	5007	0.21%	0.031%
51	8.091	2182	2193	2229	rBV	416986	997884	42.56%	6.100%
52	8.497	2316	2319	2325	rVB3	630	483	0.02%	0.003%
53	8.532	2325	2330	2333	rVB2	490	453	0.02%	0.003%
54	8.612	2351	2355	2357	rVB2	418	310	0.01%	0.002%
55	8.850	2417	2429	2454	rBV	904172	1495419	63.78%	9.142%
56	9.072	2495	2498	2501	rBV3	466	272	0.01%	0.002%
57	9.114	2507	2511	2513	rBV4	408	276	0.01%	0.002%
58	9.207	2534	2540	2543	rBV3	376	396	0.02%	0.002%
59	9.239	2547	2550	2557	rVB4	534	572	0.02%	0.003%
60	9.413	2602	2604	2607	rVV2	434	290	0.01%	0.002%
61	9.448	2610	2615	2618	rBV3	593	510	0.02%	0.003%
62	9.661	2675	2681	2682	rBV2	334	281	0.01%	0.002%
63	9.722	2694	2700	2705	rBV3	320	394	0.02%	0.002%
64	9.796	2719	2723	2724	rBV2	447	320	0.01%	0.002%
65	9.866	2741	2745	2749	rBV2	393	386	0.02%	0.002%
66	10.030	2790	2796	2798	rBV2	397	315	0.01%	0.002%
67	10.214	2840	2853	2884	rBV	727783	1149449	49.03%	7.027%
68	10.323	2884	2887	2889	rBV2	424	306	0.01%	0.002%
69	10.355	2895	2897	2903	rVB3	573	433	0.02%	0.003%
70	10.561	2957	2961	2964	rBV3	368	349	0.01%	0.002%
71	10.606	2972	2975	2980	rVB	426	415	0.02%	0.003%
72	10.680	2995	2998	3003	rBV3	324	314	0.01%	0.002%
73	10.706	3003	3006	3008	rBV2	332	278	0.01%	0.002%
74	10.744	3014	3018	3025	rBV3	324	497	0.02%	0.003%
75	11.117	3130	3134	3138	rBV2	387	419	0.02%	0.003%
76	11.136	3138	3140	3146	rVB2	352	314	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
 Data File : VV027090.D
 Acq On : 29 Jul 2022 17:20
 Operator : SY/MD
 Sample : N3880-19 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUH8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
 Title : VOC Analysis

77	11.249	3162	3175	3198	rBV	815356	1269860	54.16%	7.763%
78	11.622	3278	3291	3317	rBV	921408	1445249	61.64%	8.835%
79	11.963	3394	3397	3400	rBV2	476	328	0.01%	0.002%
80	12.053	3422	3425	3427	rBV	689	410	0.02%	0.003%
81	12.484	3556	3559	3564	rVB2	386	323	0.01%	0.002%
82	12.590	3589	3592	3594	rBV	669	437	0.02%	0.003%
83	12.750	3640	3642	3646	rVB	436	271	0.01%	0.002%
84	12.885	3682	3684	3691	rBV2	312	347	0.01%	0.002%
85	12.937	3695	3700	3703	rBV2	414	407	0.02%	0.002%
86	13.432	3852	3854	3857	rBV	435	288	0.01%	0.002%
87	13.451	3857	3860	3866	rVV3	537	443	0.02%	0.003%
88	13.519	3874	3881	3883	rBV3	670	754	0.03%	0.005%
89	13.577	3894	3899	3907	rVB4	523	577	0.02%	0.004%
90	13.680	3928	3931	3933	rBV3	540	396	0.02%	0.002%
91	13.760	3953	3956	3960	rBV3	541	519	0.02%	0.003%
92	13.853	3980	3985	3986	rBV2	385	355	0.02%	0.002%
93	14.024	4034	4038	4039	rBV2	417	300	0.01%	0.002%
94	14.156	4077	4079	4083	rBV2	512	407	0.02%	0.002%
95	14.647	4228	4232	4234	rBV3	959	764	0.03%	0.005%
96	14.786	4273	4275	4278	rBV2	650	377	0.02%	0.002%
97	15.127	4378	4381	4382	rBV2	678	405	0.02%	0.002%
98	15.217	4407	4409	4413	rBV3	709	539	0.02%	0.003%
99	15.246	4416	4418	4420	rBV2	557	292	0.01%	0.002%
100	15.409	4465	4469	4471	rBV3	640	574	0.02%	0.004%




Sum of corrected areas: 16358393

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
Data File : VV027090.D
Acq On : 29 Jul 2022 17:20
Operator : SY/MD
Sample : N3880-19 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUH8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

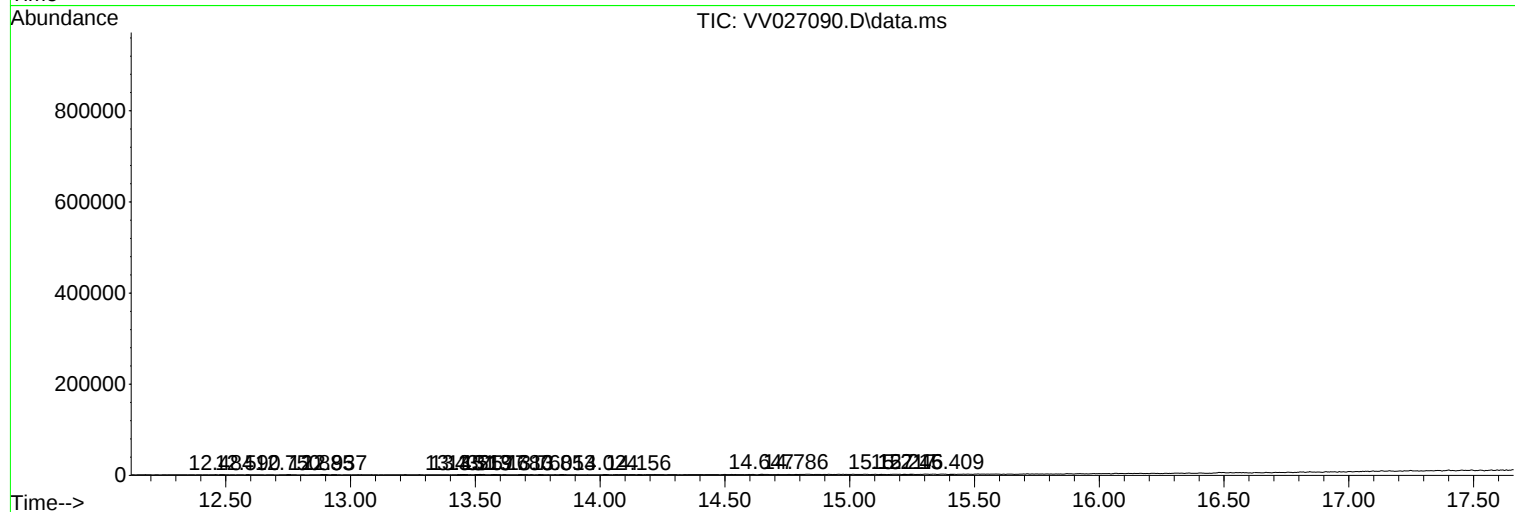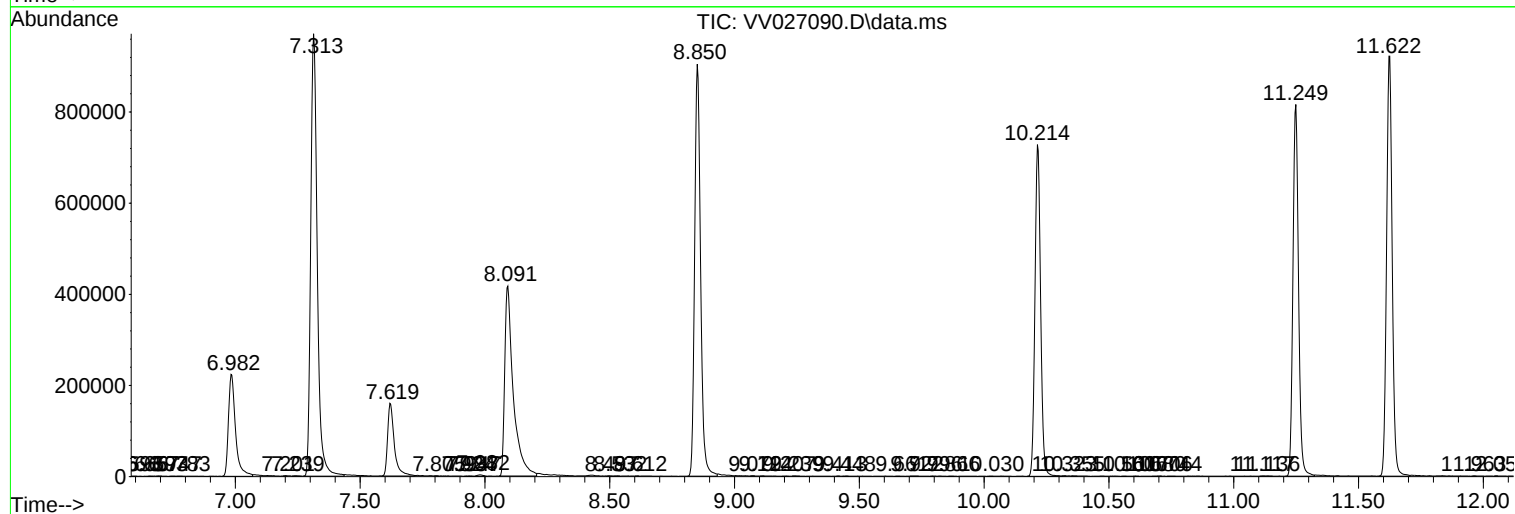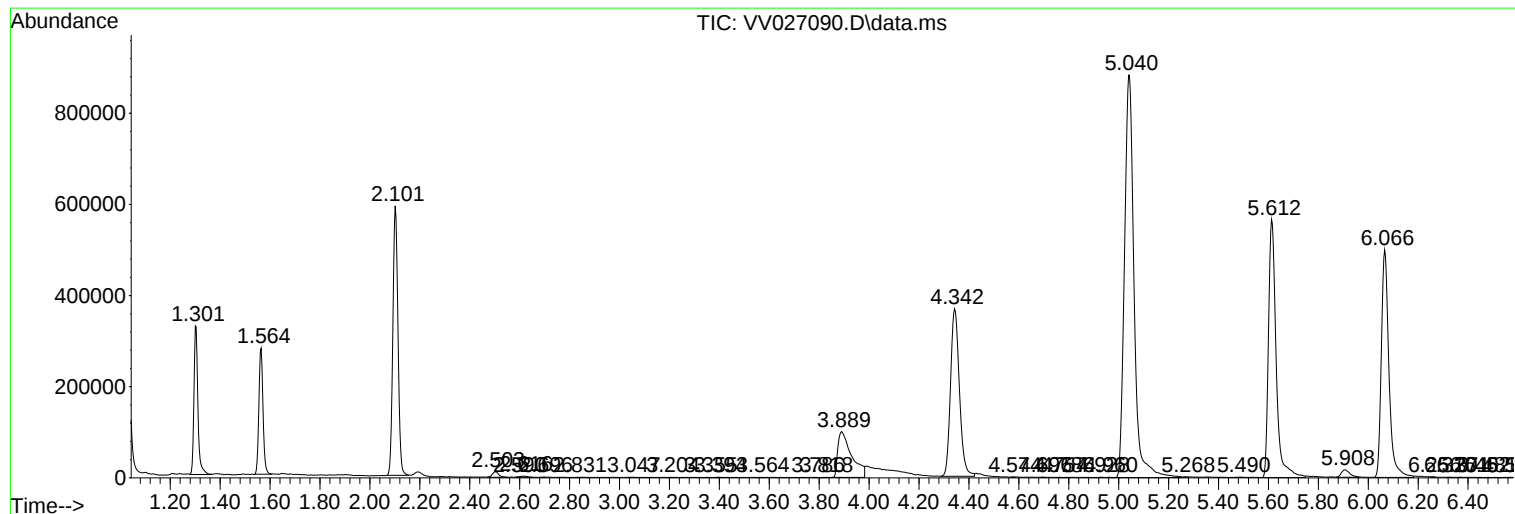

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
Data File : VV027090.D
Acq On : 29 Jul 2022 17:20
Operator : SY/MD
Sample : N3880-19 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUH8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
Data File : VV027090.D
Acq On : 29 Jul 2022 17:20
Operator : SY/MD
Sample : N3880-19 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUH8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------