

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
 Data File : VV027095.D
 Acq On : 29 Jul 2022 19:22
 Operator : SY/MD
 Sample : N3899-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUR1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
 Title : VOC Analysis

Signal : TIC: VV027095.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	101	rVB	317669	345961	14.64%	2.048%
2	1.564	156	163	180	rVB	278690	317166	13.42%	1.878%
3	2.101	321	330	345	rVB	575257	819801	34.69%	4.854%
4	2.863	566	567	568	rBV	448	108	0.00%	0.001%
5	2.873	568	570	575	rVB2	446	342	0.01%	0.002%
6	3.005	608	611	613	rBV2	315	182	0.01%	0.001%
7	3.053	623	626	629	rBV	245	185	0.01%	0.001%
8	3.082	632	635	638	rBV2	287	241	0.01%	0.001%
9	3.240	680	684	687	rBV2	373	336	0.01%	0.002%
10	3.323	708	710	713	rVB2	353	200	0.01%	0.001%
11	3.343	713	716	718	rBV	127	79	0.00%	0.000%
12	3.365	721	723	726	rVB	295	129	0.01%	0.001%
13	3.384	726	729	731	rBV2	138	99	0.00%	0.001%
14	3.558	779	783	784	rBV	359	187	0.01%	0.001%
15	3.600	793	796	797	rBV	168	89	0.00%	0.001%
16	3.709	828	830	834	rVB2	529	305	0.01%	0.002%
17	3.741	834	840	844	rBV2	381	477	0.02%	0.003%
18	3.802	856	859	860	rBV	173	89	0.00%	0.001%
19	3.834	867	869	871	rBV	98	59	0.00%	0.000%
20	3.886	876	885	923	rBV	90042	353393	14.96%	2.092%
21	4.342	1013	1027	1049	rBV	365955	889446	37.64%	5.266%
22	4.725	1143	1146	1147	rBV	258	146	0.01%	0.001%
23	4.777	1161	1162	1164	rBV2	444	108	0.00%	0.001%
24	4.931	1208	1210	1211	rBV	462	120	0.01%	0.001%
25	5.040	1227	1244	1293	rBV2	889839	2363033	100.00%	13.991%
26	5.497	1383	1386	1388	rBV3	358	248	0.01%	0.001%
27	5.532	1395	1397	1399	rBV2	409	178	0.01%	0.001%
28	5.561	1404	1406	1409	rBV2	558	213	0.01%	0.001%
29	5.613	1409	1422	1462	rBV	598615	1263715	53.48%	7.482%
30	6.005	1541	1544	1547	rVB2	583	421	0.02%	0.002%
31	6.066	1549	1563	1604	rBV	498878	1067425	45.17%	6.320%
32	6.307	1635	1638	1642	rVB2	615	359	0.02%	0.002%
33	6.326	1642	1644	1645	rBV	416	164	0.01%	0.001%
34	6.365	1654	1656	1659	rVB	367	198	0.01%	0.001%
35	6.397	1664	1666	1667	rBV	248	111	0.00%	0.001%
36	6.423	1672	1674	1676	rVB	284	103	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
 Data File : VV027095.D
 Acq On : 29 Jul 2022 19:22
 Operator : SY/MD
 Sample : N3899-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUR1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
 Title : VOC Analysis

37	6.445	1676	1681	1683	rBV2	398	311	0.01%	0.002%
38	6.471	1687	1689	1690	rBV2	94	28	0.00%	0.000%
39	6.526	1700	1706	1709	rBV2	498	452	0.02%	0.003%
40	6.545	1710	1712	1714	rVB2	452	153	0.01%	0.001%
41	6.567	1714	1719	1724	rBV3	508	571	0.02%	0.003%
42	6.600	1725	1729	1731	rBV2	265	207	0.01%	0.001%
43	6.648	1739	1744	1746	rBV3	668	636	0.03%	0.004%
44	6.741	1771	1773	1774	rBV	192	81	0.00%	0.000%
45	6.834	1800	1802	1805	rVB2	209	123	0.01%	0.001%
46	6.857	1805	1809	1810	rBV	338	191	0.01%	0.001%
47	6.934	1830	1833	1835	rBV2	277	153	0.01%	0.001%
48	6.982	1836	1848	1880	rBV	231835	451236	19.10%	2.672%
49	7.313	1939	1951	1981	rBV	1015991	1813075	76.73%	10.734%
50	7.619	2036	2046	2073	rBV	160998	300569	12.72%	1.780%
51	7.892	2129	2131	2132	rBV2	329	140	0.01%	0.001%
52	7.934	2138	2144	2147	rBV4	629	663	0.03%	0.004%
53	7.979	2155	2158	2164	rVB3	1323	1321	0.06%	0.008%
54	8.027	2171	2173	2174	rBV	145	57	0.00%	0.000%
55	8.091	2182	2193	2233	rBV	434606	1039977	44.01%	6.157%
56	8.461	2306	2308	2311	rBV2	535	429	0.02%	0.003%
57	8.574	2340	2343	2347	rBV4	491	406	0.02%	0.002%
58	8.696	2380	2381	2383	rVB	530	147	0.01%	0.001%
59	8.709	2383	2385	2388	rBV2	502	321	0.01%	0.002%
60	8.728	2388	2391	2396	rVV3	634	432	0.02%	0.003%
61	8.767	2402	2403	2404	rBV	257	71	0.00%	0.000%
62	8.780	2404	2407	2409	rVV2	269	207	0.01%	0.001%
63	8.850	2417	2429	2457	rBV	931874	1556325	65.86%	9.214%
64	9.281	2560	2563	2565	rBV2	396	226	0.01%	0.001%
65	9.352	2581	2585	2588	rBV2	402	316	0.01%	0.002%
66	9.481	2621	2625	2626	rBV2	221	144	0.01%	0.001%
67	9.551	2645	2647	2649	rBV2	310	167	0.01%	0.001%
68	9.583	2655	2657	2658	rBV	286	144	0.01%	0.001%
69	9.667	2679	2683	2685	rBV	347	218	0.01%	0.001%
70	9.715	2695	2698	2700	rBV3	332	228	0.01%	0.001%
71	9.828	2731	2733	2735	rBV	251	140	0.01%	0.001%
72	9.853	2739	2741	2742	rBV	184	44	0.00%	0.000%
73	9.873	2745	2747	2749	rVB	303	115	0.00%	0.001%
74	9.889	2749	2752	2755	rBV2	186	123	0.01%	0.001%
75	10.149	2829	2833	2840	rBV2	326	407	0.02%	0.002%
76	10.214	2840	2853	2879	rBV	746947	1190766	50.39%	7.050%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
 Data File : VV027095.D
 Acq On : 29 Jul 2022 19:22
 Operator : SY/MD
 Sample : N3899-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUR1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
 Title : VOC Analysis

77	10.371	2900	2902	2906	rVB4	485	288	0.01%	0.002%
78	10.480	2934	2936	2940	rVB	387	220	0.01%	0.001%
79	10.509	2942	2945	2946	rBV2	171	102	0.00%	0.001%
80	10.574	2961	2965	2969	rBV3	792	857	0.04%	0.005%
81	10.738	3013	3016	3019	rBV2	452	294	0.01%	0.002%
82	10.767	3023	3025	3027	rBV2	164	87	0.00%	0.001%
83	10.796	3032	3034	3035	rBV	236	92	0.00%	0.001%
84	10.892	3062	3064	3068	rVB3	557	251	0.01%	0.001%
85	10.927	3071	3075	3077	rBV	459	353	0.01%	0.002%
86	11.021	3102	3104	3110	rBV2	289	319	0.01%	0.002%
87	11.066	3115	3118	3121	rBV	226	162	0.01%	0.001%
88	11.088	3121	3125	3128	rBV2	263	273	0.01%	0.002%
89	11.140	3138	3141	3142	rBV2	350	194	0.01%	0.001%
90	11.249	3163	3175	3203	rBV	896278	1402276	59.34%	8.302%
91	11.538	3256	3265	3279	rBV7	7136	13500	0.57%	0.080%
92	11.622	3279	3291	3323	rBV	989116	1545328	65.40%	9.149%
93	11.783	3339	3341	3342	rBV	816	238	0.01%	0.001%
94	12.030	3416	3418	3422	rBV2	455	241	0.01%	0.001%
95	13.268	3801	3803	3809	rVB3	1014	789	0.03%	0.005%
96	13.432	3851	3854	3858	rBV2	478	342	0.01%	0.002%
97	13.506	3868	3877	3889	rBV	31675	51140	2.16%	0.303%
98	14.580	4205	4211	4218	rVB2	6755	9132	0.39%	0.054%
99	14.635	4220	4228	4243	rVB	31703	49679	2.10%	0.294%
100	14.815	4275	4284	4303	rBV2	15560	27279	1.15%	0.162%




Sum of corrected areas: 16890172

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
Data File : VV027095.D
Acq On : 29 Jul 2022 19:22
Operator : SY/MD
Sample : N3899-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUR1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

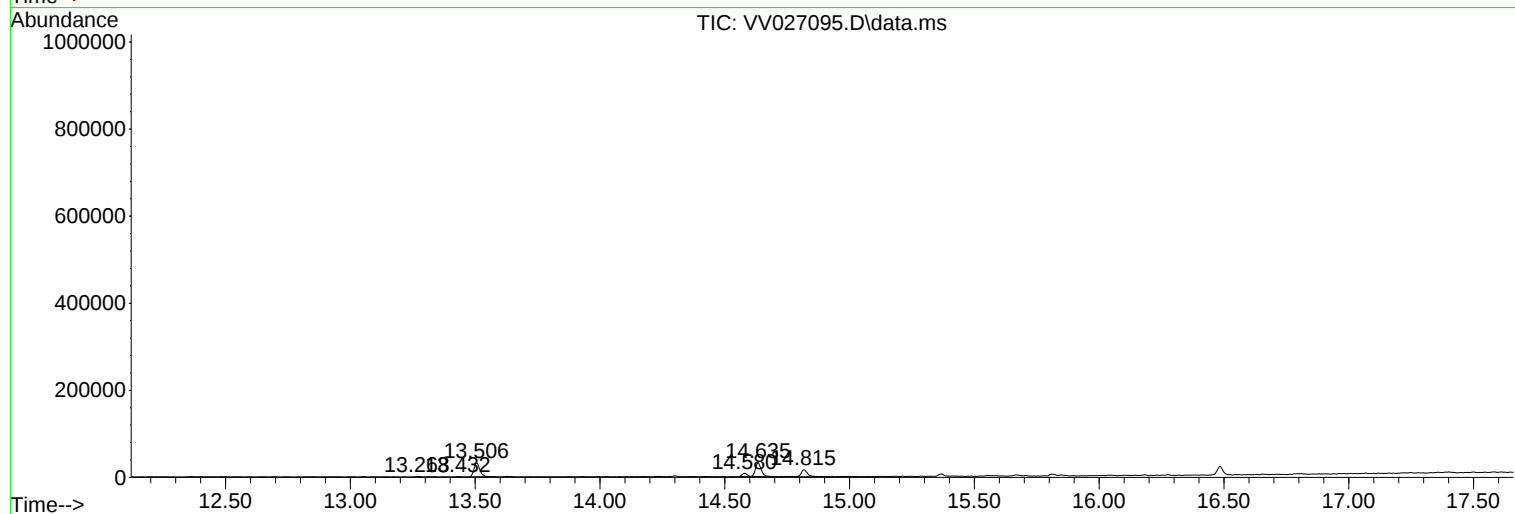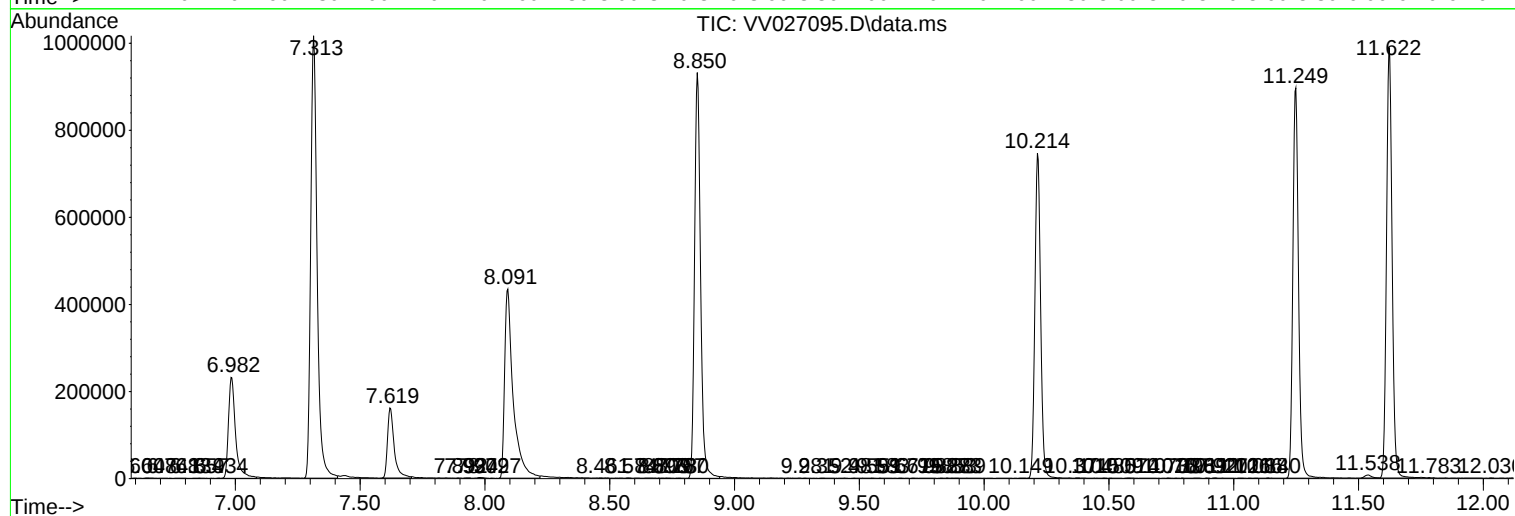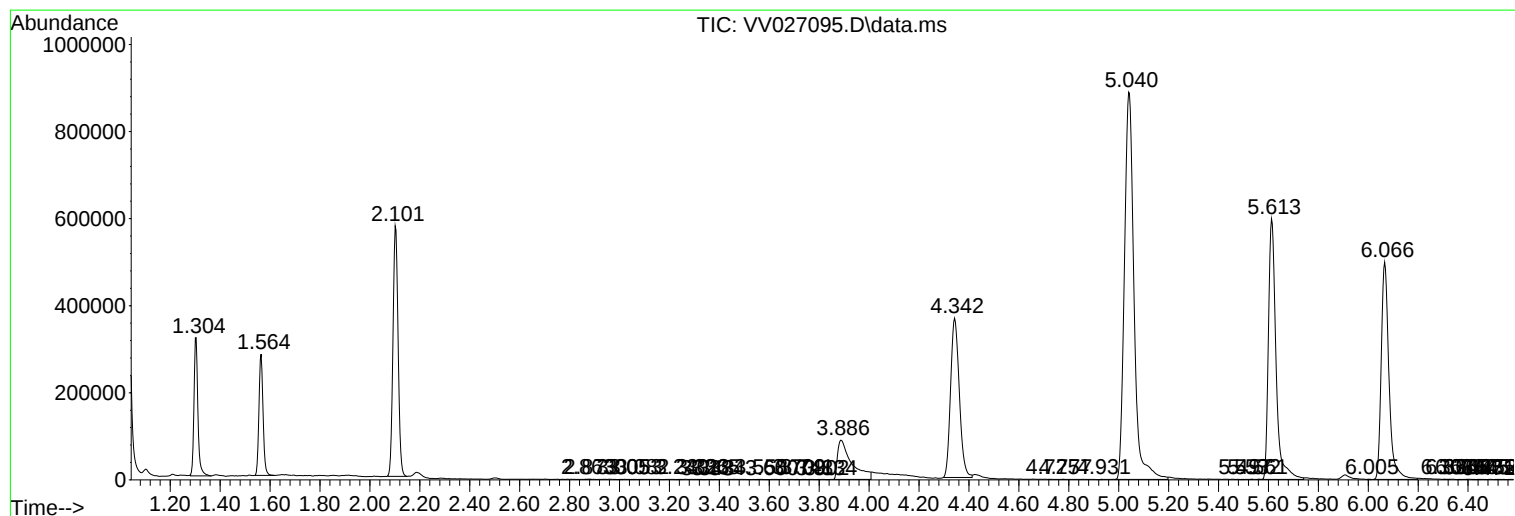

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
Data File : VV027095.D
Acq On : 29 Jul 2022 19:22
Operator : SY/MD
Sample : N3899-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUR1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
Data File : VV027095.D
Acq On : 29 Jul 2022 19:22
Operator : SY/MD
Sample : N3899-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUR1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc