

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
 Data File : VV027096.D
 Acq On : 29 Jul 2022 19:47
 Operator : SY/MD
 Sample : N3899-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUR2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
 Title : VOC Analysis

Signal : TIC: VV027096.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	100	rVB	328424	345074	14.76%	2.061%
2	1.564	156	163	180	rVB	277679	317733	13.59%	1.897%
3	2.101	321	330	346	rVB	571824	814711	34.86%	4.865%
4	2.895	574	577	582	rBV2	298	264	0.01%	0.002%
5	3.021	612	616	618	rBV	471	377	0.02%	0.002%
6	3.095	634	639	643	rBV	328	329	0.01%	0.002%
7	3.207	667	674	676	rBV2	397	308	0.01%	0.002%
8	3.291	695	700	703	rBV3	508	437	0.02%	0.003%
9	3.355	716	720	722	rBV	434	329	0.01%	0.002%
10	3.413	733	738	742	rBV2	279	337	0.01%	0.002%
11	3.484	758	760	763	rBV	307	161	0.01%	0.001%
12	3.500	763	765	770	rVB2	409	326	0.01%	0.002%
13	3.651	810	812	814	rBV2	214	142	0.01%	0.001%
14	3.754	840	844	846	rBV	306	246	0.01%	0.001%
15	3.889	875	886	917	rBV	92612	335500	14.35%	2.003%
16	4.342	1013	1027	1049	rBV	369915	897136	38.38%	5.357%
17	4.754	1152	1155	1159	rBV3	421	331	0.01%	0.002%
18	4.844	1182	1183	1186	rBV2	164	60	0.00%	0.000%
19	5.043	1227	1245	1282	rBV2	887464	2337271	100.00%	13.957%
20	5.400	1354	1356	1358	rBV2	444	254	0.01%	0.002%
21	5.535	1396	1398	1400	rBV2	360	159	0.01%	0.001%
22	5.612	1410	1422	1459	rBV	601154	1264003	54.08%	7.548%
23	6.066	1549	1563	1600	rBV	499380	1059183	45.32%	6.325%
24	6.397	1664	1666	1667	rBV	266	108	0.00%	0.001%
25	6.426	1672	1675	1678	rBV3	357	295	0.01%	0.002%
26	6.487	1692	1694	1699	rBV3	401	301	0.01%	0.002%
27	6.526	1703	1706	1707	rBV	106	53	0.00%	0.000%
28	6.561	1713	1717	1719	rBV	294	175	0.01%	0.001%
29	6.625	1735	1737	1739	rBV3	191	104	0.00%	0.001%
30	6.744	1772	1774	1775	rBV	201	60	0.00%	0.000%
31	6.789	1785	1788	1790	rBV2	462	215	0.01%	0.001%
32	6.821	1795	1798	1801	rBV	325	203	0.01%	0.001%
33	6.837	1801	1803	1805	rBV	383	163	0.01%	0.001%
34	6.863	1808	1811	1812	rBV	185	105	0.00%	0.001%
35	6.889	1817	1819	1822	rVB	255	134	0.01%	0.001%
36	6.902	1822	1823	1824	rVB	119	23	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
 Data File : VV027096.D
 Acq On : 29 Jul 2022 19:47
 Operator : SY/MD
 Sample : N3899-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUR2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
 Title : VOC Analysis

37	6.911	1824	1826	1827	rBV	188	82	0.00%	0.000%
38	6.921	1827	1829	1832	rBV2	154	97	0.00%	0.001%
39	6.937	1832	1834	1836	rVB2	315	139	0.01%	0.001%
40	6.985	1836	1849	1884	rBV	229125	449696	19.24%	2.685%
41	7.313	1939	1951	1987	rBV	1006998	1801808	77.09%	10.759%
42	7.619	2036	2046	2080	rBV	159229	301691	12.91%	1.802%
43	7.908	2133	2136	2139	rBV3	478	342	0.01%	0.002%
44	7.982	2151	2159	2165	rVB5	1312	2294	0.10%	0.014%
45	8.037	2173	2176	2178	rBV	394	264	0.01%	0.002%
46	8.091	2182	2193	2241	rBV	441259	1073401	45.93%	6.410%
47	8.715	2385	2387	2390	rBV3	250	124	0.01%	0.001%
48	8.760	2398	2401	2402	rBV	242	139	0.01%	0.001%
49	8.783	2406	2408	2409	rBV	240	82	0.00%	0.000%
50	8.850	2417	2429	2459	rBV	947215	1572813	67.29%	9.392%
51	9.249	2550	2553	2557	rVB3	496	373	0.02%	0.002%
52	9.275	2558	2561	2562	rBV3	223	120	0.01%	0.001%
53	9.339	2579	2581	2583	rBV	317	144	0.01%	0.001%
54	9.381	2593	2594	2597	rBV2	288	141	0.01%	0.001%
55	9.403	2597	2601	2604	rVB2	367	270	0.01%	0.002%
56	9.432	2604	2610	2612	rBV2	452	421	0.02%	0.003%
57	9.474	2619	2623	2625	rBV3	289	182	0.01%	0.001%
58	9.541	2641	2644	2648	rBV	303	272	0.01%	0.002%
59	9.725	2696	2701	2704	rBV2	361	342	0.01%	0.002%
60	9.750	2704	2709	2714	rBV2	395	396	0.02%	0.002%
61	9.779	2714	2718	2722	rBV3	284	337	0.01%	0.002%
62	9.818	2726	2730	2731	rBV	329	206	0.01%	0.001%
63	9.860	2741	2743	2745	rBV	279	151	0.01%	0.001%
64	9.879	2745	2749	2754	rVV2	363	427	0.02%	0.003%
65	9.902	2754	2756	2759	rBV	179	99	0.00%	0.001%
66	9.959	2770	2774	2775	rBV2	201	147	0.01%	0.001%
67	10.120	2821	2824	2826	rBV2	246	168	0.01%	0.001%
68	10.213	2840	2853	2874	rBV	751494	1194196	51.09%	7.131%
69	10.422	2916	2918	2922	rBV3	332	191	0.01%	0.001%
70	10.815	3037	3040	3041	rBV	253	125	0.01%	0.001%
71	10.905	3066	3068	3074	rVB	646	529	0.02%	0.003%
72	10.934	3075	3077	3079	rBV3	239	156	0.01%	0.001%
73	11.056	3113	3115	3118	rVB2	217	89	0.00%	0.001%
74	11.085	3120	3124	3127	rBV3	308	268	0.01%	0.002%
75	11.107	3127	3131	3134	rBV2	346	346	0.01%	0.002%
76	11.162	3145	3148	3151	rBV	300	186	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
 Data File : VV027096.D
 Acq On : 29 Jul 2022 19:47
 Operator : SY/MD
 Sample : N3899-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUR2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M

Title : VOC Analysis

77	11.249	3163	3175	3201	rBV	879999	1388123	59.39%	8.289%
78	11.535	3255	3264	3275	rBV2	12355	21685	0.93%	0.129%
79	11.622	3280	3291	3318	rVB	961348	1524121	65.21%	9.101%
80	11.828	3353	3355	3356	rBV	513	196	0.01%	0.001%
81	12.210	3472	3474	3475	rBV	277	110	0.00%	0.001%
82	12.583	3587	3590	3595	rBV2	431	438	0.02%	0.003%
83	12.799	3653	3657	3662	rBV3	496	745	0.03%	0.004%
84	12.911	3689	3692	3693	rBV	379	251	0.01%	0.001%
85	13.255	3798	3799	3800	rBV	703	155	0.01%	0.001%
86	13.506	3871	3877	3889	rVB	11024	17549	0.75%	0.105%
87	14.638	4223	4229	4244	rVB2	8741	13118	0.56%	0.078%




Sum of corrected areas: 16746355

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
Data File : VV027096.D
Acq On : 29 Jul 2022 19:47
Operator : SY/MD
Sample : N3899-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUR2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

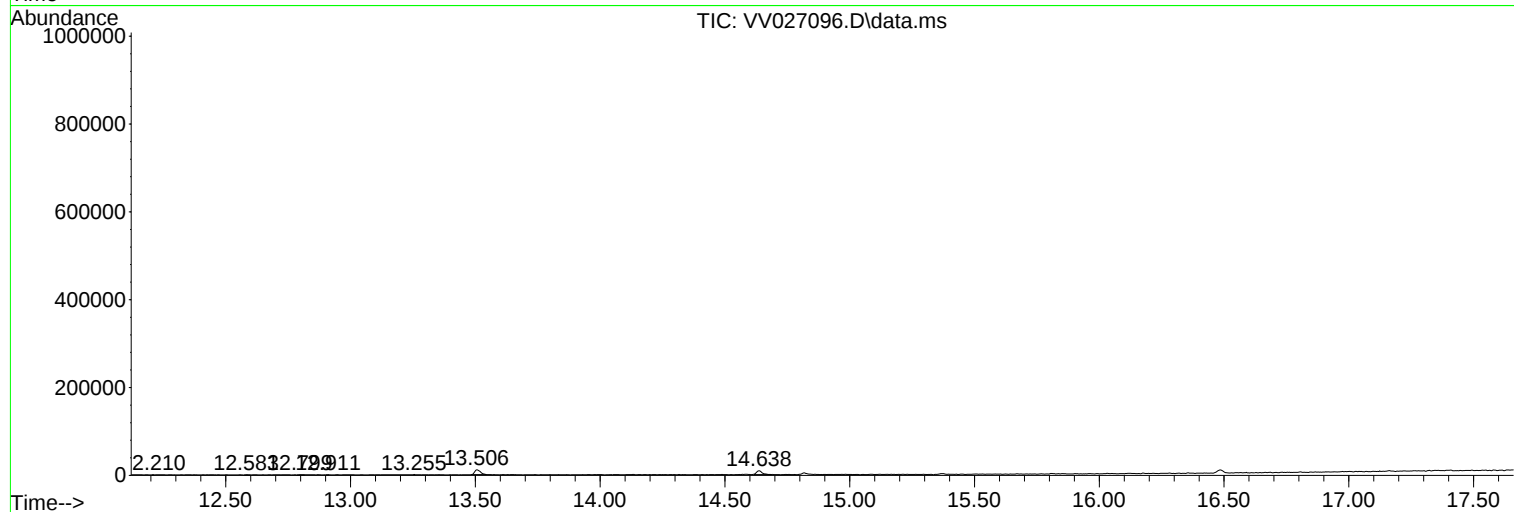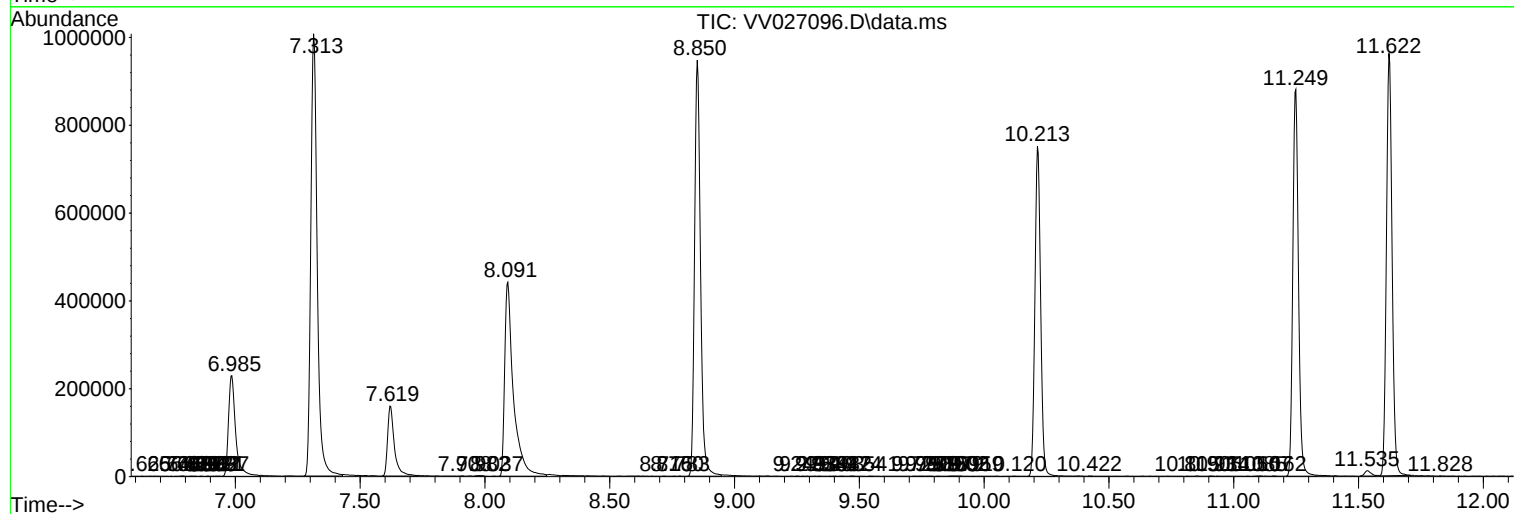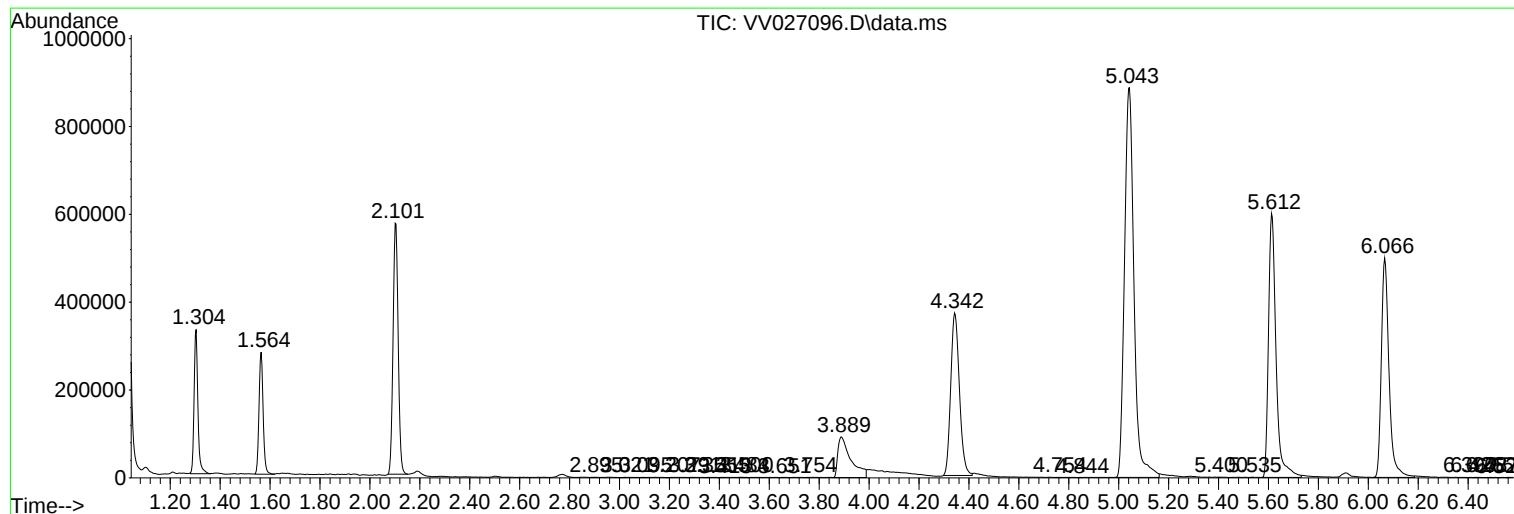

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
Data File : VV027096.D
Acq On : 29 Jul 2022 19:47
Operator : SY/MD
Sample : N3899-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUR2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
Data File : VV027096.D
Acq On : 29 Jul 2022 19:47
Operator : SY/MD
Sample : N3899-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUR2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------