

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
 Data File : VV027097.D
 Acq On : 29 Jul 2022 20:11
 Operator : SY/MD
 Sample : N3899-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUS2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
 Title : VOC Analysis

Signal : TIC: VV027097.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	75	81	101	rVB	313912	339327	14.40%	2.027%
2	1.564	155	163	179	rVB	279264	322296	13.67%	1.926%
3	2.101	320	330	345	rBV	567546	808619	34.31%	4.831%
4	2.500	446	454	463	rBV3	6699	10209	0.43%	0.061%
5	2.641	491	498	502	rBV2	388	587	0.02%	0.004%
6	2.748	528	531	535	rBV2	488	373	0.02%	0.002%
7	2.889	571	575	576	rBV2	363	243	0.01%	0.001%
8	2.912	579	582	585	rVB2	319	222	0.01%	0.001%
9	3.079	629	634	636	rBV2	408	314	0.01%	0.002%
10	3.336	712	714	721	rVB2	819	519	0.02%	0.003%
11	3.403	731	735	738	rVB2	321	274	0.01%	0.002%
12	3.490	758	762	765	rVV3	360	374	0.02%	0.002%
13	3.558	780	783	789	rVV2	436	497	0.02%	0.003%
14	3.770	846	849	857	rVB2	309	383	0.02%	0.002%
15	3.812	857	862	865	rBV2	453	325	0.01%	0.002%
16	3.889	876	886	913	rBV	93350	325270	13.80%	1.943%
17	4.342	1010	1027	1051	rBV	373604	932982	39.59%	5.574%
18	4.680	1130	1132	1135	rVB2	523	262	0.01%	0.002%
19	4.702	1137	1139	1145	rVB3	430	453	0.02%	0.003%
20	4.773	1157	1161	1163	rBV2	349	262	0.01%	0.002%
21	4.825	1173	1177	1180	rBV4	807	699	0.03%	0.004%
22	4.857	1185	1187	1190	rVB3	576	277	0.01%	0.002%
23	4.918	1204	1206	1209	rVB2	457	242	0.01%	0.001%
24	4.950	1213	1216	1219	rVB2	311	214	0.01%	0.001%
25	5.040	1227	1244	1288	rBV2	903388	2356850	100.00%	14.082%
26	5.275	1315	1317	1321	rVB3	640	351	0.01%	0.002%
27	5.297	1321	1324	1327	rBV3	478	314	0.01%	0.002%
28	5.355	1340	1342	1346	rVB4	466	281	0.01%	0.002%
29	5.400	1353	1356	1358	rBV2	382	220	0.01%	0.001%
30	5.612	1410	1422	1460	rBV	603482	1266829	53.75%	7.569%
31	5.905	1502	1513	1531	rVV5	13370	30280	1.28%	0.181%
32	6.066	1549	1563	1600	rBV	505525	1072789	45.52%	6.410%
33	6.339	1646	1648	1652	rVV4	780	471	0.02%	0.003%
34	6.378	1657	1660	1666	rVB3	422	331	0.01%	0.002%
35	6.484	1688	1693	1697	rBV2	699	838	0.04%	0.005%
36	6.628	1735	1738	1739	rBV2	437	260	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
 Data File : VV027097.D
 Acq On : 29 Jul 2022 20:11
 Operator : SY/MD
 Sample : N3899-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUS2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
 Title : VOC Analysis

37	6.924	1827	1830	1833	rBV	484	298	0.01%	0.002%
38	6.985	1837	1849	1877	rBV	230128	448058	19.01%	2.677%
39	7.162	1902	1904	1908	rVB3	499	262	0.01%	0.002%
40	7.191	1910	1913	1916	rBV3	397	311	0.01%	0.002%
41	7.313	1939	1951	1981	rBV	996935	1784604	75.72%	10.663%
42	7.561	2026	2028	2030	rVB3	537	227	0.01%	0.001%
43	7.619	2036	2046	2071	rBV	163110	302215	12.82%	1.806%
44	7.863	2120	2122	2125	rVB3	628	344	0.01%	0.002%
45	7.882	2126	2128	2135	rVB3	679	583	0.02%	0.003%
46	7.921	2135	2140	2143	rBV4	598	561	0.02%	0.003%
47	7.979	2151	2158	2162	rBV8	1669	2332	0.10%	0.014%
48	8.091	2182	2193	2240	rBV	454715	1070009	45.40%	6.393%
49	8.323	2263	2265	2272	rVB5	675	524	0.02%	0.003%
50	8.458	2304	2307	2310	rVB3	560	348	0.01%	0.002%
51	8.474	2310	2312	2315	rVB2	532	243	0.01%	0.001%
52	8.796	2409	2412	2415	rBV2	392	242	0.01%	0.001%
53	8.850	2417	2429	2468	rBV	944334	1567193	66.50%	9.364%
54	8.982	2468	2470	2476	rVB3	984	850	0.04%	0.005%
55	9.075	2494	2499	2504	rVB6	685	747	0.03%	0.004%
56	9.101	2504	2507	2512	rVB3	562	532	0.02%	0.003%
57	9.127	2512	2515	2518	rBV3	381	276	0.01%	0.002%
58	9.278	2560	2562	2565	rVB2	498	248	0.01%	0.001%
59	9.522	2635	2638	2643	rVB2	338	268	0.01%	0.002%
60	9.561	2647	2650	2654	rBV2	379	283	0.01%	0.002%
61	9.612	2662	2666	2670	rVB2	392	299	0.01%	0.002%
62	9.802	2723	2725	2731	rVB2	453	322	0.01%	0.002%
63	9.828	2731	2733	2740	rVB2	547	437	0.02%	0.003%
64	9.943	2766	2769	2771	rVV	302	236	0.01%	0.001%
65	10.133	2823	2828	2831	rVB3	483	402	0.02%	0.002%
66	10.213	2841	2853	2873	rBV	753056	1195628	50.73%	7.144%
67	10.374	2899	2903	2912	rVB4	564	795	0.03%	0.005%
68	10.516	2944	2947	2953	rVB2	331	303	0.01%	0.002%
69	10.580	2962	2967	2972	rVB4	1000	999	0.04%	0.006%
70	10.824	3038	3043	3044	rBV2	324	239	0.01%	0.001%
71	10.853	3049	3052	3058	rVB4	1031	878	0.04%	0.005%
72	10.950	3076	3082	3085	rBV2	351	387	0.02%	0.002%
73	10.982	3090	3092	3099	rVB2	601	372	0.02%	0.002%
74	11.159	3144	3147	3151	rBV2	369	226	0.01%	0.001%
75	11.249	3162	3175	3195	rBV	863258	1342542	56.96%	8.022%
76	11.538	3255	3265	3276	rBV5	7606	13924	0.59%	0.083%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
 Data File : VV027097.D
 Acq On : 29 Jul 2022 20:11
 Operator : SY/MD
 Sample : N3899-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUS2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
 Title : VOC Analysis

77	11.622	3278	3291	3311	rBV	956146	1496752	63.51%	8.943%
78	11.812	3344	3350	3351	rBV2	639	603	0.03%	0.004%
79	12.001	3404	3409	3413	rVB2	403	366	0.02%	0.002%
80	12.175	3460	3463	3466	rVB	346	229	0.01%	0.001%
81	12.361	3518	3521	3525	rVB3	530	394	0.02%	0.002%
82	12.384	3525	3528	3532	rBV2	379	305	0.01%	0.002%
83	12.551	3577	3580	3585	rVB2	386	265	0.01%	0.002%
84	12.580	3585	3589	3592	rBV3	430	388	0.02%	0.002%
85	12.998	3717	3719	3723	rVB	371	239	0.01%	0.001%
86	13.410	3844	3847	3851	rBV2	447	396	0.02%	0.002%
87	13.445	3855	3858	3860	rBV2	466	288	0.01%	0.002%
88	13.509	3871	3878	3892	rBV3	5239	9241	0.39%	0.055%
89	13.622	3911	3913	3916	rVB3	549	246	0.01%	0.001%
90	13.741	3947	3950	3953	rBV3	555	422	0.02%	0.003%
91	13.799	3965	3968	3974	rBV3	775	734	0.03%	0.004%
92	13.847	3980	3983	3986	rVB3	530	302	0.01%	0.002%
93	14.162	4078	4081	4083	rBV2	375	251	0.01%	0.001%
94	14.323	4129	4131	4137	rVB3	638	357	0.02%	0.002%
95	14.377	4144	4148	4149	rBV2	392	316	0.01%	0.002%
96	14.612	4218	4221	4222	rBV2	568	284	0.01%	0.002%
97	14.641	4222	4230	4243	rVV4	3919	6800	0.29%	0.041%
98	14.737	4256	4260	4262	rBV2	608	428	0.02%	0.003%
99	14.811	4280	4283	4288	rBV4	1455	1561	0.07%	0.009%
100	15.165	4389	4393	4397	rBV3	905	907	0.04%	0.005%




Sum of corrected areas: 16736658

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
Data File : VV027097.D
Acq On : 29 Jul 2022 20:11
Operator : SY/MD
Sample : N3899-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUS2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

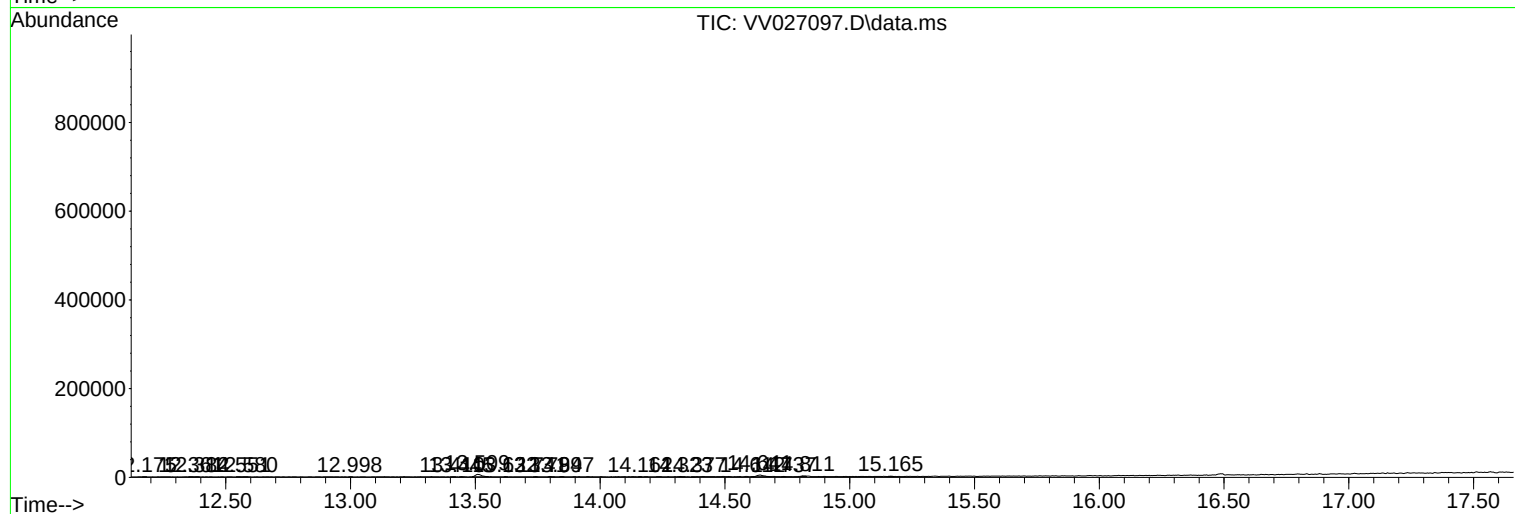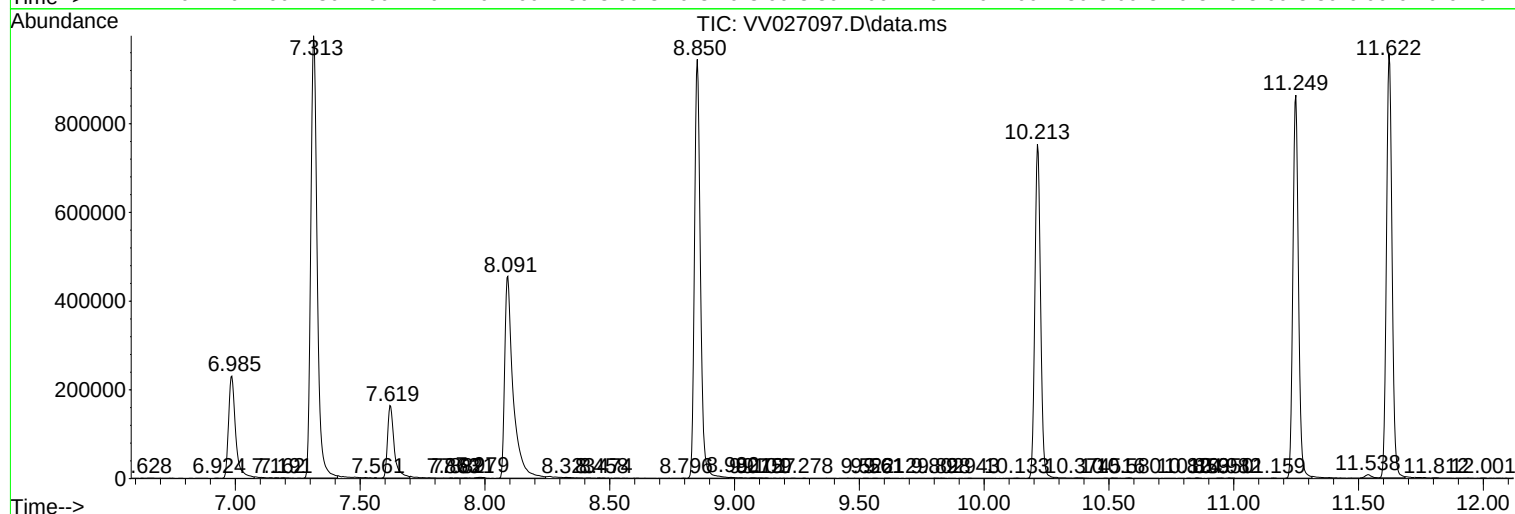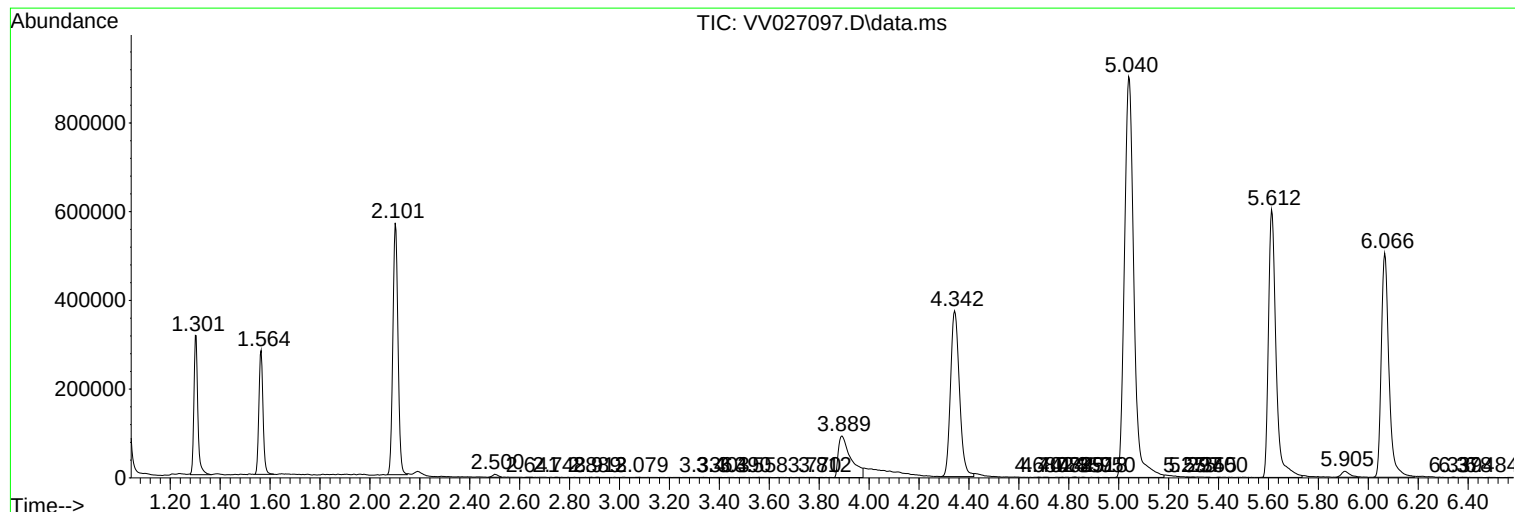

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
Data File : VV027097.D
Acq On : 29 Jul 2022 20:11
Operator : SY/MD
Sample : N3899-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUS2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
Data File : VV027097.D
Acq On : 29 Jul 2022 20:11
Operator : SY/MD
Sample : N3899-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUS2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------