

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
 Data File : VV027102.D
 Acq On : 29 Jul 2022 23:03
 Operator : SY/MD
 Sample : N3955-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0ZD7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
 Title : VOC Analysis

Signal : TIC: VV027102.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	100	rVB	291357	308597	13.92%	1.922%
2	1.565	155	163	175	rBV	257559	293899	13.26%	1.831%
3	2.102	320	330	344	rBV	537794	770967	34.78%	4.802%
4	2.751	528	532	536	rVV8	771	711	0.03%	0.004%
5	2.770	536	538	543	rVB4	650	549	0.02%	0.003%
6	2.954	591	595	600	rBV4	493	494	0.02%	0.003%
7	2.989	603	606	613	rBV2	345	349	0.02%	0.002%
8	3.278	693	696	699	rBV2	639	494	0.02%	0.003%
9	3.327	708	711	717	rBV2	374	378	0.02%	0.002%
10	3.442	742	747	750	rBV3	374	430	0.02%	0.003%
11	3.561	782	784	789	rVB2	530	351	0.02%	0.002%
12	3.671	814	818	822	rBV2	823	748	0.03%	0.005%
13	3.886	875	885	927	rBV	86797	343136	15.48%	2.137%
14	4.343	1012	1027	1051	rBV	353635	869543	39.23%	5.416%
15	4.626	1113	1115	1121	rVV3	351	327	0.01%	0.002%
16	4.680	1129	1132	1135	rVV3	551	440	0.02%	0.003%
17	4.728	1144	1147	1151	rBV3	504	337	0.02%	0.002%
18	4.928	1204	1209	1214	rBV3	678	789	0.04%	0.005%
19	5.044	1227	1245	1285	rBV2	838699	2216683	100.00%	13.807%
20	5.420	1360	1362	1368	rVB3	521	471	0.02%	0.003%
21	5.613	1410	1422	1464	rBV	571778	1207772	54.49%	7.523%
22	5.857	1494	1498	1500	rBV4	852	572	0.03%	0.004%
23	5.908	1500	1514	1526	rBV2	16816	35825	1.62%	0.223%
24	5.989	1537	1539	1542	rVB4	946	549	0.02%	0.003%
25	6.066	1549	1563	1593	rBV	477494	1005271	45.35%	6.261%
26	6.269	1623	1626	1629	rBV4	648	509	0.02%	0.003%
27	6.371	1655	1658	1661	rBV4	874	612	0.03%	0.004%
28	6.423	1672	1674	1680	rVB3	692	516	0.02%	0.003%
29	6.507	1697	1700	1701	rBV	667	364	0.02%	0.002%
30	6.642	1737	1742	1746	rBV4	726	633	0.03%	0.004%
31	6.667	1746	1750	1753	rVV2	580	434	0.02%	0.003%
32	6.908	1823	1825	1828	rBV	414	297	0.01%	0.002%
33	6.982	1837	1848	1885	rBV	215728	424160	19.13%	2.642%
34	7.214	1918	1920	1925	rVB4	812	601	0.03%	0.004%
35	7.240	1925	1928	1931	rBV4	826	525	0.02%	0.003%
36	7.256	1931	1933	1938	rVB3	625	511	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
 Data File : VV027102.D
 Acq On : 29 Jul 2022 23:03
 Operator : SY/MD
 Sample : N3955-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0ZD7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
 Title : VOC Analysis

37	7.314	1938	1951	1990	rBV	956336	1713731	77.31%	10.674%
38	7.619	2034	2046	2068	rBV	151601	281347	12.69%	1.752%
39	7.863	2119	2122	2126	rVB3	666	520	0.02%	0.003%
40	7.896	2127	2132	2137	rVB5	601	527	0.02%	0.003%
41	7.979	2150	2158	2168	rBV9	2782	5111	0.23%	0.032%
42	8.037	2174	2176	2179	rVB4	590	313	0.01%	0.002%
43	8.092	2179	2193	2232	rBV	407886	991362	44.72%	6.175%
44	8.246	2233	2241	2262	rVB3	26970	57472	2.59%	0.358%
45	8.680	2372	2376	2380	rBV3	460	407	0.02%	0.003%
46	8.850	2417	2429	2461	rBV	896914	1496607	67.52%	9.322%
47	9.024	2481	2483	2486	rBV2	757	360	0.02%	0.002%
48	9.166	2526	2527	2536	rVB4	567	629	0.03%	0.004%
49	9.207	2537	2540	2543	rVB4	554	390	0.02%	0.002%
50	9.227	2543	2546	2552	rBV2	386	315	0.01%	0.002%
51	9.294	2563	2567	2569	rBV2	698	547	0.02%	0.003%
52	9.342	2579	2582	2589	rBV3	737	660	0.03%	0.004%
53	9.535	2637	2642	2643	rBV4	725	613	0.03%	0.004%
54	9.590	2656	2659	2664	rBV5	523	424	0.02%	0.003%
55	9.693	2686	2691	2693	rBV2	440	341	0.02%	0.002%
56	9.722	2693	2700	2703	rBV4	1758	2035	0.09%	0.013%
57	9.815	2725	2729	2730	rBV2	2127	1305	0.06%	0.008%
58	10.021	2788	2793	2795	rBV4	1697	1602	0.07%	0.010%
59	10.214	2840	2853	2877	rBV	697563	1112523	50.19%	6.930%
60	10.365	2897	2900	2904	rBV3	435	364	0.02%	0.002%
61	10.384	2904	2906	2912	rVB2	579	324	0.01%	0.002%
62	10.500	2938	2942	2944	rBV2	628	417	0.02%	0.003%
63	10.584	2963	2968	2972	rVB4	528	523	0.02%	0.003%
64	10.802	3035	3036	3040	rBV2	413	301	0.01%	0.002%
65	10.834	3040	3046	3049	rBV4	1800	2291	0.10%	0.014%
66	10.937	3063	3078	3088	rBV4	4348	11302	0.51%	0.070%
67	11.050	3105	3113	3119	rVB4	956	1187	0.05%	0.007%
68	11.082	3121	3123	3131	rVB4	710	810	0.04%	0.005%
69	11.117	3131	3134	3135	rBV3	608	361	0.02%	0.002%
70	11.156	3138	3146	3152	rBV5	4281	5915	0.27%	0.037%
71	11.188	3152	3156	3163	rVB5	1793	2009	0.09%	0.013%
72	11.246	3163	3174	3205	rBV	860392	1341125	60.50%	8.353%
73	11.394	3217	3220	3223	rVB4	533	326	0.01%	0.002%
74	11.500	3249	3253	3254	rBV2	415	297	0.01%	0.002%
75	11.535	3255	3264	3277	rVV3	13854	24779	1.12%	0.154%
76	11.622	3280	3291	3313	rVV	930120	1460451	65.88%	9.097%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
 Data File : VV027102.D
 Acq On : 29 Jul 2022 23:03
 Operator : SY/MD
 Sample : N3955-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0ZD7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
 Title : VOC Analysis

77	11.837	3356	3358	3365	rVB3	600	509	0.02%	0.003%
78	11.992	3403	3406	3409	rBV4	570	400	0.02%	0.002%
79	12.021	3409	3415	3429	rVB7	2942	5513	0.25%	0.034%
80	12.281	3493	3496	3498	rBV3	391	283	0.01%	0.002%
81	12.349	3510	3517	3527	rVB5	8033	11205	0.51%	0.070%
82	12.500	3560	3564	3565	rVB2	811	303	0.01%	0.002%
83	12.526	3569	3572	3576	rVV	426	283	0.01%	0.002%
84	12.651	3604	3611	3620	rVB5	1996	2663	0.12%	0.017%
85	12.731	3631	3636	3642	rVB3	688	742	0.03%	0.005%
86	12.818	3660	3663	3666	rVB	520	284	0.01%	0.002%
87	12.834	3666	3668	3671	rBV2	592	301	0.01%	0.002%
88	13.024	3724	3727	3732	rBV3	505	536	0.02%	0.003%
89	13.146	3762	3765	3777	rVB5	746	1285	0.06%	0.008%
90	13.268	3796	3803	3809	rVV6	2242	3118	0.14%	0.019%
91	13.365	3827	3833	3837	rBV3	407	493	0.02%	0.003%
92	13.407	3842	3846	3848	rBV3	591	569	0.03%	0.004%
93	13.513	3871	3879	3887	rBV3	5127	8543	0.39%	0.053%
94	13.702	3936	3938	3942	rVB4	583	408	0.02%	0.003%
95	13.747	3945	3952	3962	rVV6	2691	3944	0.18%	0.025%
96	14.239	4103	4105	4108	rBV2	513	325	0.01%	0.002%
97	14.413	4155	4159	4162	rBV2	690	612	0.03%	0.004%
98	14.622	4221	4224	4227	rVB2	624	455	0.02%	0.003%
99	14.773	4268	4271	4273	rBV3	632	488	0.02%	0.003%
100	15.722	4563	4566	4570	rBV3	1114	795	0.04%	0.005%




Sum of corrected areas: 16054824

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
Data File : VV072102.D
Acq On : 29 Jul 2022 23:03
Operator : SY/MD
Sample : N3955-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COZD7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

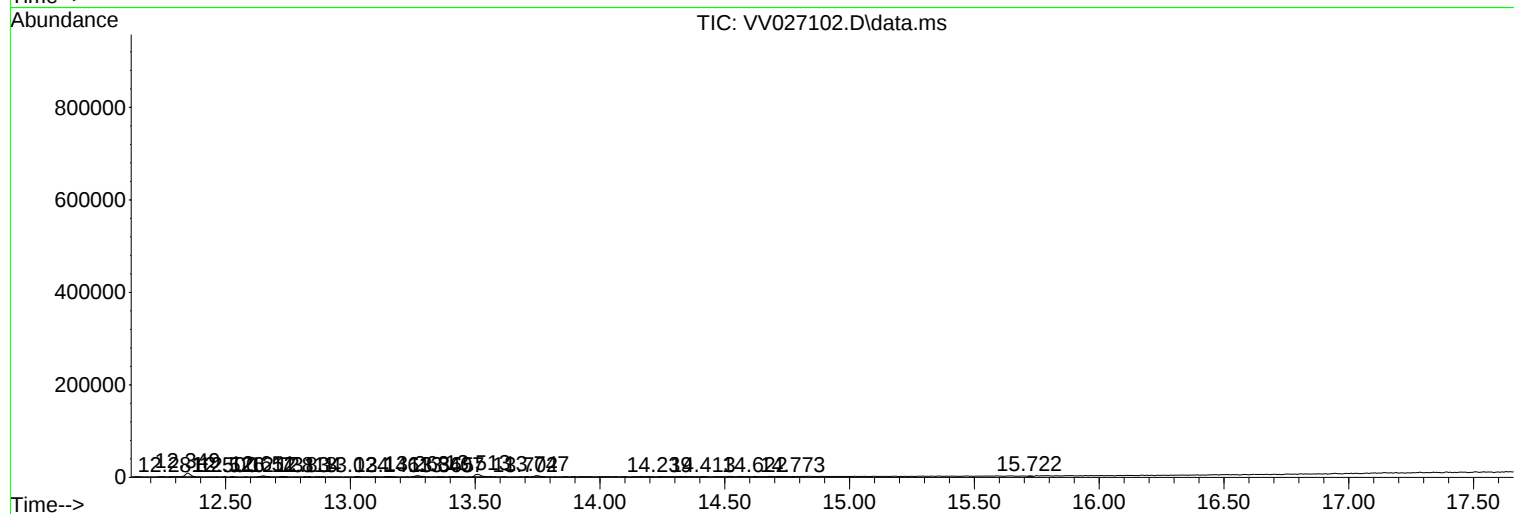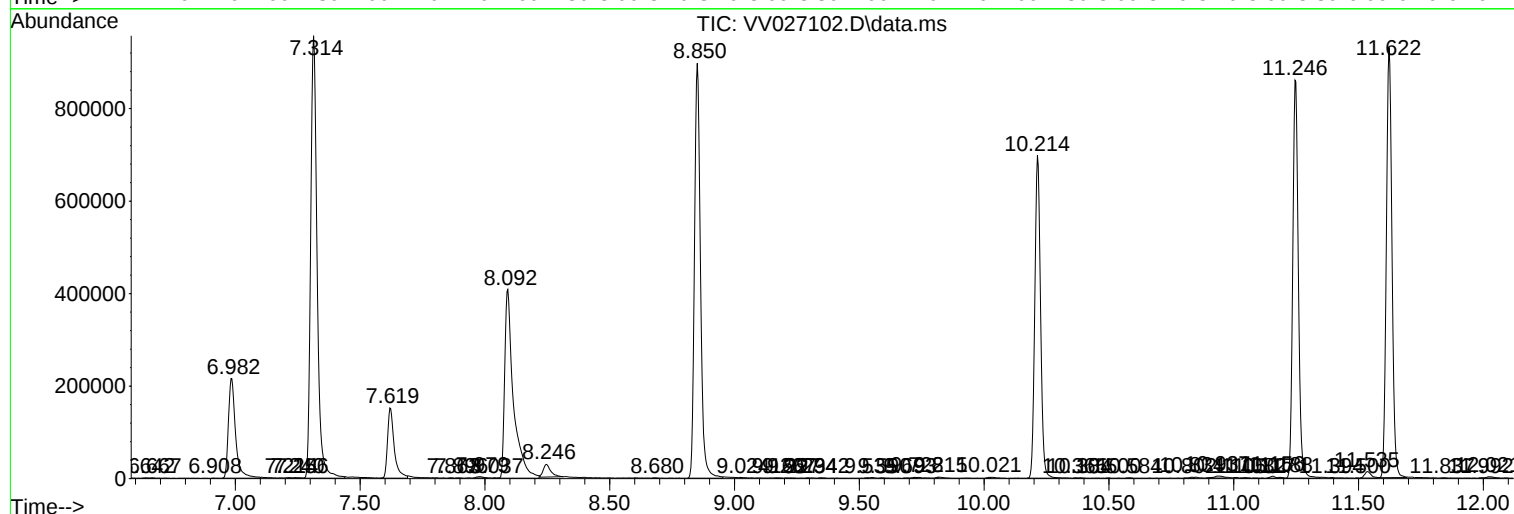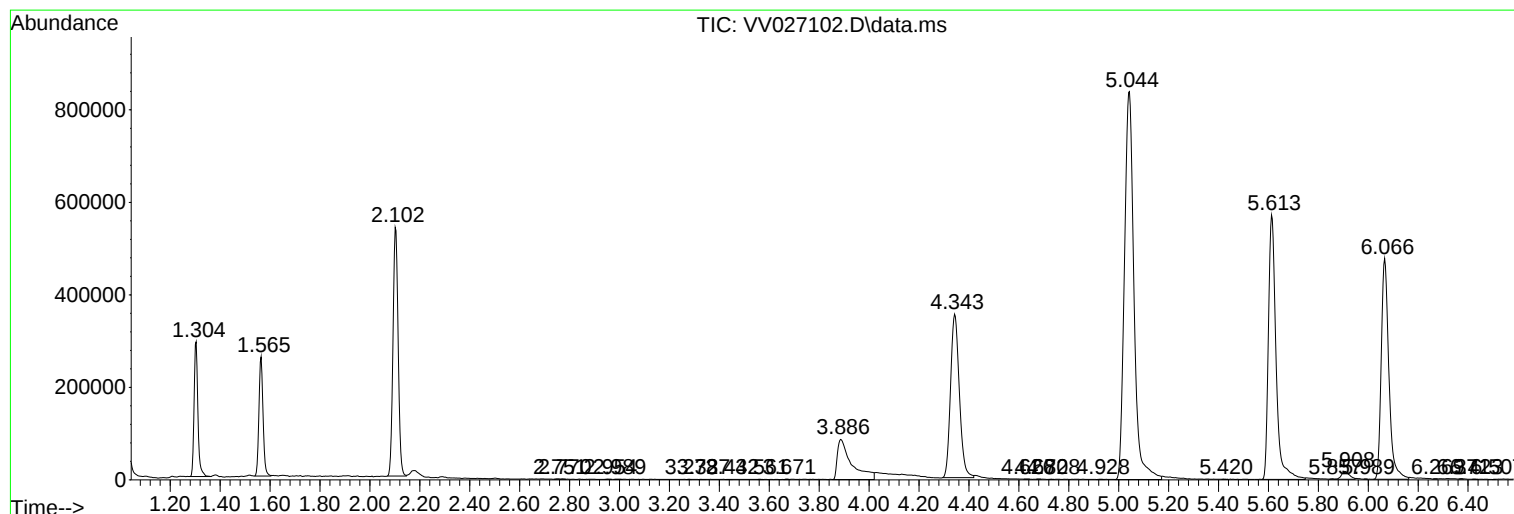

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
Data File : VV027102.D
Acq On : 29 Jul 2022 23:03
Operator : SY/MD
Sample : N3955-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0ZD7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
Data File : VV027102.D
Acq On : 29 Jul 2022 23:03
Operator : SY/MD
Sample : N3955-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0ZD7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------