

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
 Data File : VV027116.D
 Acq On : 30 Jul 2022 04:45
 Operator : SY/MD
 Sample : N3899-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUS1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
 Title : VOC Analysis

Signal : TIC: VV027116.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.105	16	20	35	rVB	67779	67625	2.73%	0.370%
2	1.304	75	82	98	rVB	327030	335553	13.57%	1.836%
3	1.564	156	163	176	rVB	273401	309117	12.50%	1.692%
4	2.105	322	331	343	rVB	565341	800674	32.38%	4.381%
5	3.101	634	641	647	rBV3	542	938	0.04%	0.005%
6	3.169	658	662	664	rBV2	965	796	0.03%	0.004%
7	3.230	677	681	683	rVB	511	320	0.01%	0.002%
8	3.333	710	713	715	rBV2	223	141	0.01%	0.001%
9	3.394	728	732	734	rVB	521	350	0.01%	0.002%
10	3.410	734	737	739	rBV	361	220	0.01%	0.001%
11	3.426	739	742	747	rBV2	200	193	0.01%	0.001%
12	3.452	747	750	754	rBV2	406	384	0.02%	0.002%
13	3.510	763	768	771	rBV	414	441	0.02%	0.002%
14	3.561	781	784	787	rBV2	220	186	0.01%	0.001%
15	3.635	803	807	811	rVB	403	315	0.01%	0.002%
16	3.731	833	837	839	rBV2	302	207	0.01%	0.001%
17	3.776	845	851	853	rBV	437	314	0.01%	0.002%
18	3.828	865	867	870	rBV3	218	152	0.01%	0.001%
19	3.886	875	885	910	rBV	93891	315936	12.78%	1.729%
20	4.342	1013	1027	1067	rBV2	498258	1363294	55.13%	7.460%
21	4.931	1206	1210	1214	rBV2	505	462	0.02%	0.003%
22	5.040	1227	1244	1285	rBV2	938083	2472910	100.00%	13.532%
23	5.481	1378	1381	1384	rBV2	458	348	0.01%	0.002%
24	5.503	1384	1388	1392	rBV4	536	527	0.02%	0.003%
25	5.612	1410	1422	1466	rBV	676307	1426454	57.68%	7.806%
26	5.911	1504	1515	1533	rVV5	7620	17533	0.71%	0.096%
27	5.985	1537	1538	1540	rBV2	421	160	0.01%	0.001%
28	6.066	1549	1563	1603	rBV	521007	1102801	44.60%	6.035%
29	6.326	1642	1644	1646	rBV	499	220	0.01%	0.001%
30	6.362	1653	1655	1658	rBV3	397	295	0.01%	0.002%
31	6.394	1662	1665	1666	rBV2	349	167	0.01%	0.001%
32	6.542	1706	1711	1713	rBV3	339	234	0.01%	0.001%
33	6.628	1732	1738	1741	rBV4	683	760	0.03%	0.004%
34	6.654	1741	1746	1747	rBV3	656	437	0.02%	0.002%
35	6.792	1785	1789	1791	rBV2	419	290	0.01%	0.002%
36	6.870	1810	1813	1814	rBV2	343	125	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
 Data File : VV027116.D
 Acq On : 30 Jul 2022 04:45
 Operator : SY/MD
 Sample : N3899-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUS1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
 Title : VOC Analysis

37	6.902	1820	1823	1826	rBV	355	284	0.01%	0.002%
38	6.931	1830	1832	1833	rBV	348	142	0.01%	0.001%
39	6.940	1833	1835	1838	rVB2	293	166	0.01%	0.001%
40	6.985	1838	1849	1870	rBV	240590	456881	18.48%	2.500%
41	7.313	1939	1951	1988	rBV	1078293	1920509	77.66%	10.509%
42	7.583	2032	2035	2036	rBV2	590	260	0.01%	0.001%
43	7.619	2037	2046	2076	rVV	164805	304829	12.33%	1.668%
44	8.021	2165	2171	2181	rBV3	4435	7588	0.31%	0.042%
45	8.091	2183	2193	2237	rVV	453260	1060537	42.89%	5.803%
46	8.458	2303	2307	2310	rBV3	685	588	0.02%	0.003%
47	8.686	2376	2378	2381	rVB	310	154	0.01%	0.001%
48	8.709	2381	2385	2389	rBV4	428	344	0.01%	0.002%
49	8.728	2389	2391	2393	rBV	555	258	0.01%	0.001%
50	8.747	2393	2397	2400	rBV3	394	293	0.01%	0.002%
51	8.850	2416	2429	2459	rBV	1043918	1774246	71.75%	9.709%
52	9.259	2554	2556	2558	rBV2	384	169	0.01%	0.001%
53	9.281	2558	2563	2565	rBV2	429	281	0.01%	0.002%
54	9.329	2576	2578	2579	rBV2	310	133	0.01%	0.001%
55	9.365	2586	2589	2594	rBV2	498	502	0.02%	0.003%
56	9.387	2594	2596	2599	rVV2	382	167	0.01%	0.001%
57	9.432	2607	2610	2614	rVB	385	233	0.01%	0.001%
58	9.452	2614	2616	2620	rVV	383	306	0.01%	0.002%
59	9.480	2623	2625	2628	rVB	400	165	0.01%	0.001%
60	9.500	2628	2631	2634	rVB2	255	176	0.01%	0.001%
61	9.525	2634	2639	2642	rBV3	374	342	0.01%	0.002%
62	9.554	2646	2648	2651	rVB2	484	272	0.01%	0.001%
63	9.577	2651	2655	2658	rVB2	301	144	0.01%	0.001%
64	9.599	2658	2662	2665	rBV	465	295	0.01%	0.002%
65	9.699	2687	2693	2695	rBV2	414	414	0.02%	0.002%
66	9.728	2699	2702	2703	rBV2	308	176	0.01%	0.001%
67	9.873	2743	2747	2750	rBV3	350	318	0.01%	0.002%
68	9.889	2750	2752	2755	rVV	339	249	0.01%	0.001%
69	9.905	2755	2757	2760	rVB2	491	291	0.01%	0.002%
70	10.033	2786	2797	2804	rBV7	2627	5291	0.21%	0.029%
71	10.214	2840	2853	2876	rBV	782785	1239138	50.11%	6.781%
72	10.435	2917	2922	2923	rBV2	597	487	0.02%	0.003%
73	10.577	2960	2966	2967	rBV4	801	674	0.03%	0.004%
74	10.660	2988	2992	2995	rBV2	318	316	0.01%	0.002%
75	10.689	2999	3001	3005	rBV3	270	172	0.01%	0.001%
76	10.847	3048	3050	3057	rVB2	286	282	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
 Data File : VV027116.D
 Acq On : 30 Jul 2022 04:45
 Operator : SY/MD
 Sample : N3899-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUS1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
 Title : VOC Analysis

77	10.876	3057	3059	3061	rBV	248	138	0.01%	0.001%
78	10.924	3071	3074	3075	rBV2	382	188	0.01%	0.001%
79	10.995	3094	3096	3099	rVB2	391	199	0.01%	0.001%
80	11.062	3112	3117	3126	rBV3	595	704	0.03%	0.004%
81	11.172	3148	3151	3153	rBV	649	421	0.02%	0.002%
82	11.249	3163	3175	3201	rBV	989797	1557600	62.99%	8.523%
83	11.535	3256	3264	3276	rBV4	10607	19173	0.78%	0.105%
84	11.622	3279	3291	3319	rVV	1046440	1628440	65.85%	8.911%
85	11.850	3361	3362	3366	rBV2	281	148	0.01%	0.001%
86	11.979	3399	3402	3405	rBV2	489	308	0.01%	0.002%
87	12.249	3482	3486	3495	rVB6	964	1505	0.06%	0.008%
88	12.403	3527	3534	3543	rVB5	2844	4454	0.18%	0.024%
89	12.651	3609	3611	3614	rBV3	231	166	0.01%	0.001%
90	12.670	3615	3617	3621	rBV2	407	277	0.01%	0.002%
91	12.824	3657	3665	3674	rBV7	3545	5744	0.23%	0.031%
92	12.969	3707	3710	3717	rVB3	589	458	0.02%	0.003%
93	13.011	3720	3723	3725	rBV2	564	286	0.01%	0.002%
94	13.213	3784	3786	3788	rBV2	324	189	0.01%	0.001%
95	13.397	3840	3843	3849	rBV3	479	545	0.02%	0.003%
96	13.599	3902	3906	3910	rBV3	571	647	0.03%	0.004%
97	13.731	3945	3947	3950	rBV2	502	247	0.01%	0.001%
98	13.908	3994	4002	4012	rVB7	7912	12217	0.49%	0.067%
99	14.426	4161	4163	4167	rBV2	652	483	0.02%	0.003%
100	14.966	4322	4331	4341	rBV2	26482	40729	1.65%	0.223%




Sum of corrected areas: 18274217

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
Data File : VV027116.D
Acq On : 30 Jul 2022 04:45
Operator : SY/MD
Sample : N3899-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUS1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

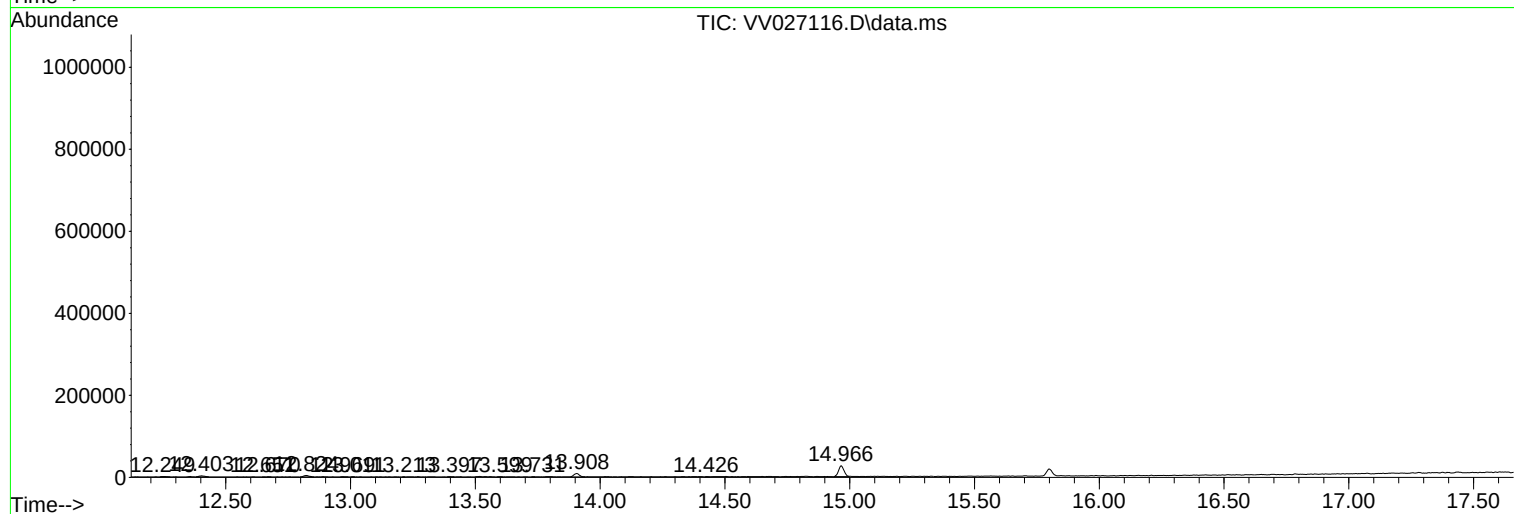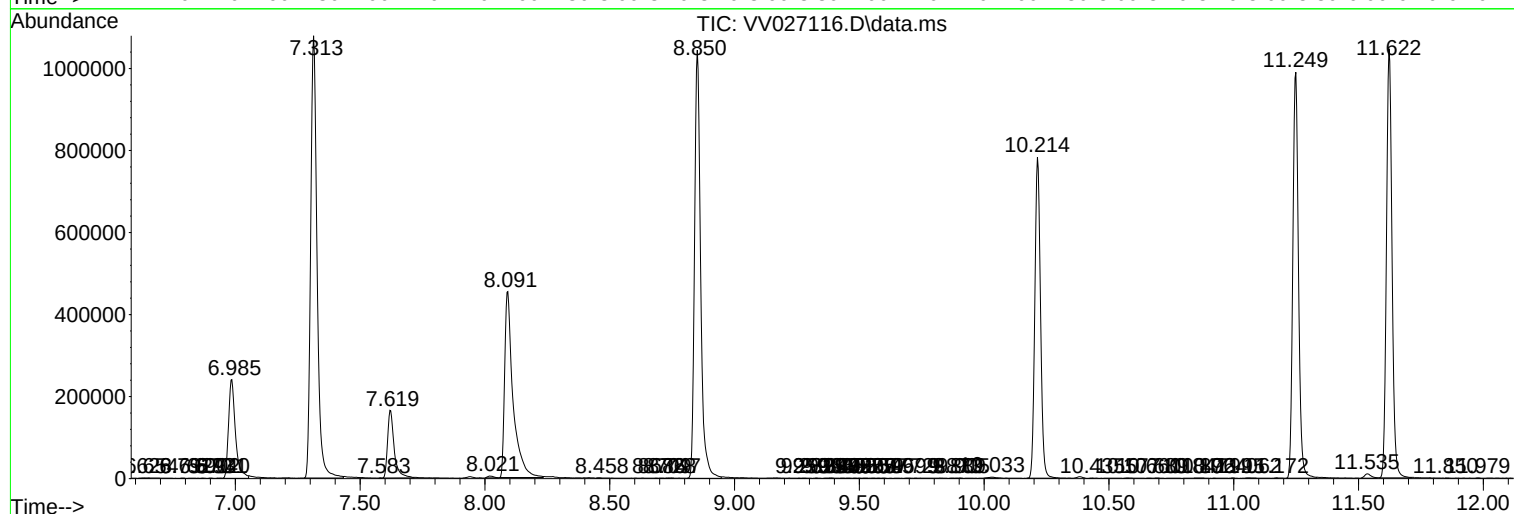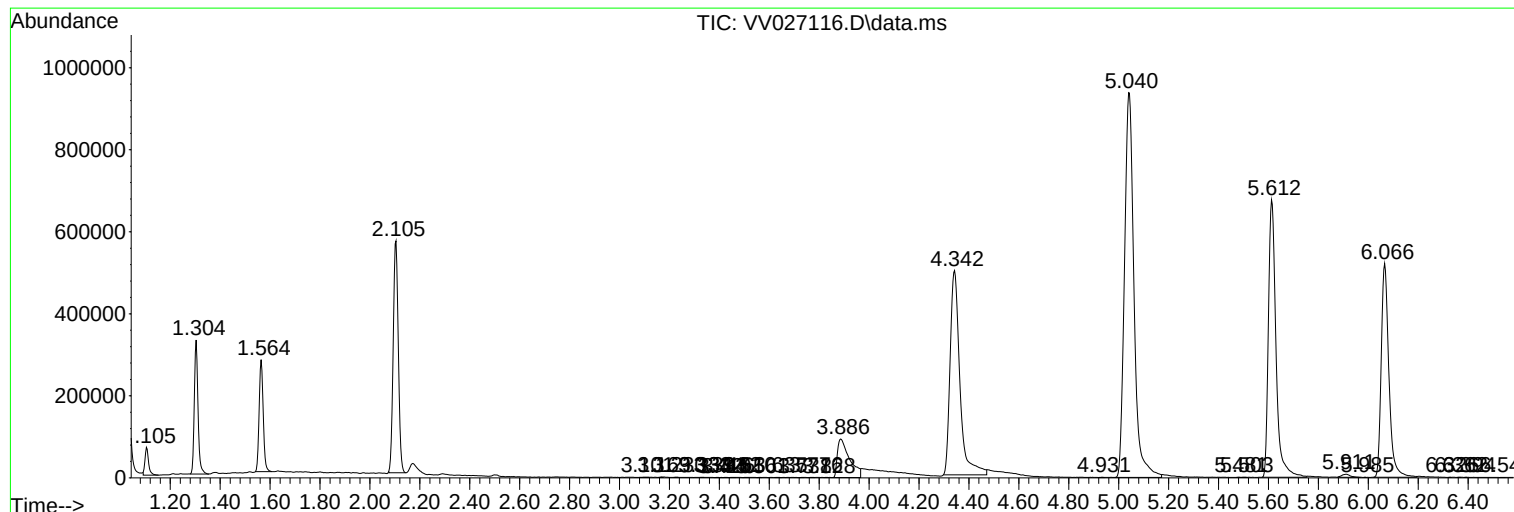

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
Data File : VV027116.D
Acq On : 30 Jul 2022 04:45
Operator : SY/MD
Sample : N3899-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUS1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
Data File : VV027116.D
Acq On : 30 Jul 2022 04:45
Operator : SY/MD
Sample : N3899-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUS1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc