

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
 Data File : VV027118.D
 Acq On : 30 Jul 2022 05:34
 Operator : SY/MD
 Sample : N3899-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUR6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
 Title : VOC Analysis

Signal : TIC: VV027118.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.105	16	20	33	rVB	46747	47023	1.93%	0.270%
2	1.304	75	82	98	rVB	330220	343037	14.04%	1.968%
3	1.564	156	163	178	rVB	282406	322719	13.21%	1.851%
4	2.105	322	331	345	rVB	586210	833106	34.11%	4.779%
5	3.018	612	615	618	rVB2	537	366	0.01%	0.002%
6	3.037	618	621	622	rBV	262	157	0.01%	0.001%
7	3.224	677	679	681	rBV2	223	97	0.00%	0.001%
8	3.285	696	698	701	rBV3	324	229	0.01%	0.001%
9	3.336	711	714	717	rBV	238	175	0.01%	0.001%
10	3.388	728	730	733	rVB2	425	237	0.01%	0.001%
11	3.410	733	737	742	rBV2	561	500	0.02%	0.003%
12	3.442	742	747	749	rBV2	242	241	0.01%	0.001%
13	3.558	779	783	784	rBV2	248	164	0.01%	0.001%
14	3.587	790	792	796	rBV2	244	221	0.01%	0.001%
15	3.651	806	812	815	rVB2	356	375	0.02%	0.002%
16	3.690	822	824	826	rBV2	101	54	0.00%	0.000%
17	3.706	826	829	833	rBV2	341	318	0.01%	0.002%
18	3.886	875	885	915	rBV	94089	336246	13.77%	1.929%
19	4.342	1013	1027	1069	rVB	378690	949202	38.86%	5.445%
20	4.667	1126	1128	1129	rVB	686	193	0.01%	0.001%
21	4.728	1144	1147	1150	rBV3	372	245	0.01%	0.001%
22	4.953	1215	1217	1219	rBV2	374	151	0.01%	0.001%
23	5.040	1225	1244	1292	rBV2	928819	2442448	100.00%	14.010%
24	5.613	1409	1422	1469	rBV	642766	1352018	55.36%	7.755%
25	6.066	1549	1563	1592	rBV	522603	1088782	44.58%	6.245%
26	6.326	1642	1644	1646	rBV	474	250	0.01%	0.001%
27	6.378	1656	1660	1662	rBV2	529	364	0.01%	0.002%
28	6.413	1669	1671	1674	rVB2	393	145	0.01%	0.001%
29	6.436	1674	1678	1681	rBV2	438	388	0.02%	0.002%
30	6.513	1699	1702	1703	rBV2	387	240	0.01%	0.001%
31	6.542	1709	1711	1716	rBV3	207	205	0.01%	0.001%
32	6.593	1724	1727	1728	rBV	418	205	0.01%	0.001%
33	6.651	1739	1745	1746	rBV3	658	568	0.02%	0.003%
34	6.786	1782	1787	1788	rBV	424	300	0.01%	0.002%
35	6.841	1802	1804	1807	rVB2	303	141	0.01%	0.001%
36	6.857	1807	1809	1812	rVB	196	87	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW072922\
 Data File : VW027118.D
 Acq On : 30 Jul 2022 05:34
 Operator : SY/MD
 Sample : N3899-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUR6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
 Title : VOC Analysis

37	6.876	1812	1815	1820	rVB3	350	315	0.01%	0.002%
38	6.905	1820	1824	1827	rBV2	368	283	0.01%	0.002%
39	6.944	1834	1836	1837	rBV	149	61	0.00%	0.000%
40	6.982	1837	1848	1881	rBV	234208	448634	18.37%	2.573%
41	7.313	1938	1951	2003	rBV	1078732	1915116	78.41%	10.985%
42	7.619	2036	2046	2088	rBV	160069	302416	12.38%	1.735%
43	7.831	2108	2112	2117	rBV6	749	764	0.03%	0.004%
44	7.976	2150	2157	2166	rBV4	6009	9445	0.39%	0.054%
45	8.088	2182	2192	2235	rBV	440701	1055904	43.23%	6.057%
46	8.484	2313	2315	2318	rBV2	543	267	0.01%	0.002%
47	8.561	2337	2339	2342	rVB2	490	270	0.01%	0.002%
48	8.574	2342	2343	2344	rBV	405	108	0.00%	0.001%
49	8.702	2377	2383	2385	rBV3	531	405	0.02%	0.002%
50	8.744	2392	2396	2398	rBV	335	201	0.01%	0.001%
51	8.764	2398	2402	2406	rVB3	599	586	0.02%	0.003%
52	8.792	2406	2411	2413	rBV2	360	341	0.01%	0.002%
53	8.805	2413	2415	2417	rBV3	658	337	0.01%	0.002%
54	8.850	2417	2429	2456	rBV	1004951	1684219	68.96%	9.660%
55	9.156	2521	2524	2528	rVB4	771	611	0.03%	0.004%
56	9.182	2528	2532	2534	rBV	568	426	0.02%	0.002%
57	9.210	2539	2541	2544	rBV2	415	275	0.01%	0.002%
58	9.233	2544	2548	2551	rBV2	373	285	0.01%	0.002%
59	9.268	2556	2559	2560	rBV	336	183	0.01%	0.001%
60	9.307	2567	2571	2574	rBV	403	310	0.01%	0.002%
61	9.387	2593	2596	2599	rBV2	539	332	0.01%	0.002%
62	9.474	2621	2623	2626	rBV2	274	124	0.01%	0.001%
63	9.529	2635	2640	2641	rBV	303	227	0.01%	0.001%
64	9.558	2647	2649	2654	rVB4	328	237	0.01%	0.001%
65	9.583	2656	2657	2660	rVB2	195	79	0.00%	0.000%
66	9.641	2671	2675	2678	rBV	344	291	0.01%	0.002%
67	9.786	2716	2720	2722	rBV2	286	156	0.01%	0.001%
68	9.844	2733	2738	2741	rBV4	539	373	0.02%	0.002%
69	9.860	2741	2743	2746	rBV2	288	190	0.01%	0.001%
70	9.911	2755	2759	2768	rVB2	495	651	0.03%	0.004%
71	9.995	2781	2785	2792	rVB3	371	389	0.02%	0.002%
72	10.037	2792	2798	2803	rVB2	297	369	0.02%	0.002%
73	10.072	2803	2809	2812	rBV2	374	372	0.02%	0.002%
74	10.136	2826	2829	2832	rBV2	317	188	0.01%	0.001%
75	10.214	2841	2853	2878	rBV	770241	1217900	49.86%	6.986%
76	10.410	2913	2914	2919	rVB2	445	217	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
 Data File : VV027118.D
 Acq On : 30 Jul 2022 05:34
 Operator : SY/MD
 Sample : N3899-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUR6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
 Title : VOC Analysis

77	10.432	2919	2921	2922	rBV	318	132	0.01%	0.001%
78	10.561	2959	2961	2962	rBV	160	62	0.00%	0.000%
79	10.574	2962	2965	2967	rBV2	525	317	0.01%	0.002%
80	10.773	3023	3027	3028	rBV	274	200	0.01%	0.001%
81	10.808	3036	3038	3039	rBV	242	110	0.00%	0.001%
82	10.844	3047	3049	3052	rBV2	294	121	0.00%	0.001%
83	10.979	3088	3091	3094	rBV3	230	181	0.01%	0.001%
84	11.069	3111	3119	3123	rBV3	395	550	0.02%	0.003%
85	11.194	3155	3158	3160	rBV2	469	284	0.01%	0.002%
86	11.246	3163	3174	3197	rBV	925064	1457844	59.69%	8.362%
87	11.538	3257	3265	3272	rBV6	5118	8200	0.34%	0.047%
88	11.622	3280	3291	3318	rBV	1006990	1577827	64.60%	9.050%
89	11.950	3391	3393	3395	rBV2	339	207	0.01%	0.001%
90	12.027	3415	3417	3421	rBV2	420	293	0.01%	0.002%
91	12.468	3552	3554	3558	rBV	415	333	0.01%	0.002%
92	12.821	3660	3664	3673	rVB3	2033	2693	0.11%	0.015%
93	14.767	4266	4269	4272	rBV3	645	524	0.02%	0.003%
94	14.966	4324	4331	4340	rBV6	13820	19171	0.78%	0.110%



Sum of corrected areas: 17434103

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
Data File : VV027118.D
Acq On : 30 Jul 2022 05:34
Operator : SY/MD
Sample : N3899-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUR6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

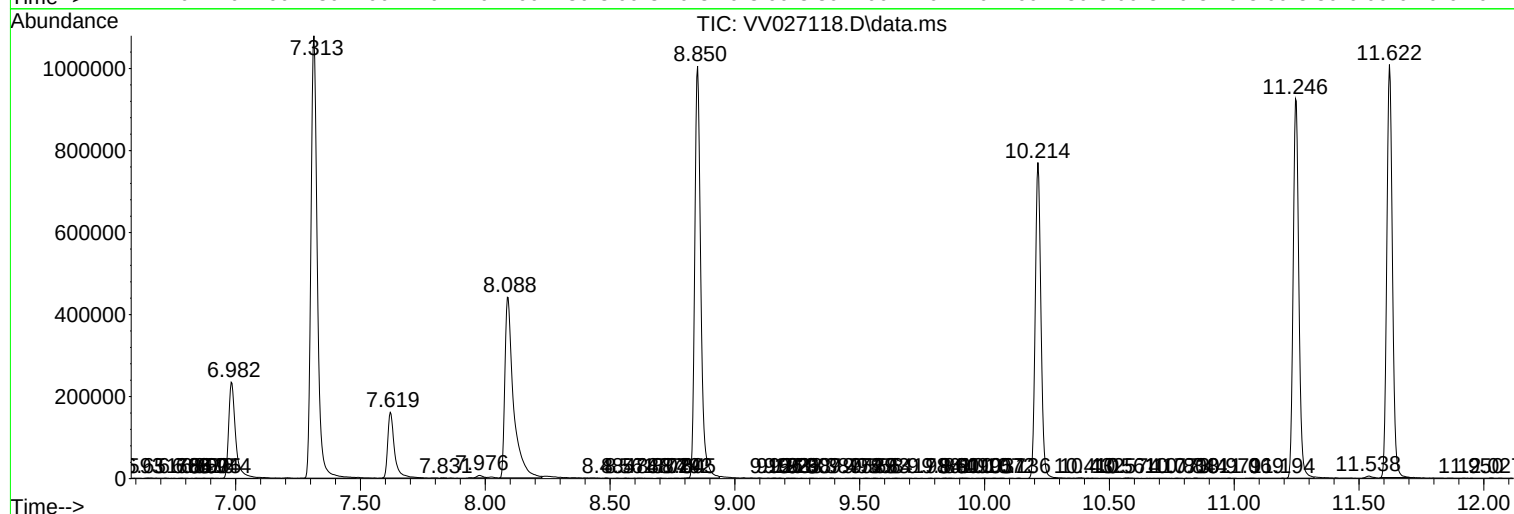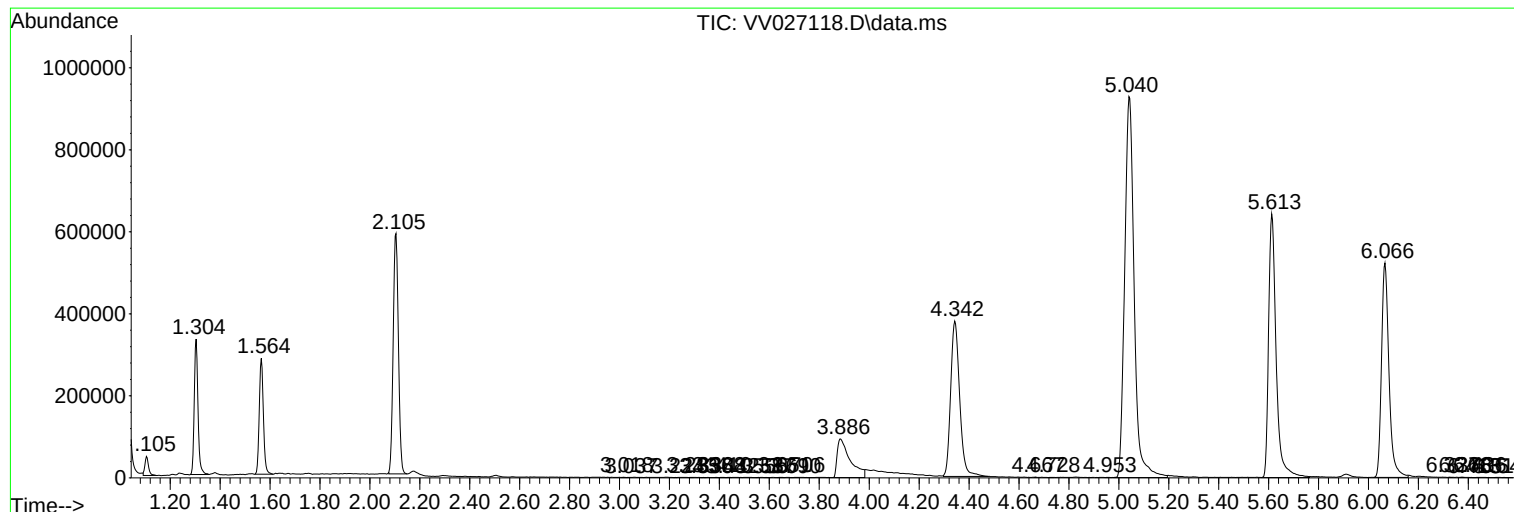

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
Data File : VV027118.D
Acq On : 30 Jul 2022 05:34
Operator : SY/MD
Sample : N3899-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUR6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
Data File : VV027118.D
Acq On : 30 Jul 2022 05:34
Operator : SY/MD
Sample : N3899-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUR6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc