

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
 Data File : VV027119.D
 Acq On : 30 Jul 2022 05:59
 Operator : SY/MD
 Sample : N3899-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUS3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
 Title : VOC Analysis

Signal : TIC: VV027119.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.105	16	20	30	rVB	36645	35252	1.43%	0.199%
2	1.304	75	82	99	rVB	320722	338118	13.72%	1.907%
3	1.565	156	163	177	rVB	282829	316701	12.85%	1.786%
4	2.102	321	330	346	rVB	581067	827535	33.57%	4.668%
5	3.047	622	624	625	rBV	360	128	0.01%	0.001%
6	3.137	649	652	654	rBV2	438	181	0.01%	0.001%
7	3.301	700	703	706	rBV3	335	228	0.01%	0.001%
8	3.474	756	757	758	rBV	155	30	0.00%	0.000%
9	3.497	763	764	768	rBV2	311	168	0.01%	0.001%
10	3.571	784	787	789	rBV3	201	116	0.00%	0.001%
11	3.677	809	820	822	rBV7	2137	3197	0.13%	0.018%
12	3.812	860	862	863	rBV	407	164	0.01%	0.001%
13	3.892	872	887	919	rBV	92088	372961	15.13%	2.104%
14	4.343	1013	1027	1075	rVB	384737	972363	39.45%	5.485%
15	4.683	1131	1133	1137	rBV2	501	359	0.01%	0.002%
16	4.883	1192	1195	1196	rBV	253	151	0.01%	0.001%
17	5.040	1227	1244	1287	rBV2	939739	2464938	100.00%	13.904%
18	5.429	1364	1365	1366	rBV	162	50	0.00%	0.000%
19	5.545	1398	1401	1403	rBV	621	464	0.02%	0.003%
20	5.613	1410	1422	1457	rBV	657974	1363956	55.33%	7.694%
21	5.905	1506	1513	1536	rVB3	12507	28287	1.15%	0.160%
22	6.066	1546	1563	1593	rBV	522957	1105786	44.86%	6.237%
23	6.487	1692	1694	1695	rBV	225	91	0.00%	0.001%
24	6.542	1698	1711	1713	rBV8	1386	2655	0.11%	0.015%
25	6.687	1754	1756	1757	rBV	486	154	0.01%	0.001%
26	6.738	1768	1772	1776	rVB3	538	554	0.02%	0.003%
27	6.764	1776	1780	1781	rBV	304	157	0.01%	0.001%
28	6.870	1812	1813	1814	rBV	147	45	0.00%	0.000%
29	6.899	1818	1822	1823	rBV	271	185	0.01%	0.001%
30	6.908	1823	1825	1829	rBV	176	135	0.01%	0.001%
31	6.982	1837	1848	1874	rBV	233073	450236	18.27%	2.540%
32	7.314	1939	1951	1980	rBV	1069441	1922220	77.98%	10.843%
33	7.619	2036	2046	2084	rBV	161971	305400	12.39%	1.723%
34	7.873	2123	2125	2128	rBV3	420	240	0.01%	0.001%
35	7.941	2139	2146	2153	rVB6	2586	3793	0.15%	0.021%
36	8.002	2163	2165	2166	rBV	580	257	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
 Data File : VV027119.D
 Acq On : 30 Jul 2022 05:59
 Operator : SY/MD
 Sample : N3899-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBUS3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
 Title : VOC Analysis

37	8.088	2182	2192	2235	rBV	454978	1065096	43.21%	6.008%
38	8.648	2364	2366	2372	rVB2	563	429	0.02%	0.002%
39	8.850	2417	2429	2454	rBV	1008539	1709902	69.37%	9.645%
40	9.211	2539	2541	2543	rBV2	293	128	0.01%	0.001%
41	9.291	2564	2566	2569	rVB3	265	135	0.01%	0.001%
42	9.410	2601	2603	2605	rBV	342	194	0.01%	0.001%
43	9.445	2613	2614	2617	rBV	274	144	0.01%	0.001%
44	9.484	2623	2626	2629	rBV3	360	274	0.01%	0.002%
45	9.535	2640	2642	2645	rVB2	398	196	0.01%	0.001%
46	9.606	2661	2664	2665	rBV	328	172	0.01%	0.001%
47	9.699	2692	2693	2694	rVB	434	84	0.00%	0.000%
48	9.725	2696	2701	2702	rBV2	780	628	0.03%	0.004%
49	9.818	2726	2730	2731	rBV3	876	573	0.02%	0.003%
50	9.960	2771	2774	2777	rBV	8237	4453	0.18%	0.025%
51	9.982	2778	2781	2784	rVB2	336	254	0.01%	0.001%
52	10.014	2788	2791	2794	rBV2	446	308	0.01%	0.002%
53	10.092	2813	2815	2817	rBV3	550	220	0.01%	0.001%
54	10.137	2827	2829	2832	rBV	259	181	0.01%	0.001%
55	10.214	2841	2853	2875	rBV	755833	1220661	49.52%	6.885%
56	10.558	2954	2960	2963	rBV2	272	318	0.01%	0.002%
57	10.583	2963	2968	2973	rVB4	618	701	0.03%	0.004%
58	10.625	2978	2981	2984	rBV	309	195	0.01%	0.001%
59	10.645	2984	2987	2989	rBV	251	149	0.01%	0.001%
60	10.709	3005	3007	3008	rBV	237	61	0.00%	0.000%
61	10.741	3015	3017	3023	rVB	430	282	0.01%	0.002%
62	10.770	3023	3026	3032	rBV3	520	574	0.02%	0.003%
63	10.854	3049	3052	3053	rBV2	387	225	0.01%	0.001%
64	11.024	3101	3105	3108	rBV3	388	333	0.01%	0.002%
65	11.120	3133	3135	3138	rBV	210	132	0.01%	0.001%
66	11.156	3140	3146	3150	rVV4	1905	1963	0.08%	0.011%
67	11.246	3162	3174	3200	rBV	973115	1521639	61.73%	8.583%
68	11.535	3257	3264	3276	rBV5	7663	12700	0.52%	0.072%
69	11.622	3279	3291	3312	rBV	1032473	1630114	66.13%	9.195%
70	11.857	3361	3364	3368	rVB3	811	665	0.03%	0.004%
71	12.127	3446	3448	3451	rBV2	616	391	0.02%	0.002%
72	12.349	3510	3517	3529	rVB4	5932	9589	0.39%	0.054%
73	12.776	3647	3650	3655	rVB2	543	387	0.02%	0.002%
74	12.825	3655	3665	3675	rBV6	2394	4198	0.17%	0.024%
75	13.069	3738	3741	3745	rBV2	500	472	0.02%	0.003%
76	13.291	3807	3810	3811	rBV	455	224	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
Data File : VV027119.D
Acq On : 30 Jul 2022 05:59
Operator : SY/MD
Sample : N3899-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUS3

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
Title : VOC Analysis

77	13.718	3940	3943	3945	rBV2	385	187	0.01%	0.001%
78	13.905	3995	4001	4009	rVB6	2982	4108	0.17%	0.023%
79	14.969	4323	4332	4344	rBV6	11327	17660	0.72%	0.100%




Sum of corrected areas: 17728554

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
Data File : VV027119.D
Acq On : 30 Jul 2022 05:59
Operator : SY/MD
Sample : N3899-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUS3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

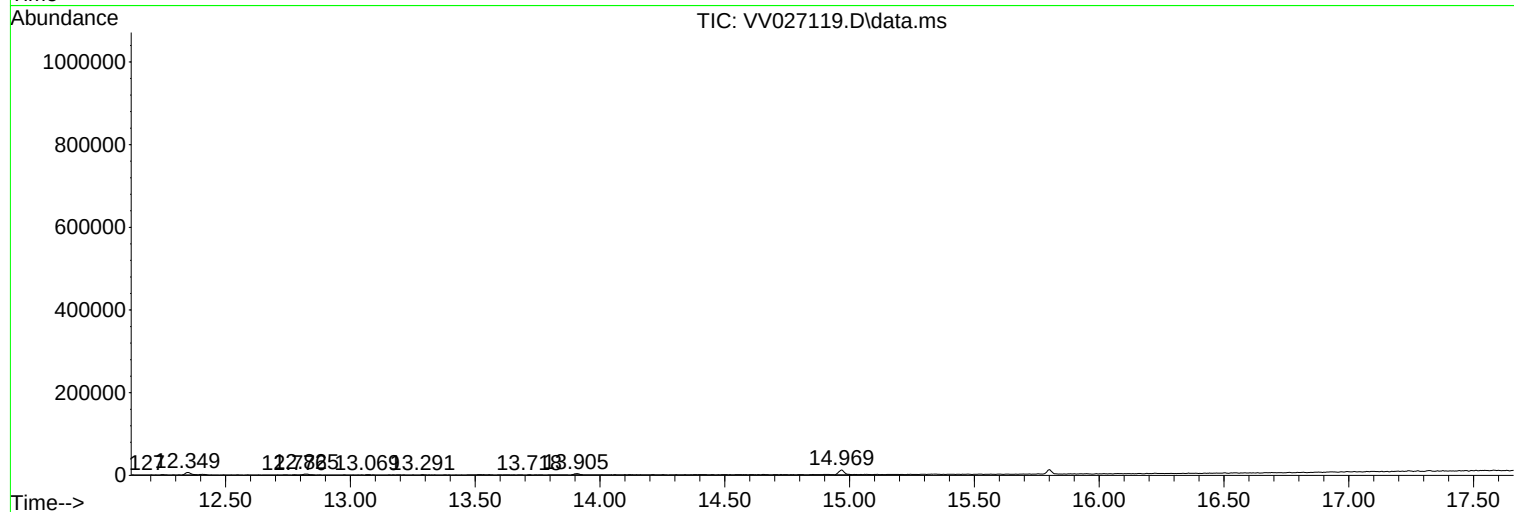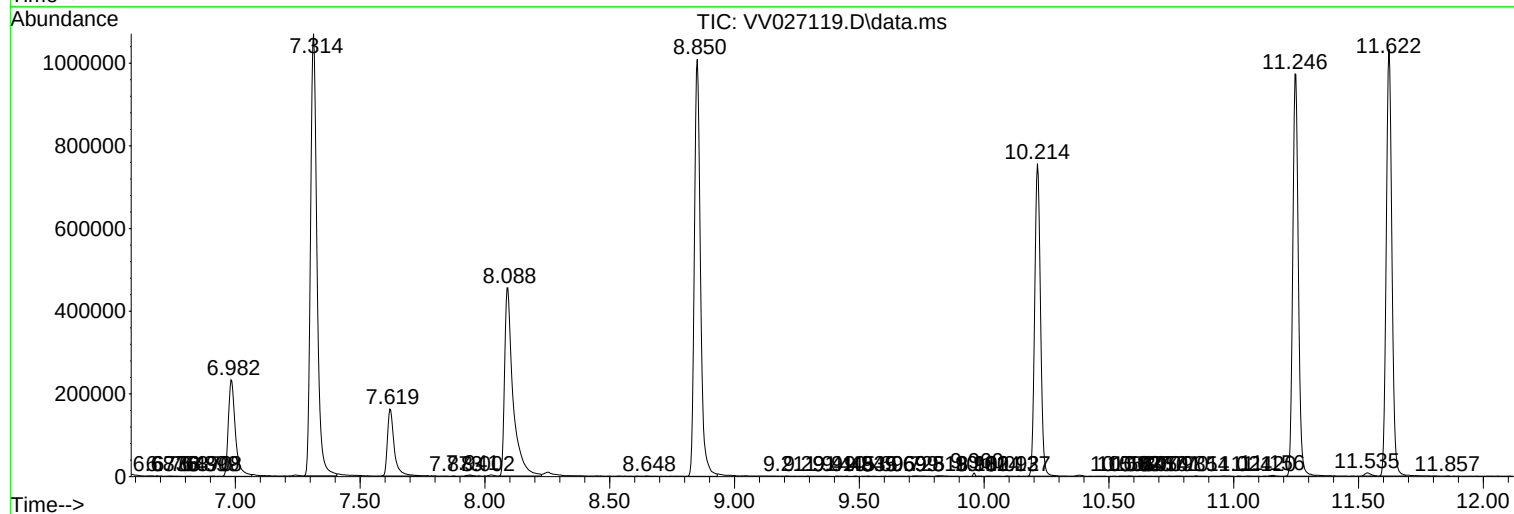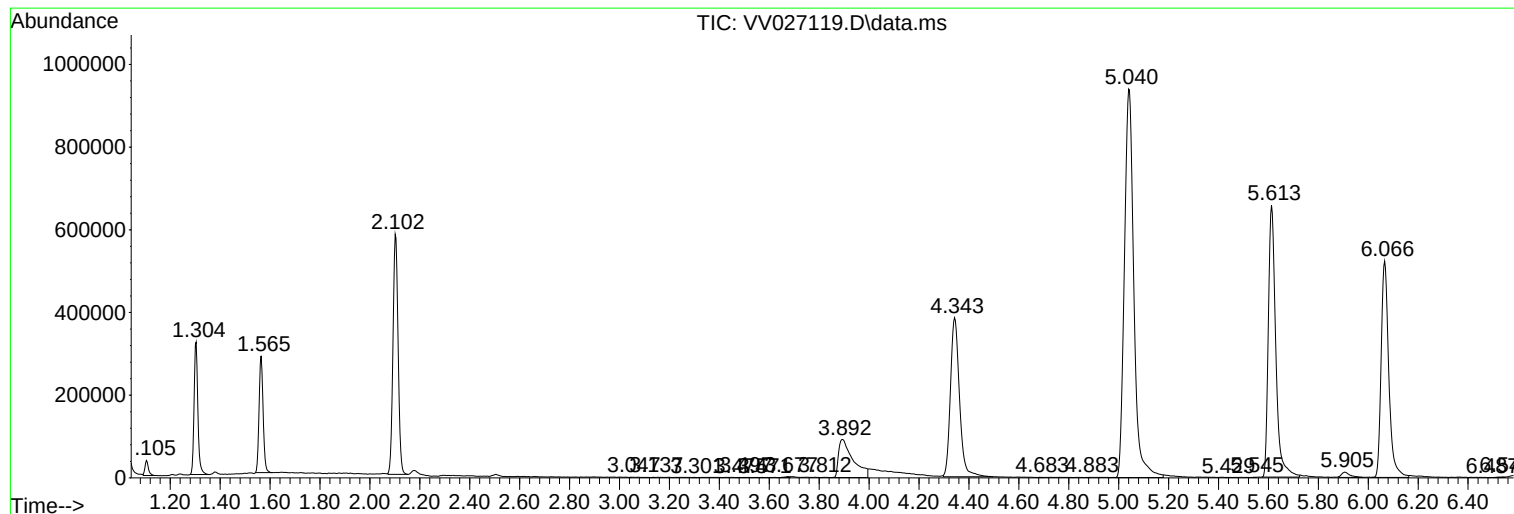

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
Data File : VV027119.D
Acq On : 30 Jul 2022 05:59
Operator : SY/MD
Sample : N3899-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUS3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
Data File : VV027119.D
Acq On : 30 Jul 2022 05:59
Operator : SY/MD
Sample : N3899-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBUS3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc