


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072922\
 Data File : VV027073.D
 Acq On : 29 Jul 2022 10:10
 Operator : SY/MD
 Sample : BFB302
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB302

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM072822WMA.M
 Title : VOC Analysis
 Last Update : Sat Jul 30 01:28:32 2022

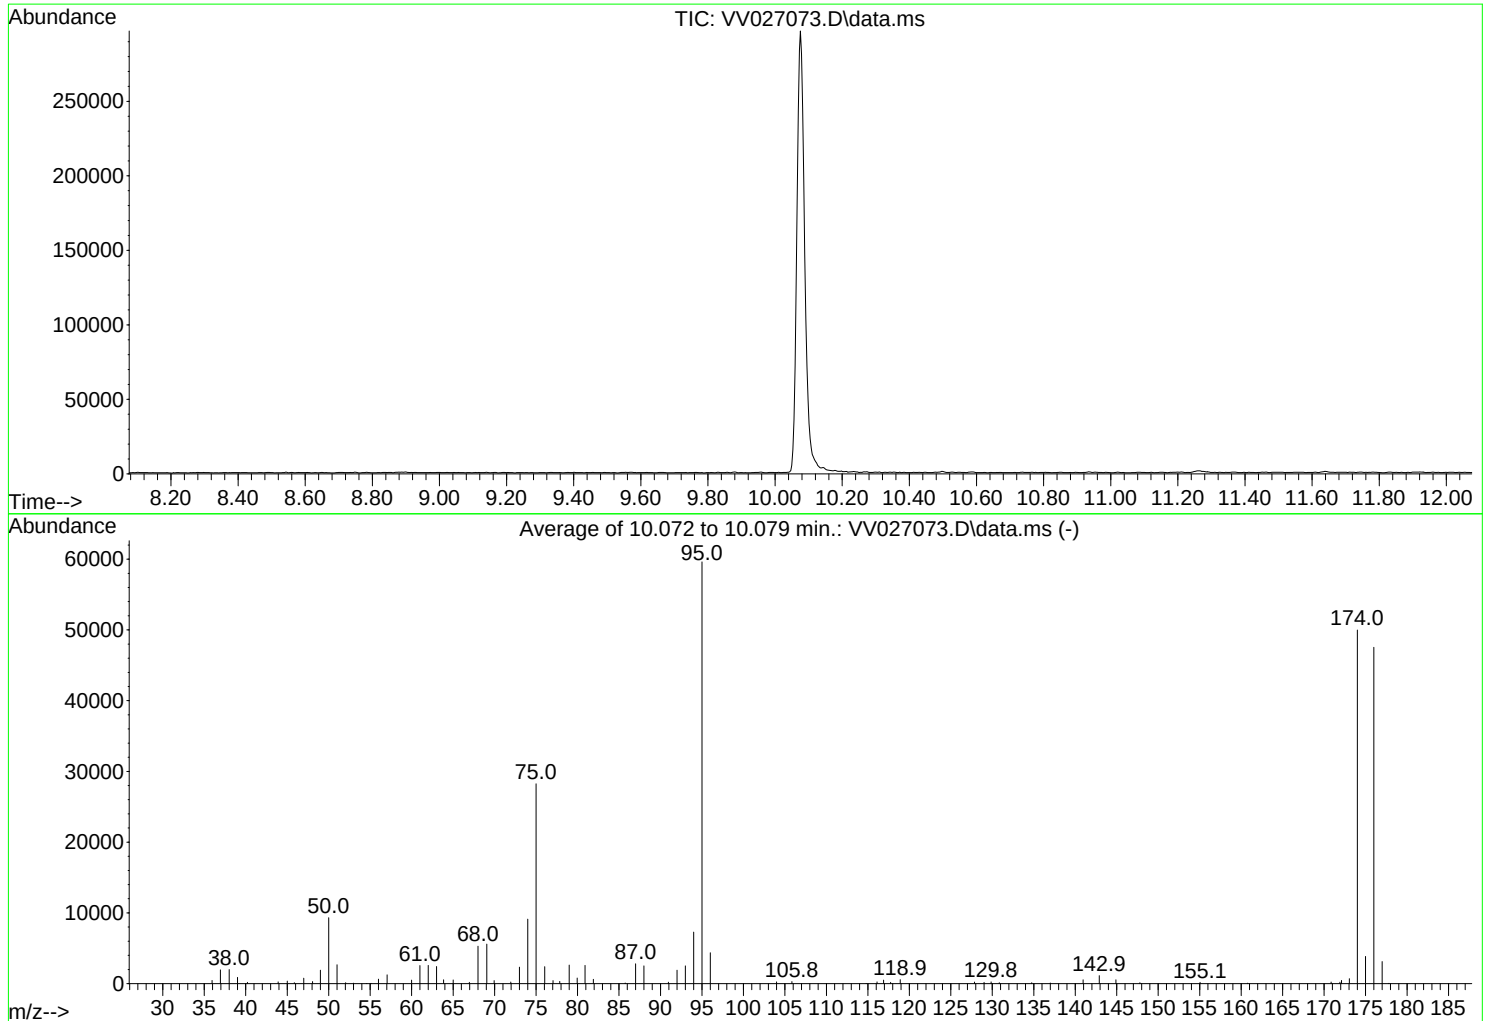

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2798

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.6	9320	PASS
75	95	30	80	47.4	28240	PASS
95	95	100	100	100.0	59624	PASS
96	95	5	9	7.3	4366	PASS
173	174	0.00	2	1.4	704	PASS
174	95	50	120	83.8	49984	PASS
175	174	5	9	7.7	3838	PASS
176	174	95	105	95.1	47533	PASS
177	176	5	10	6.6	3117	PASS

m/z	Abundance
39.90	430.0
43.90	606.0

Instrument :
MSVOA_V
ClientSampleId :
BFB302

m/z	Abundance
36.00	486.0
37.00	2121.0
38.00	2017.0
39.00	899.0
39.90	349.0
44.00	934.0
45.00	421.0
45.80	108.0
47.00	748.0
48.00	249.0
49.00	2063.0
50.00	9309.0
51.00	2583.0
52.00	127.0
55.10	139.0
56.00	693.0
57.10	1276.0
60.00	476.0
61.00	2509.0
62.00	2576.0
63.00	2320.0
63.80	605.0
65.00	466.0
67.00	192.0
68.00	5266.0
69.10	5501.0
70.00	477.0
72.10	242.0
73.00	2374.0
74.00	9044.0
75.00	28480.0
76.10	2527.0
77.00	418.0
77.80	265.0
79.00	2657.0
79.90	719.0
80.90	2391.0
81.90	520.0
85.80	140.0
87.00	2765.0
88.00	2394.0
91.00	197.0
92.00	1944.0
93.00	2288.0
94.00	7017.0
95.00	59656.0
96.00	4728.0
104.00	264.0
105.80	271.0
116.10	234.0
116.90	482.0
117.80	204.0
118.90	600.0
127.80	178.0
129.10	194.0
129.90	256.0
130.80	118.0
134.80	137.0
141.00	573.0
142.90	1168.0
144.90	559.0
147.80	136.0
155.10	138.0
170.80	220.0
171.90	645.0
173.10	658.0
174.00	48480.0
175.00	3969.0
176.00	45888.0
177.00	3112.0

Instrument :
MSVOA_V
ClientSampleId :
BFB302

m/z	Abundance
35.90	481.0
36.90	2027.0
38.00	2039.0
39.00	881.0
39.80	326.0
40.20	295.0
43.90	851.0
45.00	343.0
45.90	138.0
47.00	798.0
48.00	295.0
49.00	1908.0
50.00	9606.0
51.00	2685.0
52.10	134.0
53.00	102.0
56.00	664.0
57.10	1273.0
60.00	508.0
61.00	2644.0
62.00	2597.0
63.00	2539.0
63.90	548.0
65.00	541.0
66.90	193.0
68.00	5393.0
69.00	5807.0
70.00	426.0
71.90	214.0
73.00	2392.0
74.00	9530.0
75.00	29112.0
76.00	2473.0
77.00	441.0
77.80	330.0
79.00	2728.0
79.90	793.0
80.90	2659.0
81.90	653.0
85.70	120.0
87.00	2928.0
88.00	2568.0
90.90	195.0
92.00	2001.0
93.00	2606.0
94.00	7605.0
95.00	61584.0
96.00	4502.0
104.00	272.0
105.90	313.0
114.80	100.0
116.10	269.0
116.90	536.0
117.70	179.0
118.90	575.0
127.90	223.0
129.00	187.0
129.90	276.0
130.80	148.0
134.70	152.0
137.00	119.0
141.00	567.0
142.90	1188.0
144.90	576.0
147.80	136.0
155.10	190.0
160.80	112.0
170.80	228.0
172.10	633.0
173.00	753.0
174.00	51576.0
175.00	4017.0
176.00	49184.0
177.00	3197.0

Instrument :
MSVOA_V
ClientSampleId :
BFB302

m/z	Abundance
35.90	378.0
36.90	1700.0
38.00	1899.0
39.00	852.0
39.80	298.0
40.20	274.0
43.90	811.0
45.00	294.0
45.90	165.0
47.00	797.0
48.10	307.0
49.00	1751.0
50.00	9044.0
51.00	2736.0
52.10	126.0
53.00	101.0
54.60	105.0
56.00	574.0
57.00	1210.0
60.00	532.0
61.00	2522.0
62.00	2535.0
63.00	2434.0
63.90	448.0
65.00	572.0
66.90	165.0
68.00	5236.0
69.00	5449.0
69.90	384.0
71.90	195.0
73.00	2258.0
74.00	8754.0
75.00	27128.0
76.00	2199.0
77.10	403.0
77.90	386.0
79.00	2476.0
80.00	845.0
80.90	2680.0
81.90	674.0
87.00	2749.0
88.00	2557.0
90.90	206.0
92.00	1766.0
93.00	2648.0
94.00	7221.0
95.00	57632.0
96.00	3869.0
104.00	228.0
105.90	281.0
116.10	248.0
116.90	508.0
117.70	181.0
118.90	509.0
127.90	249.0
128.90	144.0
129.80	252.0
130.90	131.0
134.70	143.0
137.00	139.0
140.90	526.0
142.90	1059.0
144.90	523.0
147.80	118.0
155.00	216.0
160.80	123.0
170.90	238.0
172.10	715.0
173.00	701.0
174.00	49896.0
175.00	3528.0
176.00	47528.0
177.00	3042.0
177.80	108.0

Instrument :
MSVOA_V
ClientSampleId :
BFB302