

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV073018\
 Data File : VV006762.D
 Acq On : 30 Jul 2018 14:50
 Operator : SY/MD
 Sample : J4209-01 20X
 Misc : 25 mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AB6

Quant Time: Jul 30 17:20:26 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072318WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Jul 30 16:58:50 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	232024	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	217422	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	89885	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	66176	5.48	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	109.60%
7) Chloroethane-d5	1.58	69	53889	5.68	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	113.60%
11) 1,1-Dichloroethene-d2	2.13	63	91190	3.85	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	77.00%
20) 2-Butanone-d5	3.96	46	198535	52.62	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	105.24%
24) Chloroform-d	4.41	84	122467	5.40	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	108.00%
26) 1,2-Dichloroethane-d4	5.09	65	63895	5.78	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	115.60%
32) Benzene-d6	5.10	84	251906	5.64	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	112.80%
36) 1,2-Dichloropropane-d6	6.12	67	84105	5.57	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	111.40%
41) Toluene-d8	7.37	98	206360	5.28	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	105.60%
43) trans-1,3-Dichloropropene-	7.67	79	25964	5.27	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	105.40%
46) 2-Hexanone-d5	8.14	63	152242	48.81	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	97.62%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	61953	5.03	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	100.60%
64) 1,2-Dichlorobenzene-d4	11.68	152	76356	5.70	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	114.00%


Target Compounds					Ovalue
13) Acetone	2.21	43	22154	9.23 ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV073018\
Data File : VV006762.D
Acq On : 30 Jul 2018 14:50
Operator : SY/MD
Sample : J4209-01 20X
Misc : 25 mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AB6

Quant Time: Jul 30 17:20:26 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072318WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Jul 30 16:58:50 2018
Response via : Initial Calibration

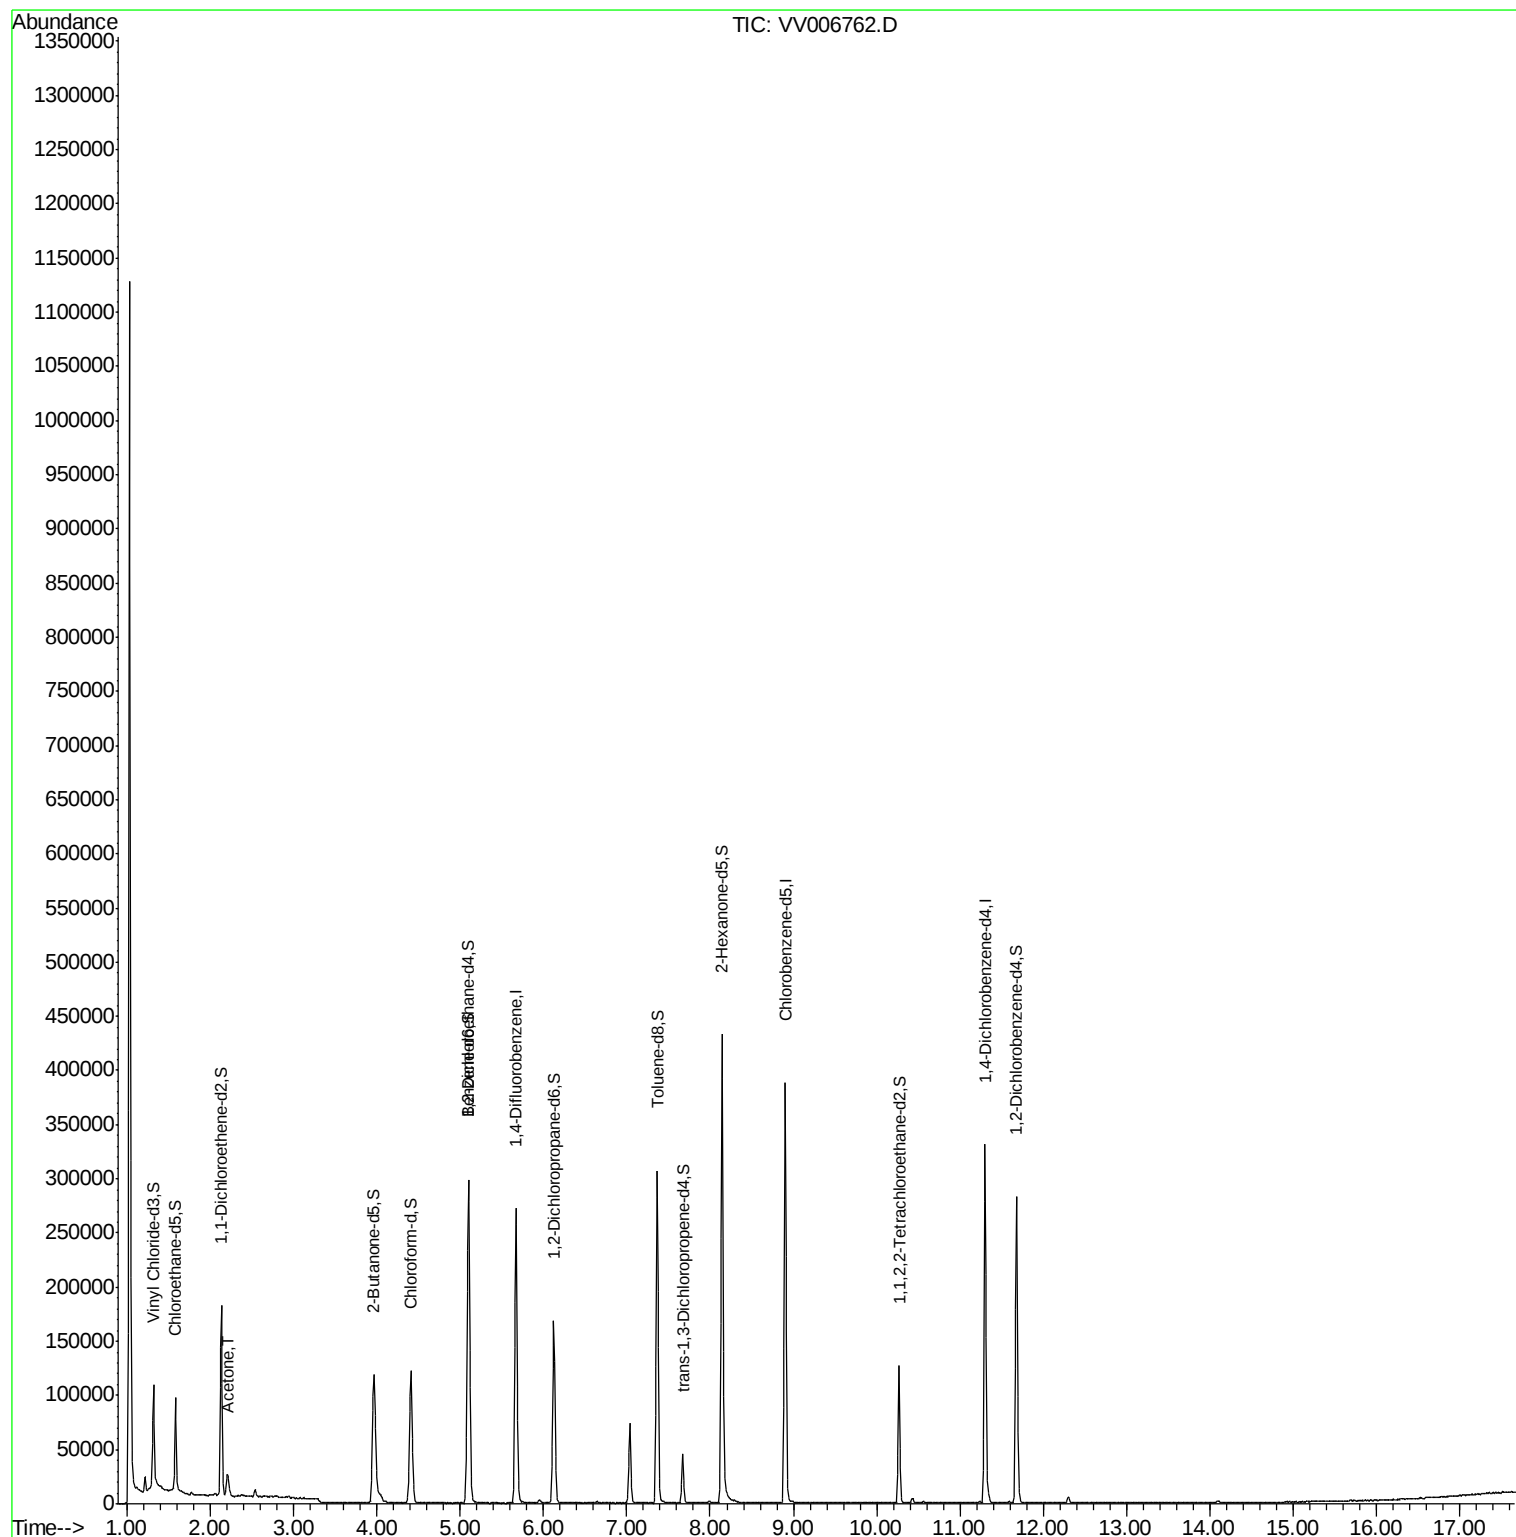

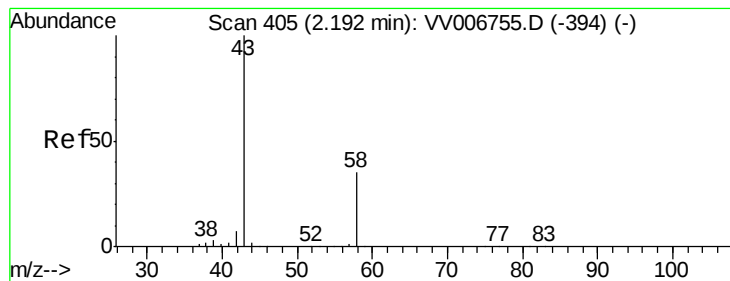

#13

Acetone

Concen: 9.23 ug/L

RT: 2.21 min Scan# 409

Delta R.T. 0.00 min

Lab File: VV006762.D

Acq: 30 Jul 2018 14:50

Instrument :
MSVOA_V
ClientSampleId :
C0AB6

Tot Ion: 43 Resp: 22154

Ion Ratio Lower Upper

43 100

58 36.2 0.0 71.4

