

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV073018\
 Data File : VV006763.D
 Acq On : 30 Jul 2018 15:24
 Operator : SY/MD
 Sample : J4209-01 10X
 Misc : 25 mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AB6

Quant Time: Jul 30 17:23:05 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072318WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Jul 30 16:58:50 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	226178	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	208994	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	87426	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	62356	5.30	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	106.00%
7) Chloroethane-d5	1.58	69	52228	5.65	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	113.00%
11) 1,1-Dichloroethene-d2	2.13	63	85588	3.71	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	74.20%
20) 2-Butanone-d5	3.96	46	186223	50.63	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	101.26%
24) Chloroform-d	4.40	84	120679	5.46	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	109.20%
26) 1,2-Dichloroethane-d4	5.09	65	62229	5.78	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	115.60%
32) Benzene-d6	5.10	84	245152	5.71	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	114.20%
36) 1,2-Dichloropropane-d6	6.12	67	81291	5.60	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	112.00%
41) Toluene-d8	7.36	98	200238	5.33	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	106.60%
43) trans-1,3-Dichloropropene-	7.67	79	24977	5.27	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	105.40%
46) 2-Hexanone-d5	8.14	63	146300	48.79	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	97.58%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	59412	5.02	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	100.40%
64) 1,2-Dichlorobenzene-d4	11.68	152	74840	5.74	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	114.80%


Target Compounds					Ovalue
13) Acetone	2.21	43	43932	18.77 ug/L	98
16) Methylene chloride	2.54	84	6059	0.36 ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV073018\
Data File : VV006763.D
Acq On : 30 Jul 2018 15:24
Operator : SY/MD
Sample : J4209-01 10X
Misc : 25 mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AB6

Quant Time: Jul 30 17:23:05 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072318WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Jul 30 16:58:50 2018
Response via : Initial Calibration

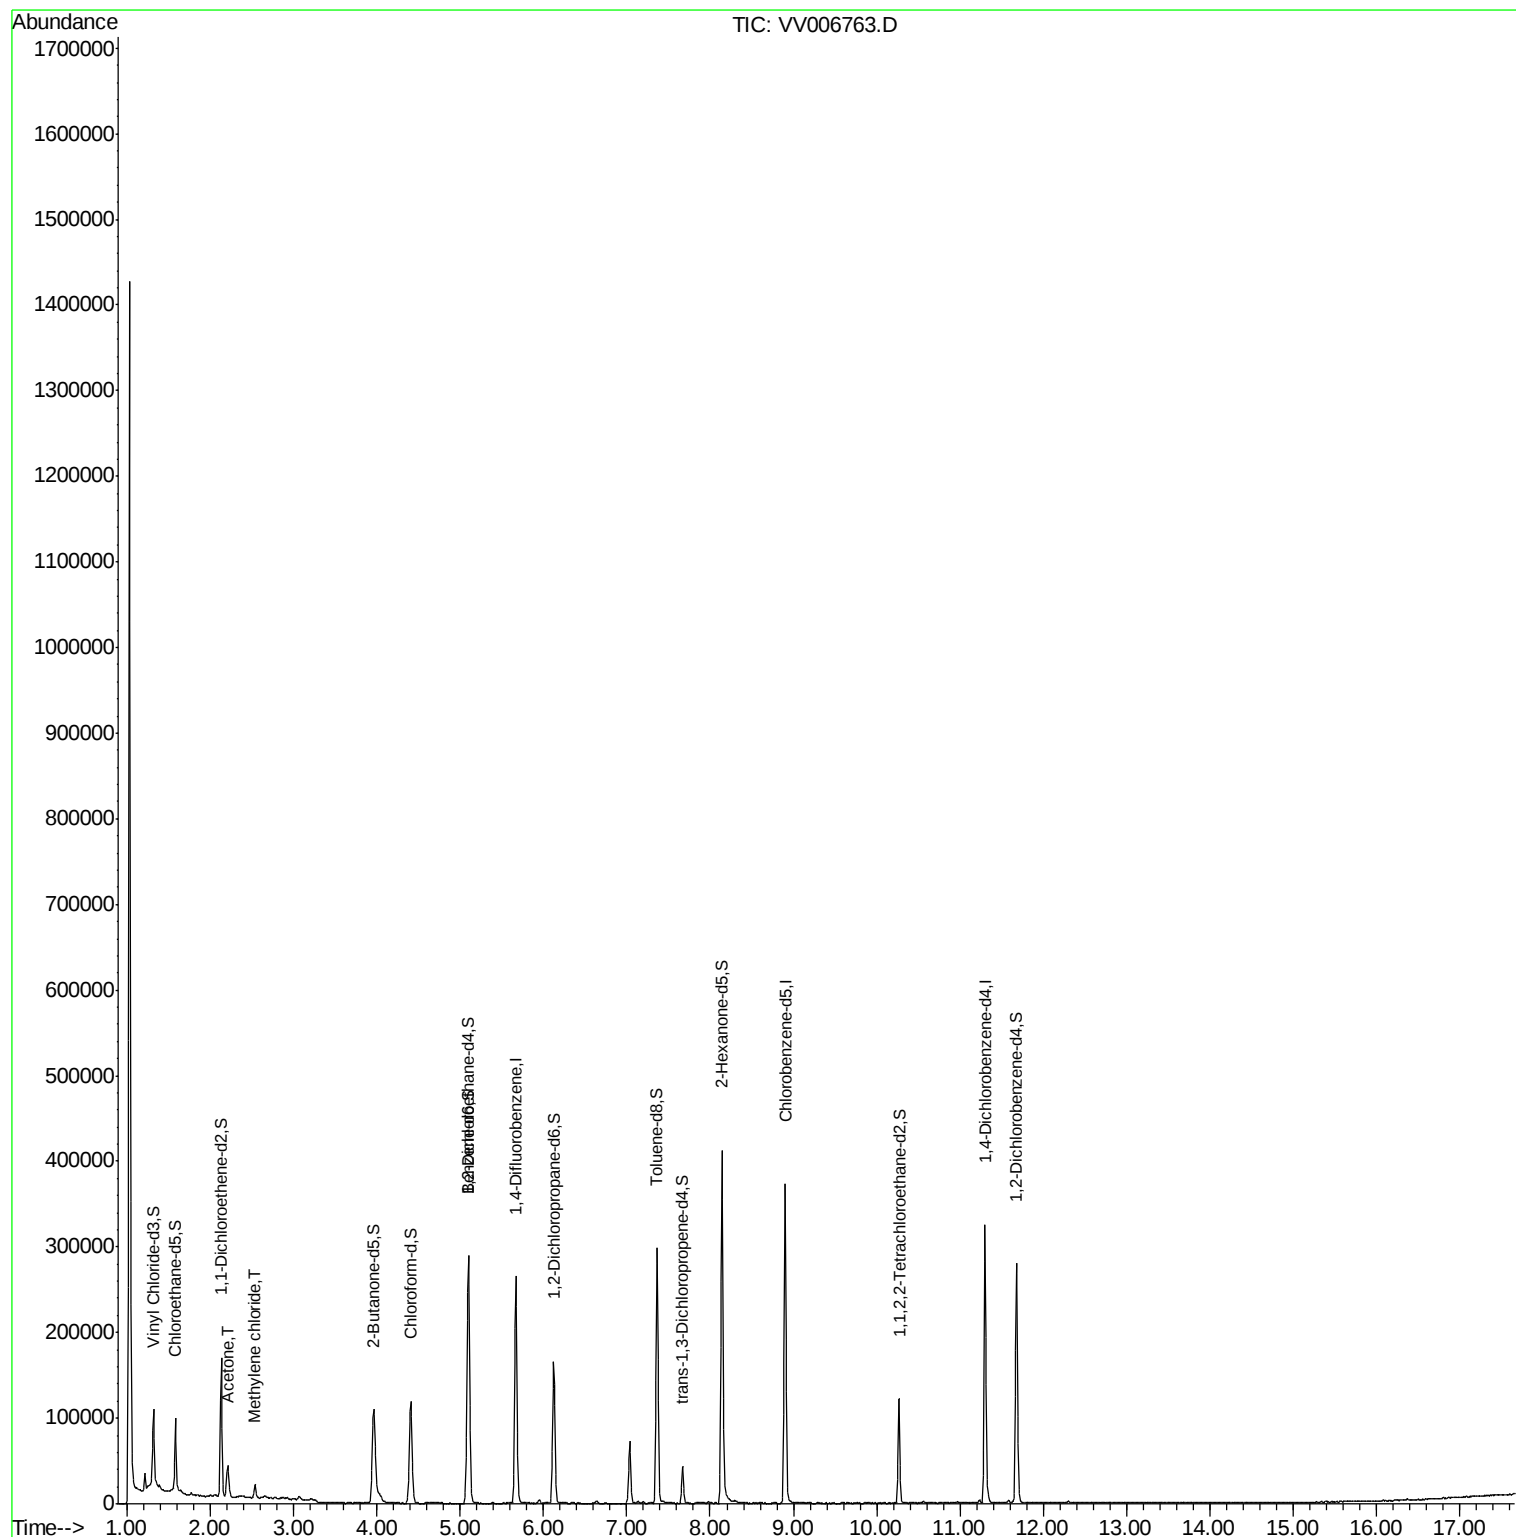

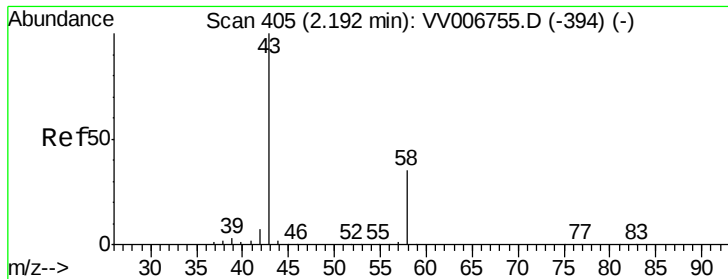

#13

Acetone

Concen: 18.77 ug/L

RT: 2.21 min Scan# 410

Delta R.T. 0.01 min

Lab File: VV006763.D

Acq: 30 Jul 2018 15:24

Instrument :

MSVOA_V

ClientSampled :


C0AB6

Tot Ion: 43 Resp: 43932

Ion Ratio Lower Upper

43 100

58 36.9 0.0 71.4

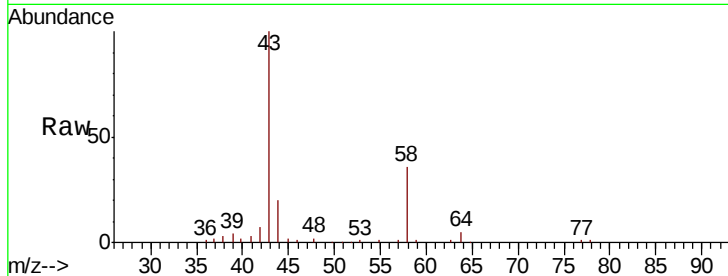

Abundance Ion 43.05 (42.75 to 43.75): VV006763.D (-410) (-)

Ion 58.05 (57.75 to 58.75): VV006763.D (-410) (-)

25000

20000

15000

10000



5000

0

Time-->

2.15 2.20 2.25 2.30

2.21

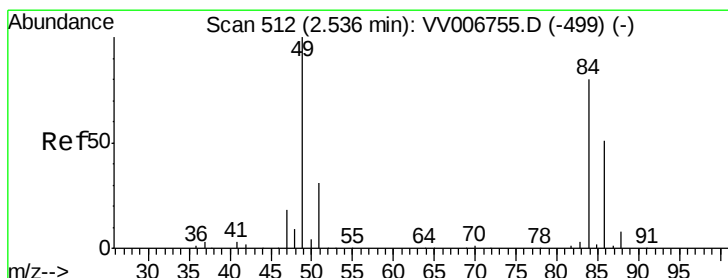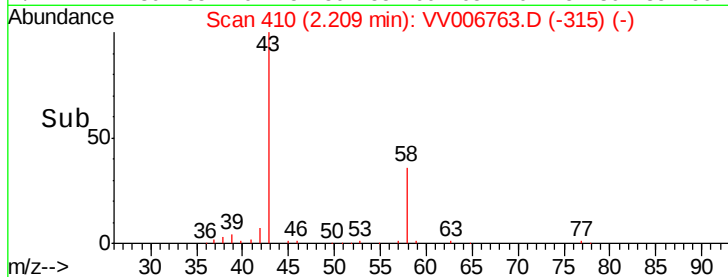

#16

Methylene chloride

Concen: 0.36 ug/L

RT: 2.54 min Scan# 512

Delta R.T. -0.00 min

Lab File: VV006763.D

Acq: 30 Jul 2018 15:24


Tgt Ion: 84 Resp: 6059

Ion Ratio Lower Upper

84 100

86 64.4 44.7 83.1

49 130.4 86.7 160.9

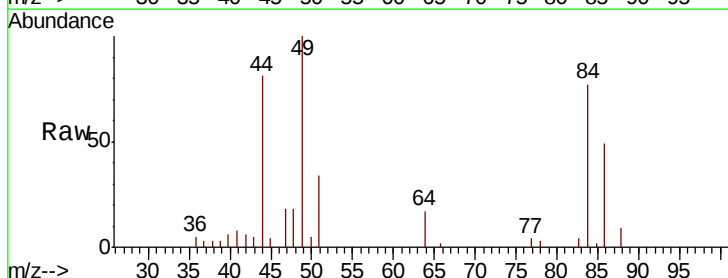

Abundance Ion 84.05 (83.75 to 84.75): VV006763.D (-512) (-)

Ion 86.00 (85.70 to 86.70): VV006763.D (-512) (-)

Ion 49.10 (48.80 to 49.80): VV006763.D (-512) (-)

6000

5000

4000

3000

2000

1000

0

Time-->

2.50 2.55 2.60

2.54

