

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV073018\
 Data File : VV006764.D
 Acq On : 30 Jul 2018 15:56
 Operator : SY/MD
 Sample : J4209-06
 Misc : 26 mL/MSVOA V/WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AC1

Quant Time: Jul 30 17:25:54 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072318WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Jul 30 16:58:50 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	256602	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	242786	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	97006	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	63108	4.73	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	94.60%
7) Chloroethane-d5	1.58	69	52996	5.05	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	101.00%
11) 1,1-Dichloroethene-d2	2.13	63	87323	3.33	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	66.60%
20) 2-Butanone-d5	3.95	46	177709	42.59	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	85.18%
24) Chloroform-d	4.40	84	118949	4.75	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.00%
26) 1,2-Dichloroethane-d4	5.09	65	61830	5.06	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.20%
32) Benzene-d6	5.10	84	241193	4.83	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.60%
36) 1,2-Dichloropropane-d6	6.12	67	80592	4.78	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	95.60%
41) Toluene-d8	7.36	98	199417	4.57	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.40%
43) trans-1,3-Dichloropropene-	7.67	79	23936	4.35	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	87.00%
46) 2-Hexanone-d5	8.14	63	137380	39.44	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	78.88%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	58705	4.27	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	85.40%
64) 1,2-Dichlorobenzene-d4	11.68	152	74288	5.14	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	102.80%


Target Compounds					Ovalue
13) Acetone	2.19	43	10354	3.90 ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV073018\
Data File : VV006764.D
Acq On : 30 Jul 2018 15:56
Operator : SY/MD
Sample : J4209-06
Misc : 26 mL/MSVOA V/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AC1

Quant Time: Jul 30 17:25:54 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072318WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Jul 30 16:58:50 2018
Response via : Initial Calibration

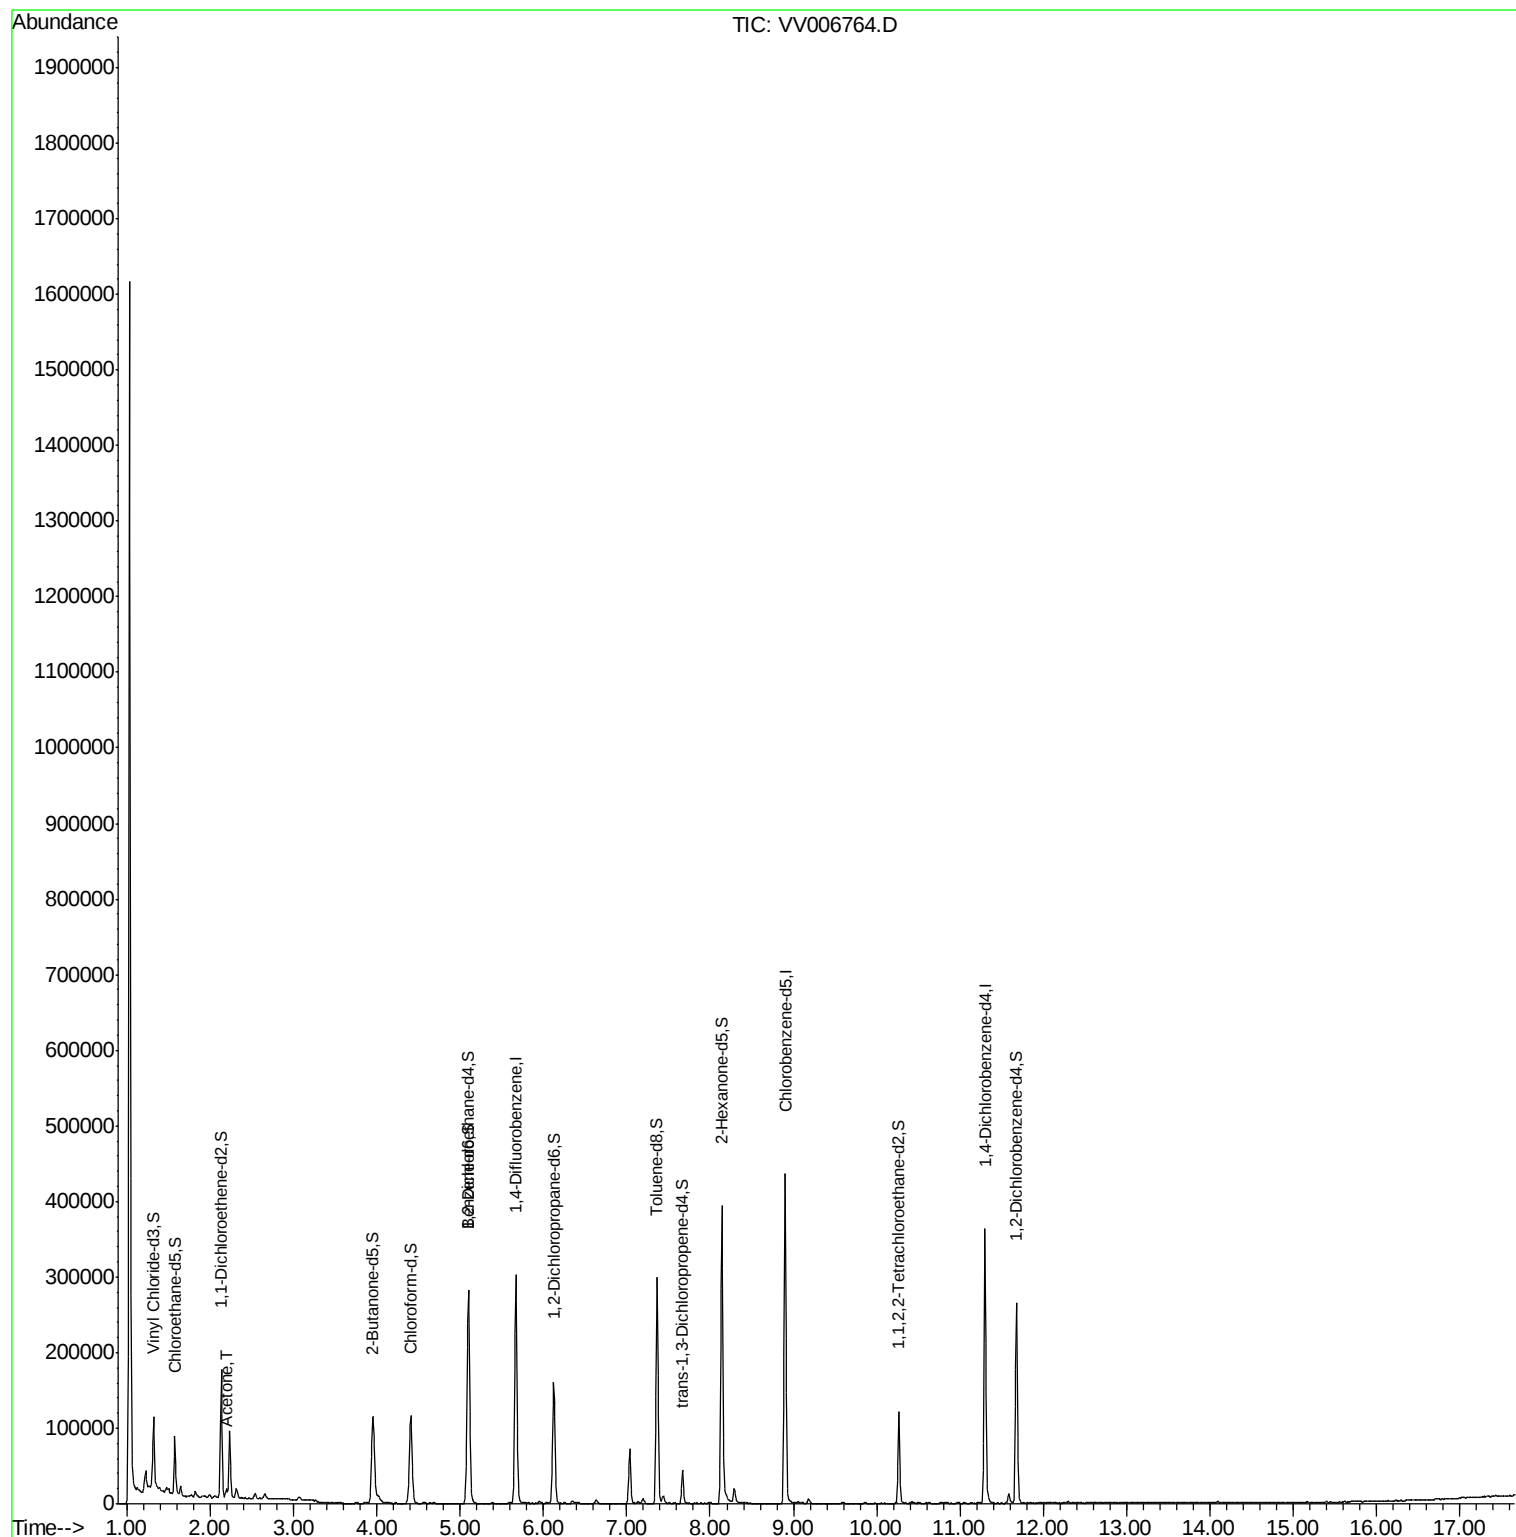

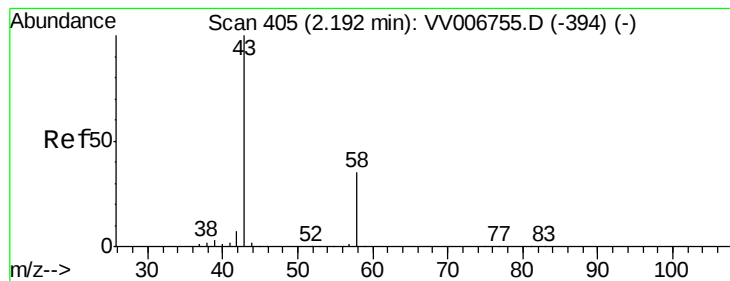

#13
 Acetone
 Concen: 3.90 ug/L
 RT: 2.19 min Scan# 405
 Delta R.T. -0.01 min
 Lab File: VV006764.D
 Acq: 30 Jul 2018 15:56

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AC1

Tot Ion: 43 Resp: 10354
 Ion Ratio Lower Upper
 43 100
 58 33.3 0.0 71.4

