

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV073018\
 Data File : VV006765.D
 Acq On : 30 Jul 2018 16:23
 Operator : SY/MD
 Sample : J4204-02
 Misc : 26 mL/MSVOA V/WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 JJ1H7

Quant Time: Jul 30 17:27:58 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072318WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Jul 30 16:58:50 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	253386	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	235977	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	96604	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	60551	4.59	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	91.80%
7) Chloroethane-d5	1.58	69	51273	4.95	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	99.00%
11) 1,1-Dichloroethene-d2	2.13	63	82170	3.18	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	63.60%
20) 2-Butanone-d5	3.95	46	167397	40.63	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	81.26%
24) Chloroform-d	4.41	84	109697	4.43	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.60%
26) 1,2-Dichloroethane-d4	5.09	65	59371	4.92	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.40%
32) Benzene-d6	5.10	84	232713	4.80	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.00%
36) 1,2-Dichloropropane-d6	6.12	67	77535	4.73	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	94.60%
41) Toluene-d8	7.37	98	190892	4.50	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.00%
43) trans-1,3-Dichloropropene-	7.67	79	23123	4.32	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	86.40%
46) 2-Hexanone-d5	8.14	63	129281	38.19	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	76.38%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	56482	4.23	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	84.60%
64) 1,2-Dichlorobenzene-d4	11.68	152	70316	4.88	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	97.60%


Target Compounds					Ovalue
13) Acetone	2.19	43	5826	2.22 ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV073018\
Data File : VV006765.D
Acq On : 30 Jul 2018 16:23
Operator : SY/MD
Sample : J4204-02
Misc : 26 mL/MSVOA V/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
JJ1H7

Quant Time: Jul 30 17:27:58 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072318WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Jul 30 16:58:50 2018
Response via : Initial Calibration

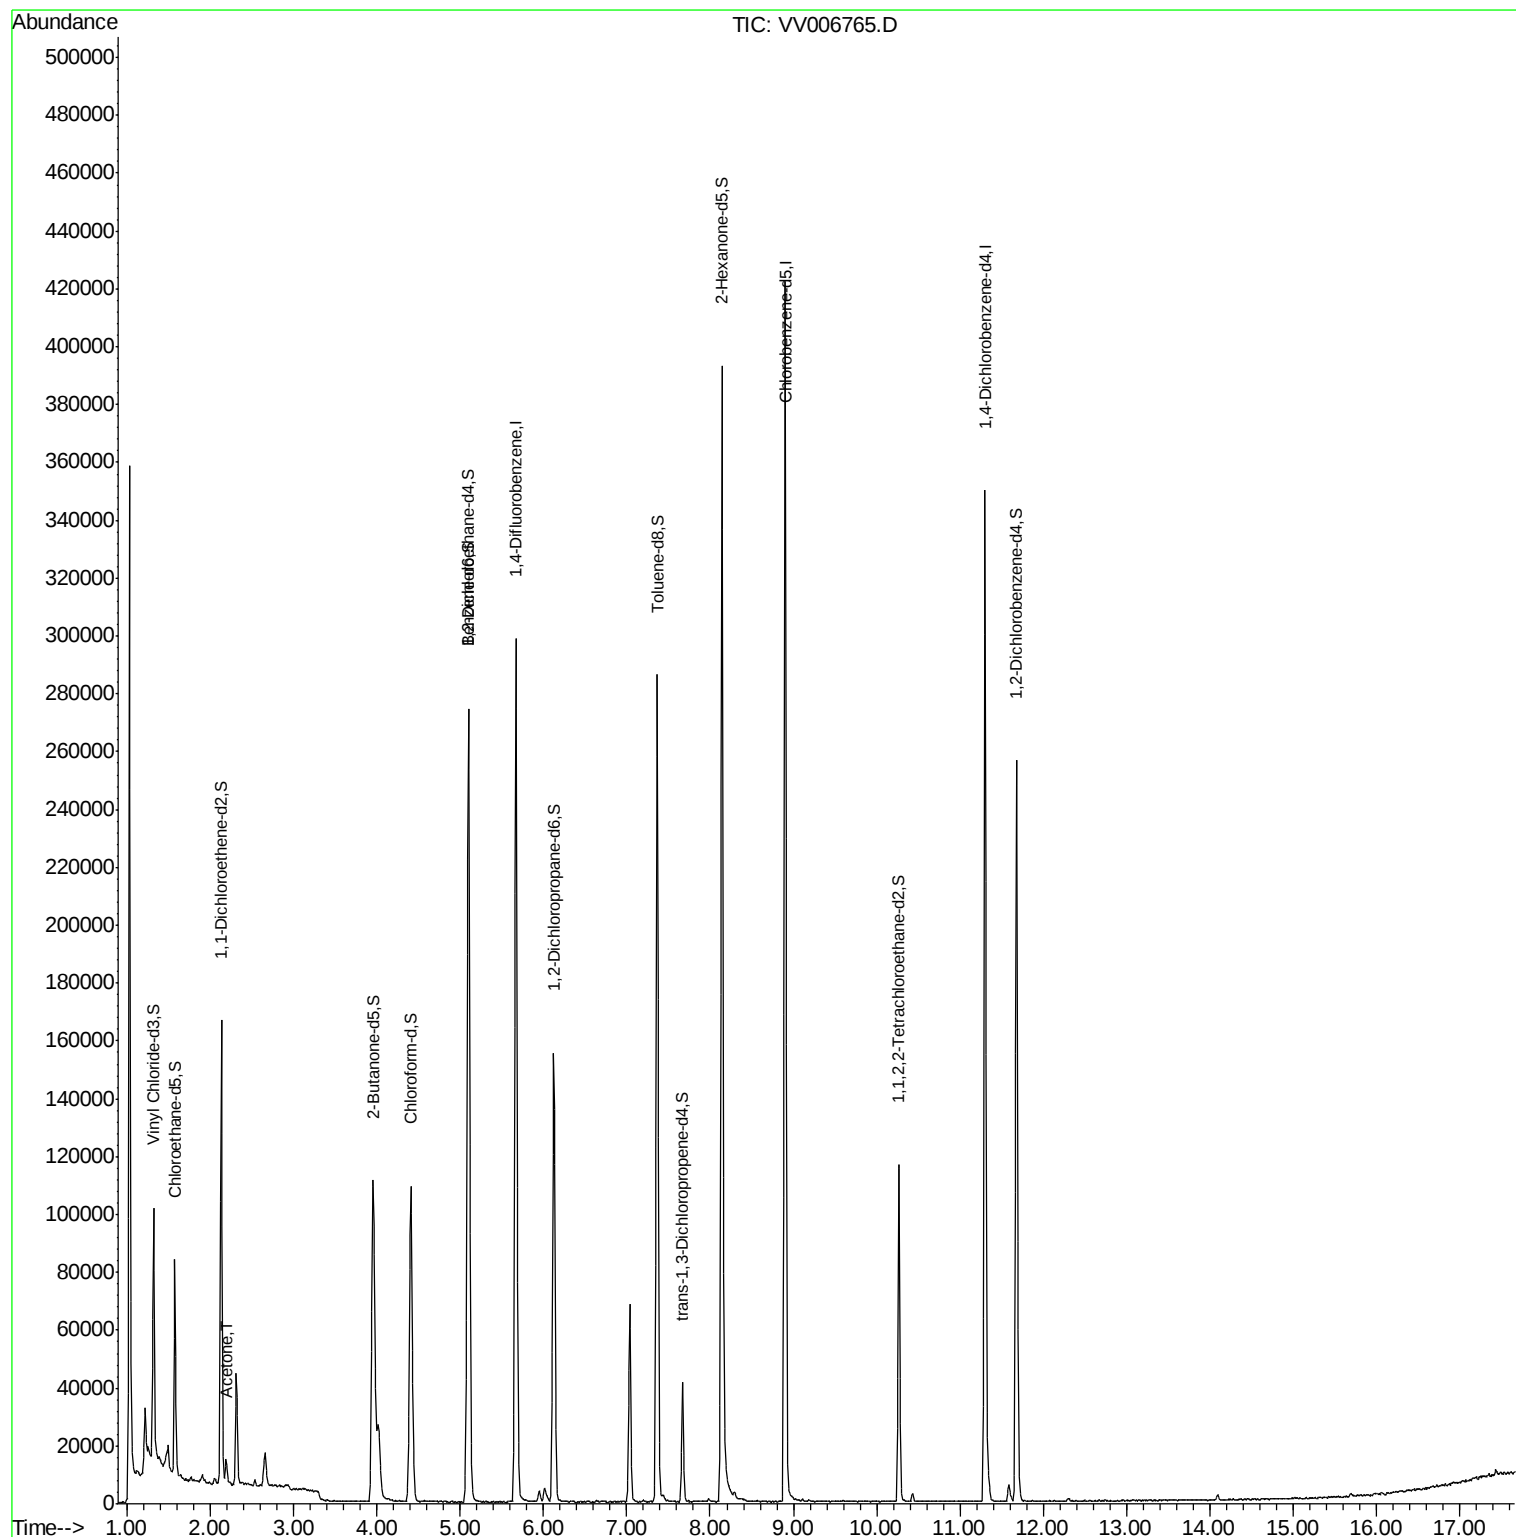

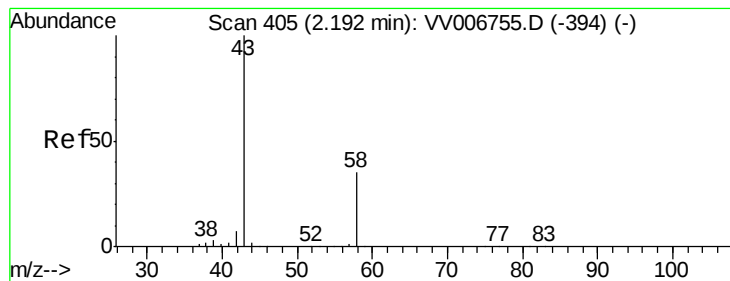

#13
Acetone
Concen: 2.22 ug/L
RT: 2.19 min Scan# 405
Delta R.T. -0.01 min
Lab File: VV006765.D
Acq: 30 Jul 2018 16:23

Instrument :
MSVOA_V
ClientSampleId :
JJ1H7

Tot Ion: 43 Resp: 5826
Ion Ratio Lower Upper
43 100
58 39.8 0.0 71.4

