

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV073018\
 Data File : VV006770.D
 Acq On : 30 Jul 2018 18:42
 Operator : SY/MD
 Sample : J4225-01
 Misc : 25 mL/MSVOA V/WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ESWN8

Quant Time: Jul 30 19:13:23 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072318WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Jul 30 16:58:50 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	190579	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	178139	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	71336	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	50608	5.10	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	102.00%
7) Chloroethane-d5	1.57	69	44269	5.68	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	113.60%
11) 1,1-Dichloroethene-d2	2.13	63	68884	3.54	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	70.80%
20) 2-Butanone-d5	3.95	46	168301	54.31	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	108.62%
24) Chloroform-d	4.40	84	101270	5.44	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	108.80%
26) 1,2-Dichloroethane-d4	5.09	65	53448	5.89	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	117.80%
32) Benzene-d6	5.10	84	203116	5.55	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	111.00%
36) 1,2-Dichloropropane-d6	6.12	67	68955	5.57	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	111.40%
41) Toluene-d8	7.36	98	164200	5.13	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	102.60%
43) trans-1,3-Dichloropropene-	7.67	79	20922	5.18	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	103.60%
46) 2-Hexanone-d5	8.14	63	123569	48.35	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	96.70%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	54818	5.43	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	108.60%
64) 1,2-Dichlorobenzene-d4	11.68	152	60860	5.72	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	114.40%


Target Compounds					Ovalue
13) Acetone	2.19	43	4792	2.43 ug/L	81


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV073018\
Data File : VV006770.D
Acq On : 30 Jul 2018 18:42
Operator : SY/MD
Sample : J4225-01
Misc : 25 mL/MSVOA V/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ESWN8

Quant Time: Jul 30 19:13:23 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072318WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Jul 30 16:58:50 2018
Response via : Initial Calibration

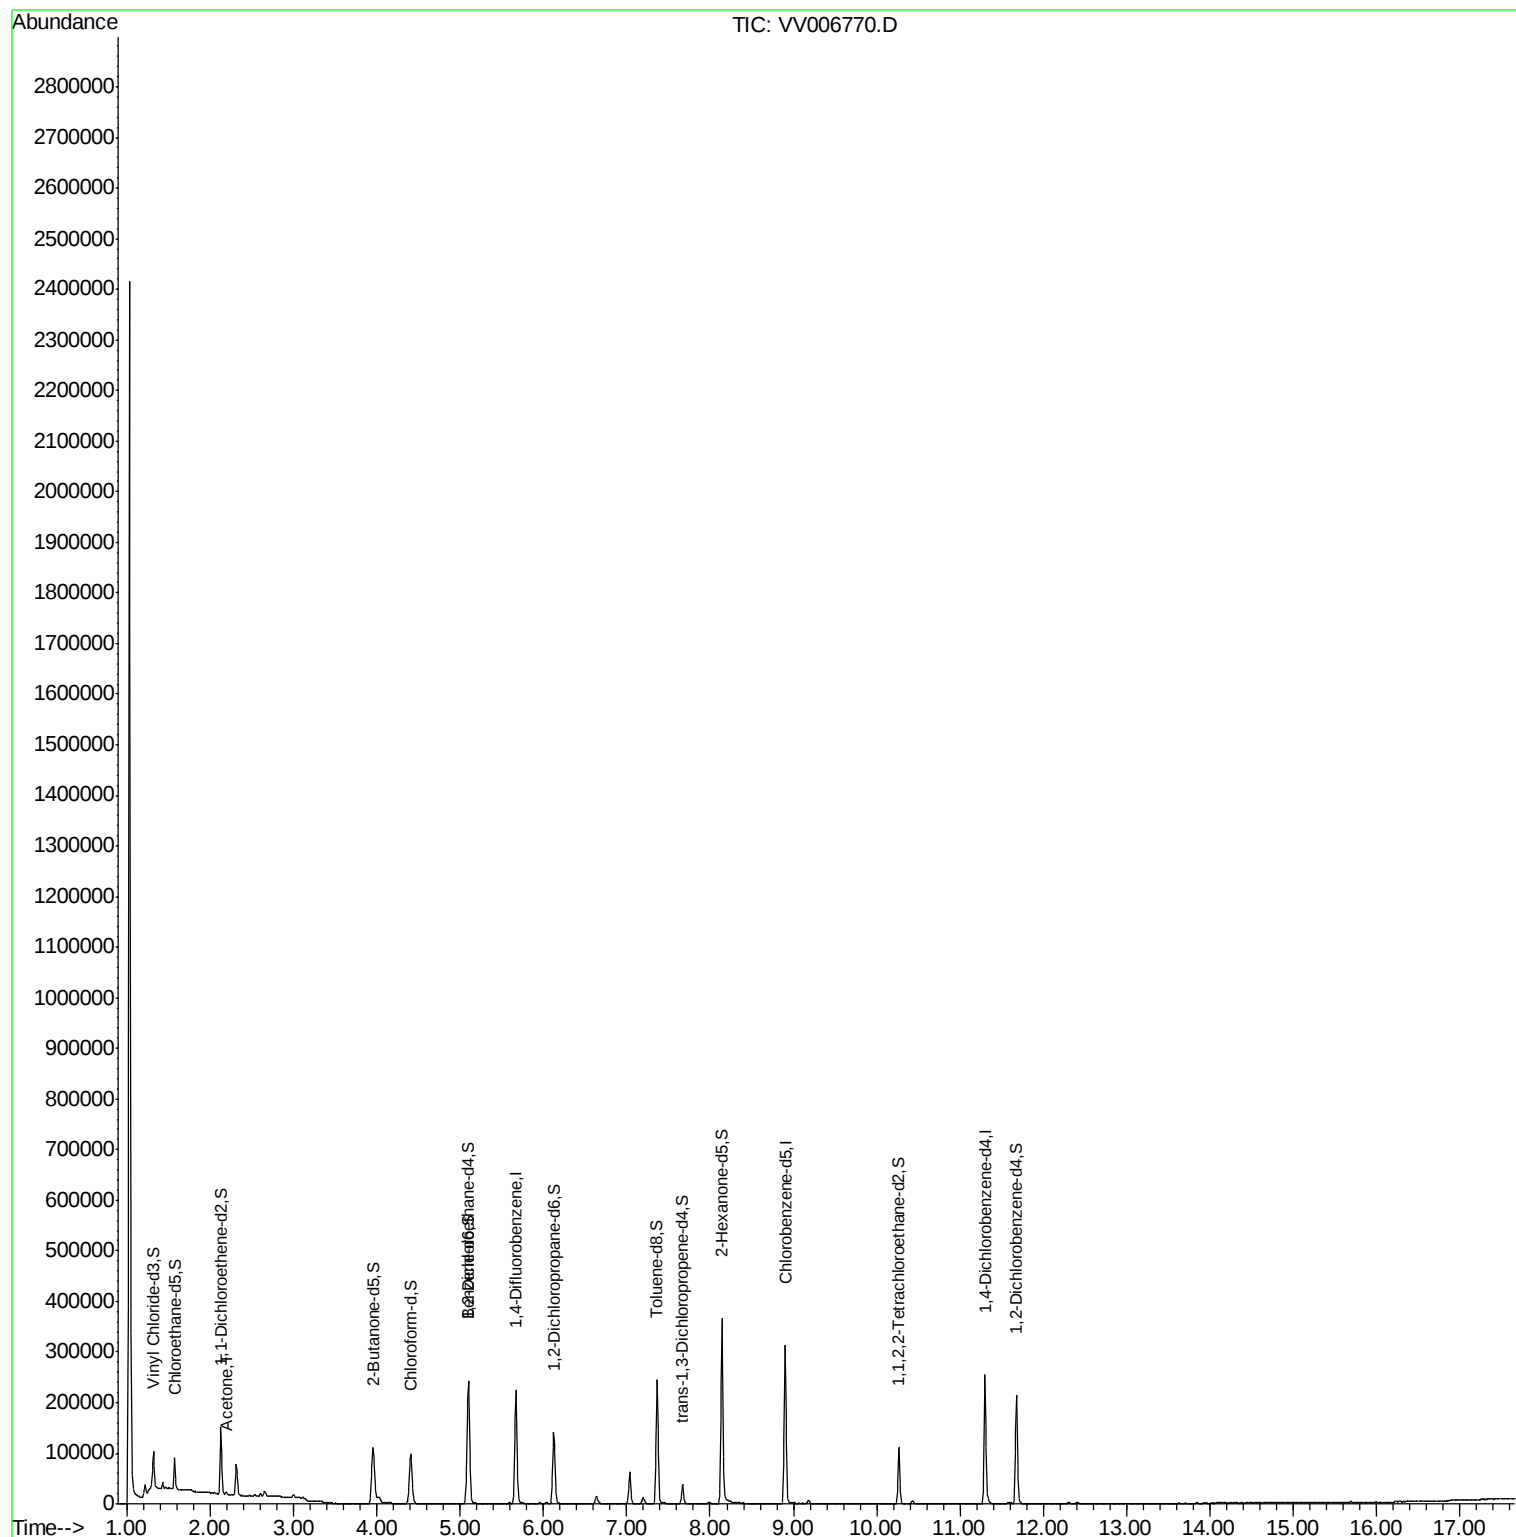

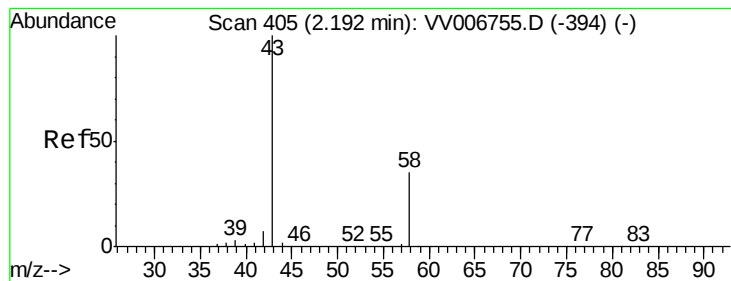

#13

Acetone

Concen: 2.43 ug/L

RT: 2.19 min Scan# 405

Delta R.T. -0.01 min

Lab File: VV006770.D

Acq: 30 Jul 2018 18:42

Instrument :
MSVOA_V
ClientSampleId :
ESWN8

Tot Ion: 43 Resp: 4792

Ion Ratio Lower Upper

43 100

58 24.7 0.0 71.4

