

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV073018\
 Data File : VV006771.D
 Acq On : 30 Jul 2018 19:09
 Operator : SY/MD
 Sample : J4225-02
 Misc : 25 mL/MSVOA V/WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ESWN9

Quant Time: Jul 31 07:45:46 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072318WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Jul 31 07:41:28 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	192713	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	181773	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	72198	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	50115	5.00	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	100.00%
7) Chloroethane-d5	1.57	69	43298	5.50	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	110.00%
11) 1,1-Dichloroethene-d2	2.13	63	68486	3.48	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	69.60%
20) 2-Butanone-d5	3.95	46	171305	54.66	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	109.32%
24) Chloroform-d	4.41	84	102323	5.44	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	108.80%
26) 1,2-Dichloroethane-d4	5.09	65	53716	5.85	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	117.00%
32) Benzene-d6	5.10	84	201943	5.41	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	108.20%
36) 1,2-Dichloropropane-d6	6.12	67	68817	5.45	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	109.00%
41) Toluene-d8	7.37	98	159220	4.87	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.40%
43) trans-1,3-Dichloropropene-	7.67	79	20210	4.91	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	98.20%
46) 2-Hexanone-d5	8.14	63	124133	47.60	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	95.20%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	55130	5.35	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	107.00%
64) 1,2-Dichlorobenzene-d4	11.68	152	61748	5.74	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	114.80%


Target Compounds					Ovalue
13) Acetone	2.19	43	4187	2.10 ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV073018\
Data File : VV006771.D
Acq On : 30 Jul 2018 19:09
Operator : SY/MD
Sample : J4225-02
Misc : 25 mL/MSVOA V/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ESWN9

Quant Time: Jul 31 07:45:46 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072318WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Jul 31 07:41:28 2018
Response via : Initial Calibration

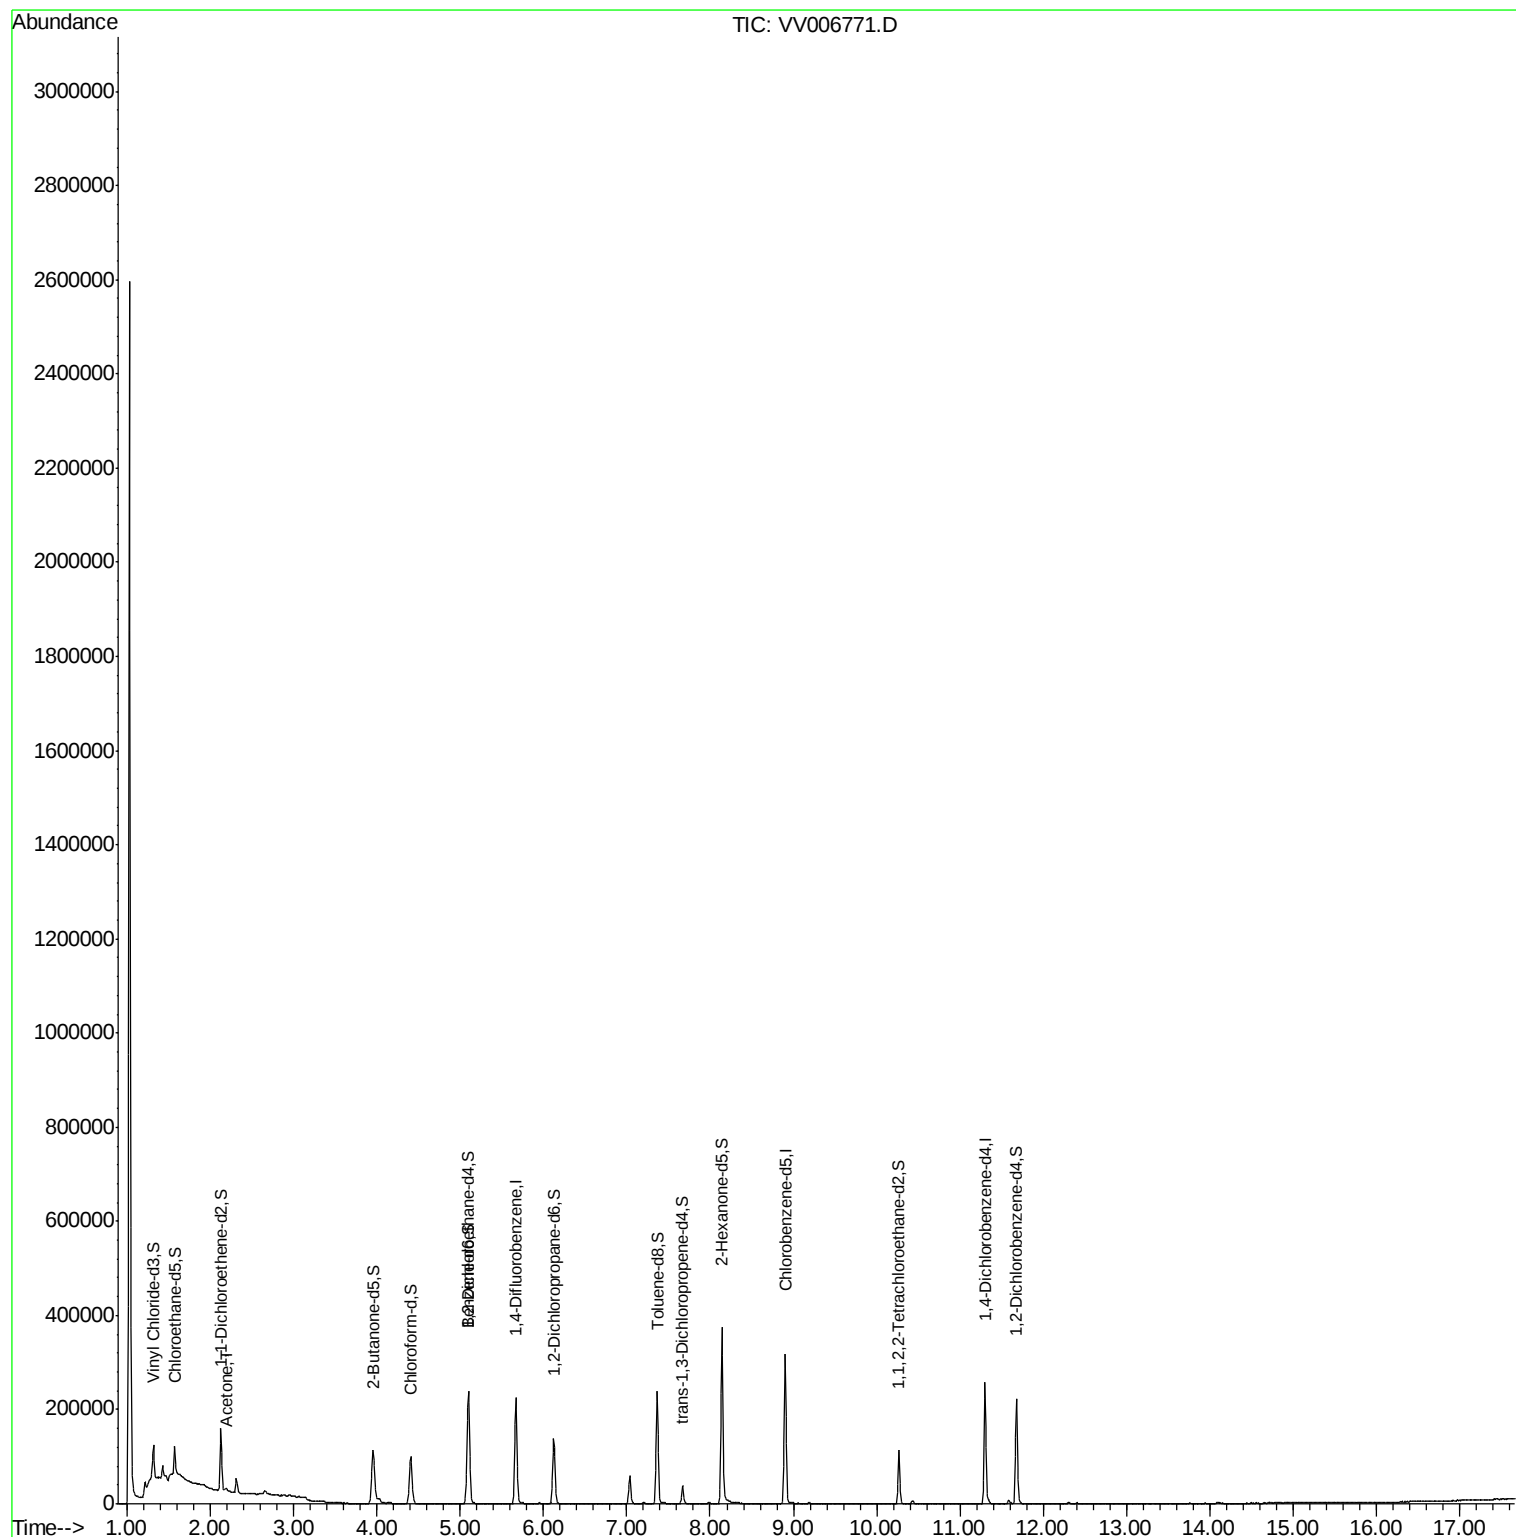

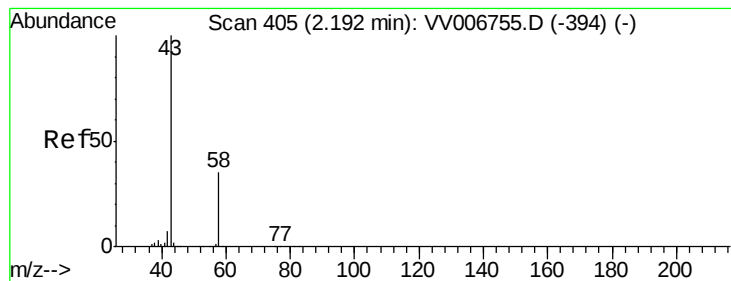

#13
 Acetone
 Concen: 2.10 ug/L
 RT: 2.19 min Scan# 405
 Delta R.T. 0.00 min
 Lab File: VV006771.D
 Acq: 30 Jul 2018 19:09

Instrument :
 MSVOA_V
 ClientSampleId :
 ESWN9

Tot Ion: 43 Resp: 4187
 Ion Ratio Lower Upper
 43 100
 58 30.7 0.0 71.4

