

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV073018\
 Data File : VV006759.D
 Acq On : 30 Jul 2018 13:30
 Operator : SY/MD
 Sample : J4190-07
 Misc : 25 mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BE747

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.1

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072318WMA.M

Title : TRACE VOA SOM01.0

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.029	28	43	68	rBV	1825344	2324326	100.00%	28.569%
2	1.318	124	133	155	rVB	87753	113239	4.87%	1.392%
3	1.579	207	214	228	rVB	75015	89369	3.84%	1.098%
4	2.132	376	386	396	rBV	160805	224237	9.65%	2.756%
5	2.193	398	405	422	rVB	17742	29466	1.27%	0.362%
6	2.318	435	444	460	rVB	36961	69276	2.98%	0.851%
7	3.955	936	953	966	rBV	112505	288276	12.40%	3.543%
8	4.408	1075	1094	1120	rBV	112403	268094	11.53%	3.295%
9	5.099	1292	1309	1331	rBV2	275167	629364	27.08%	7.736%
10	5.668	1471	1486	1510	rBV	298007	577367	24.84%	7.097%
11	6.125	1612	1628	1651	rBV	156337	308018	13.25%	3.786%
12	7.035	1899	1911	1933	rBV2	70957	123386	5.31%	1.517%
13	7.363	2000	2013	2030	rBV	289045	493734	21.24%	6.069%
14	7.668	2098	2108	2124	rBV	42404	69867	3.01%	0.859%
15	8.141	2242	2255	2293	rBV	400453	690969	29.73%	8.493%
16	8.900	2477	2491	2520	rBV	418197	675891	29.08%	8.308%
17	10.269	2905	2917	2932	rBV	115364	180158	7.75%	2.214%
18	11.302	3226	3238	3267	rBV	354152	566907	24.39%	6.968%
19	11.678	3342	3355	3378	rVB	257690	413875	17.81%	5.087%


Sum of corrected areas: 8135819

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV073018\
Data File : VV006759.D
Acq On : 30 Jul 2018 13:30
Operator : SY/MD
Sample : J4190-07
Misc : 25 mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BE747

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072318WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

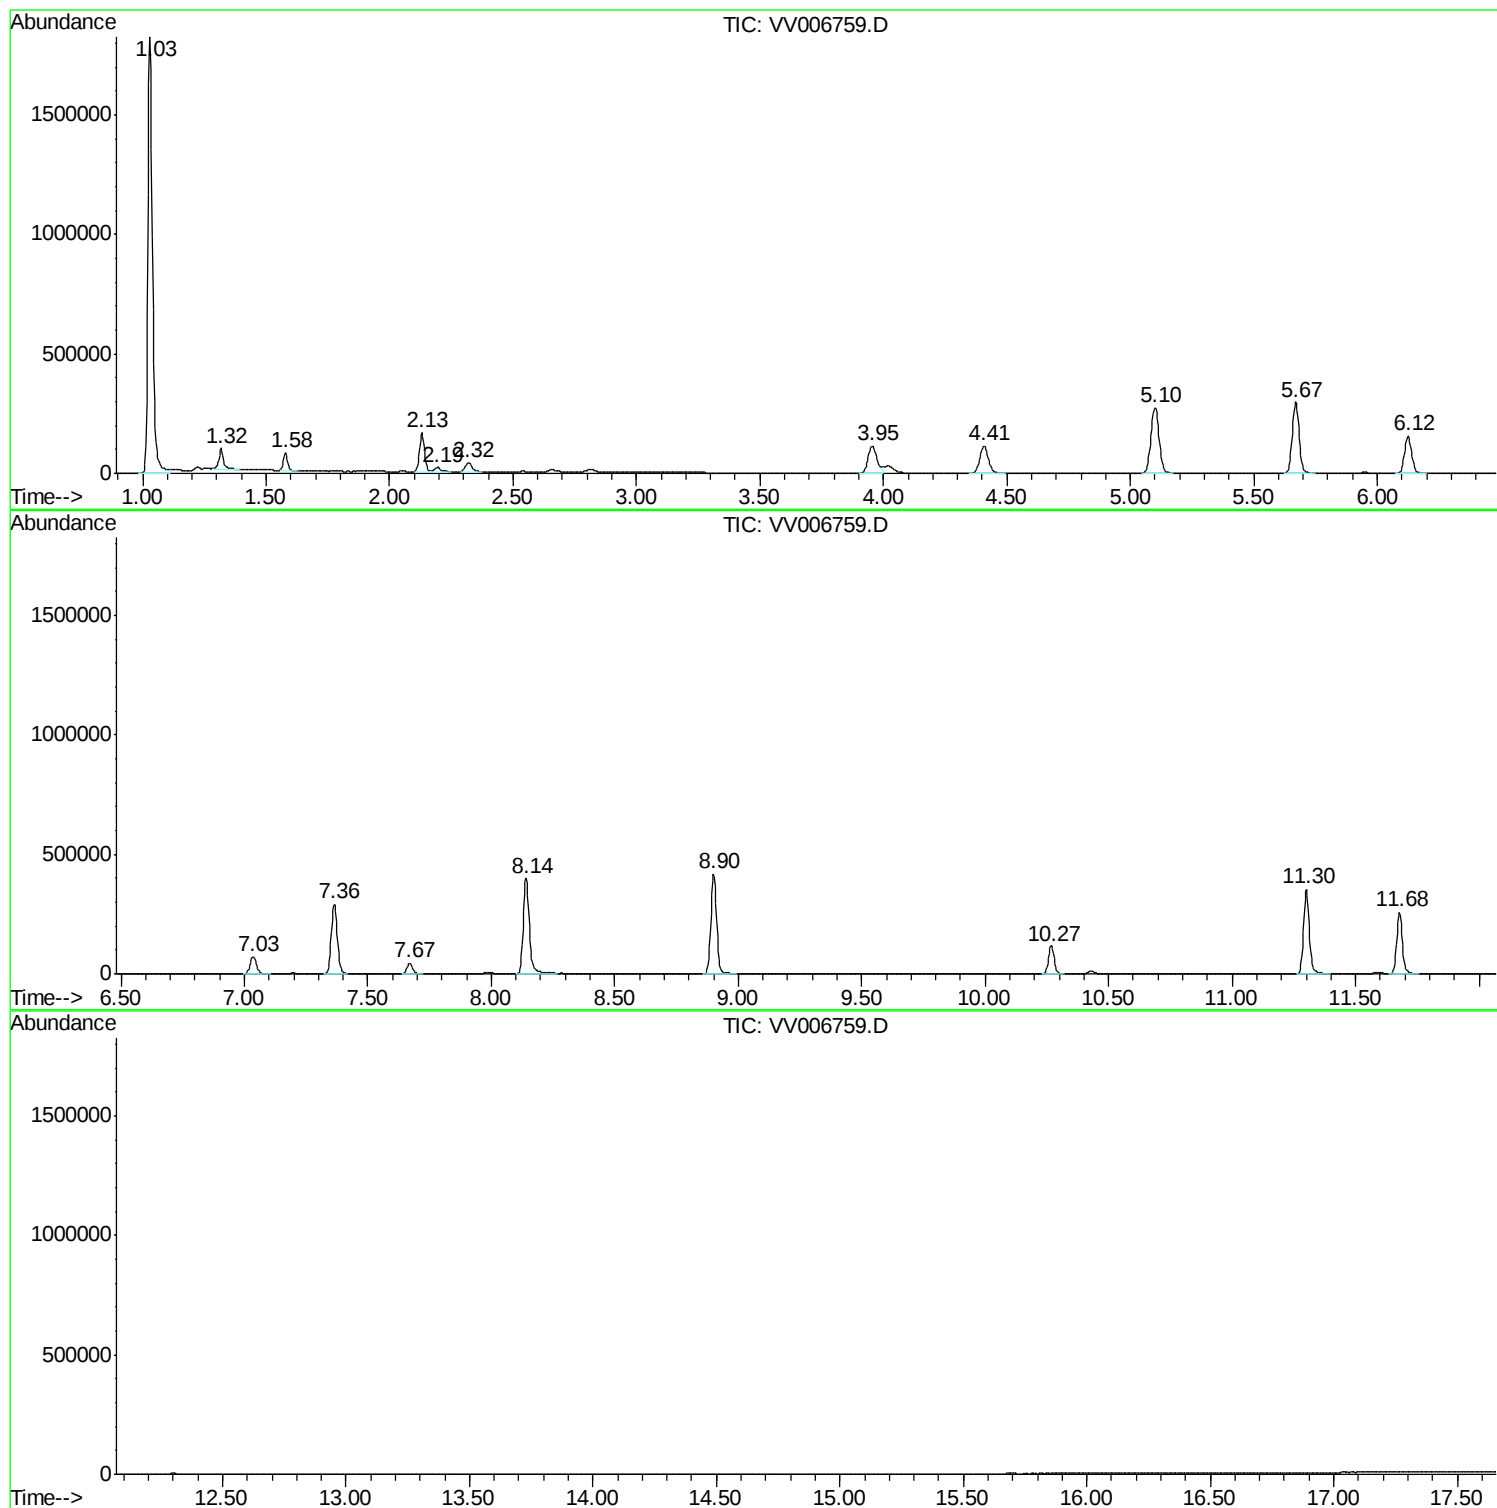

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV073018\
Data File : VV006759.D
Acq On : 30 Jul 2018 13:30
Operator : SY/MD
Sample : J4190-07
Misc : 25 mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BE747










Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072318WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Isopropyl Alcohol Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.32	0.60 ug/L	69276	1,4-Difluorobenzene	5.67

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Isopropyl Alcohol	60	C3H8O	000067-63-0	86
2			Isopropyl Alcohol	60	C3H8O	000067-63-0	78
3			Isopropyl Alcohol	60	C3H8O	000067-63-0	78
4			Propane, 2-ethoxy-	88	C5H12O	000625-54-7	56
5			Propane, 2-ethoxy-	88	C5H12O	000625-54-7	56

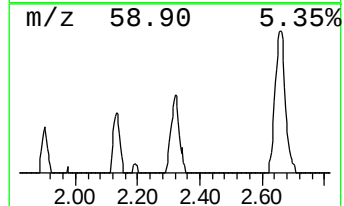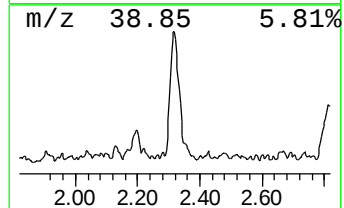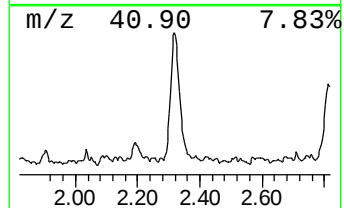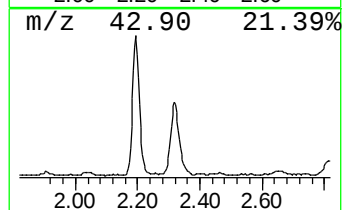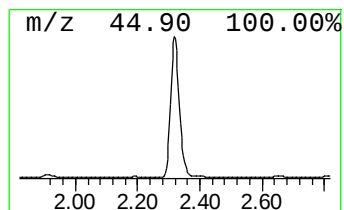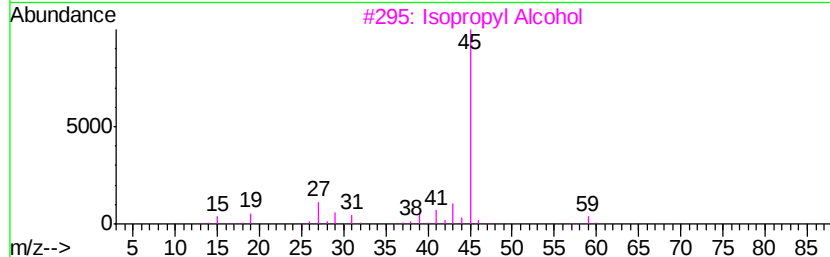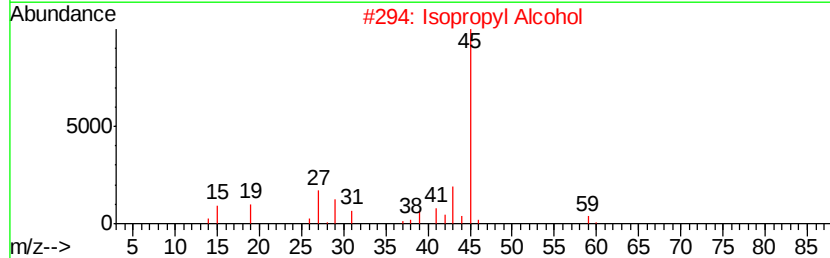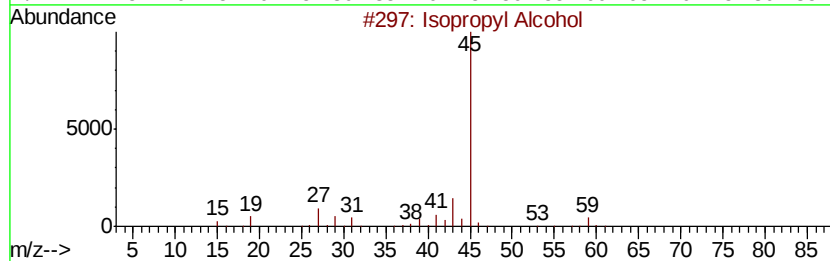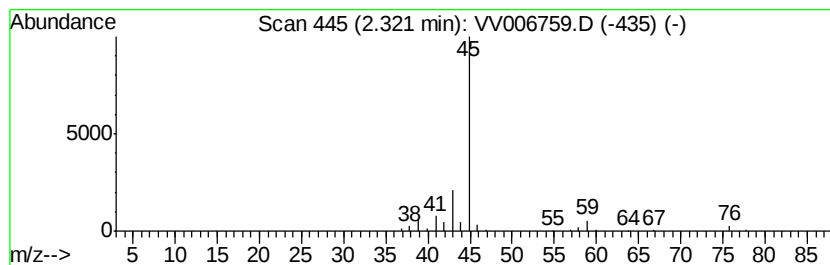

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV073018\
Data File : VV006759.D
Acq On : 30 Jul 2018 13:30
Operator : SY/MD
Sample : J4190-07
Misc : 25 mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BE747

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072318WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Isopropyl Alcohol	2.32	0.6	ug/L	69276	1	5.67	577367	5.0