


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV073019\
 Data File : VV012066.D
 Acq On : 30 Jul 2019 09:40
 Operator : SY/MD
 Sample : BFB42
 Misc : 25ML/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB42

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SFAMVTR072919WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Wed Jul 31 09:22:51 2019

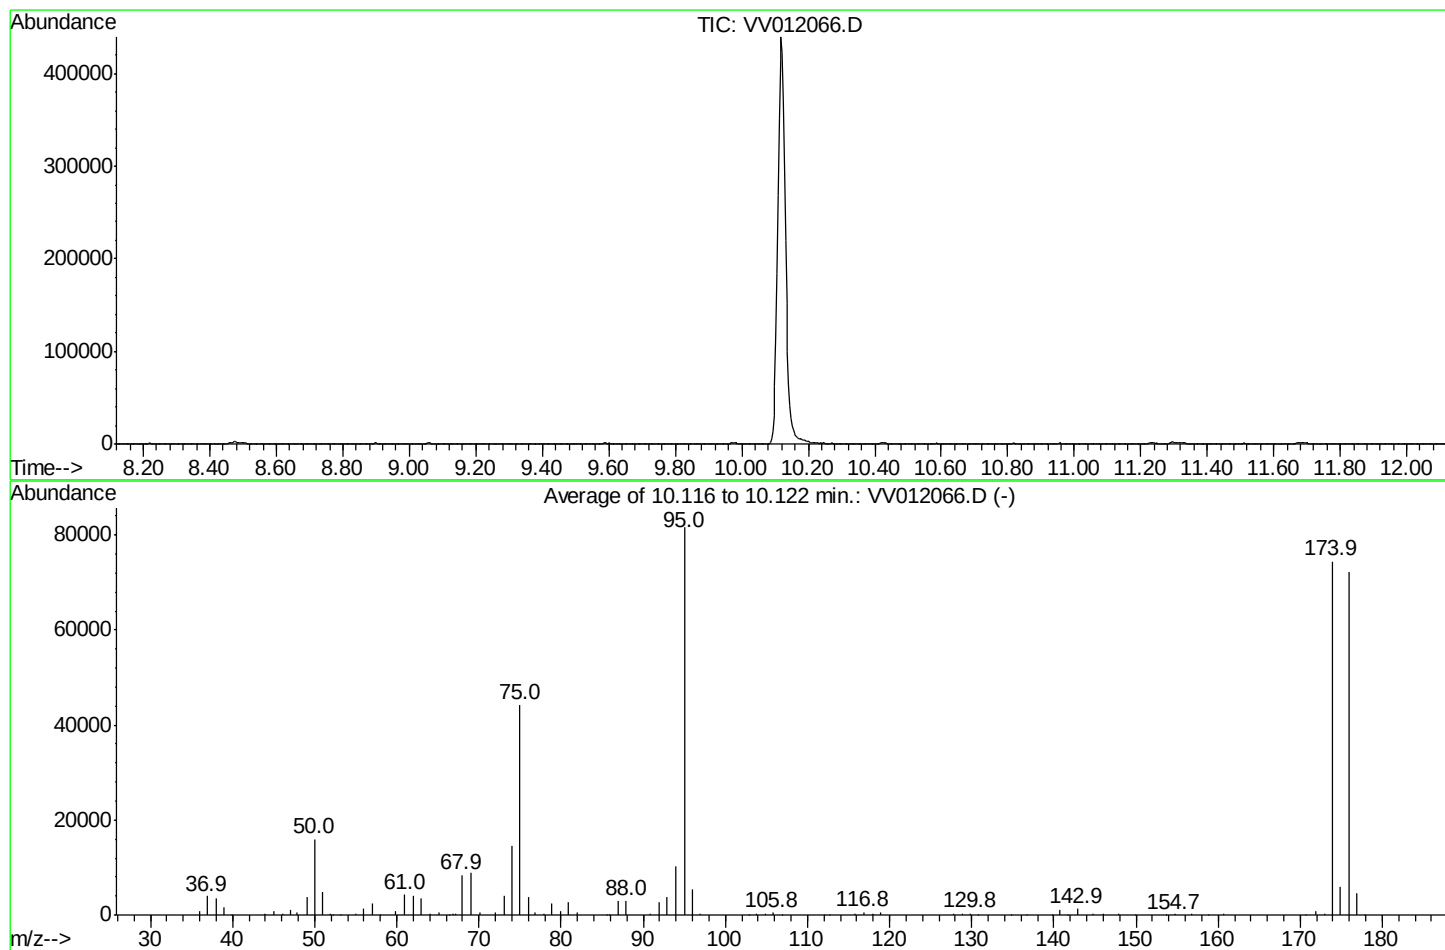

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2794

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.7	16047	PASS
75	95	30	80	54.2	44258	PASS
95	95	100	100	100.0	81640	PASS
96	95	5	9	6.5	5317	PASS
173	174	0.00	2	0.5	372	PASS
174	95	50	120	91.2	74434	PASS
175	174	5	9	7.8	5814	PASS
176	174	95	101	97.1	72306	PASS
177	176	5	9	6.2	4466	PASS

Scan 2794 (10.074 min): VV012066.D
BFB42

m/z	Abundance
39.80	127.0
41.10	102.0
44.00	211.0

Instrument :
MSVOA_V
ClientSampleId :
BFB42

m/z	Abundance
35.90	707.0
36.90	3997.0
38.00	3608.0
38.90	1620.0
39.80	277.0
43.90	595.0
45.00	783.0
46.10	210.0
47.00	1051.0
47.90	509.0
49.00	3637.0
50.00	15978.0
51.00	4811.0
51.90	230.0
53.00	113.0
55.00	270.0
55.90	1311.0
57.00	2289.0
57.90	129.0
59.90	735.0
60.90	4142.0
62.00	3905.0
63.00	3310.0
64.00	436.0
65.00	578.0
66.30	110.0
66.90	189.0
67.90	8301.0
69.00	8834.0
70.00	579.0
72.00	450.0
73.00	3959.0
74.00	14581.0
75.00	43640.0
76.00	3981.0
76.80	501.0
77.80	301.0
78.90	2374.0
80.00	747.0
80.80	2707.0
81.90	576.0
85.60	108.0
86.90	2716.0
87.90	3094.0
90.80	321.0
91.90	2594.0
92.90	3412.0
93.90	10333.0
95.00	79024.0
96.00	5369.0
96.90	183.0
102.80	114.0
103.90	321.0
104.80	154.0
105.80	479.0
106.90	118.0
115.80	389.0
116.80	559.0
117.90	332.0
118.80	452.0
127.80	426.0
128.90	204.0
129.90	377.0
130.80	110.0
134.90	138.0
136.70	162.0
139.80	112.0
140.80	970.0
142.80	1195.0
144.80	288.0
146.00	110.0
147.90	234.0
149.80	148.0
154.70	169.0
156.80	123.0
158.80	112.0
160.60	159.0
171.90	777.0
173.00	1116.0
173.90	71720.0
174.90	5661.0
175.90	68784.0
176.90	4230.0

Instrument :
MSVOA_V
ClientSampleId :
BFB42

m/z	Abundance
35.90	736.0
36.90	4148.0
37.90	3616.0
38.90	1782.0
39.80	229.0
43.90	640.0
45.00	752.0
46.00	220.0
47.00	1020.0
47.80	490.0
49.00	3919.0
50.00	16552.0
51.00	5033.0
51.80	229.0
53.10	139.0
55.00	281.0
55.90	1492.0
57.00	2431.0
58.00	119.0
59.90	712.0
60.90	4398.0
62.00	4154.0
63.00	3755.0
64.00	411.0
65.00	539.0
66.90	218.0
67.10	217.0
67.90	8633.0
69.00	9342.0
70.00	619.0
72.00	513.0
73.00	4243.0
74.00	15083.0
75.00	45880.0
76.00	4027.0
76.80	487.0
77.90	323.0
78.90	2507.0
80.00	826.0
80.80	2854.0
81.90	717.0
85.80	102.0
86.90	3066.0
88.00	3113.0
90.80	366.0
91.90	2710.0
92.90	3793.0
94.00	10606.0
95.00	84288.0
96.00	5480.0
96.90	174.0
102.80	112.0
103.80	334.0
104.80	177.0
105.80	449.0
106.90	124.0
112.70	103.0
115.90	397.0
116.80	553.0
117.90	380.0
118.90	481.0
127.80	414.0
128.90	206.0
129.90	420.0
130.80	129.0
134.80	134.0
136.70	145.0
139.80	129.0
140.80	1076.0
142.90	1269.0
144.80	252.0
146.00	187.0
147.90	245.0
149.90	139.0
153.70	116.0
154.70	179.0
156.70	140.0
158.80	130.0
160.60	159.0
171.90	893.0
173.90	76856.0
174.90	5968.0
175.90	74896.0
176.90	4598.0

Instrument :
MSVOA_V
ClientSampleId :
BFB42

m/z	Abundance
35.90	714.0
36.90	3729.0
37.90	3309.0
38.90	1576.0
39.90	148.0
43.90	632.0
44.90	677.0
46.00	201.0
47.00	841.0
47.90	428.0
49.00	3773.0
50.00	15613.0
51.00	4841.0
51.80	229.0
52.20	149.0
53.10	146.0
54.90	254.0
56.00	1407.0
56.90	2340.0
58.00	113.0
59.90	702.0
61.00	4122.0
62.00	4100.0
63.00	3651.0
64.00	385.0
65.10	420.0
66.30	103.0
66.90	215.0
67.10	218.0
67.90	8346.0
69.00	8760.0
70.10	597.0
72.00	484.0
73.00	3997.0
74.00	14291.0
75.00	43256.0
76.00	3637.0
76.80	408.0
77.90	316.0
78.90	2493.0
79.90	794.0
80.80	2682.0
81.90	704.0
86.90	3177.0
88.00	3035.0
90.90	422.0
92.00	2519.0
92.90	3867.0
94.00	9931.0
95.00	81608.0
96.00	5102.0
97.00	152.0
103.80	333.0
104.80	205.0
105.80	388.0
106.90	119.0
112.00	102.0
115.90	381.0
116.80	549.0
117.90	352.0
118.90	479.0
127.80	337.0
128.90	208.0
129.80	416.0
130.80	160.0
134.80	142.0
136.70	115.0
139.80	106.0
140.80	1051.0
141.70	106.0
143.00	1294.0
144.70	195.0
146.00	237.0
148.00	211.0
149.90	108.0
154.70	179.0
156.70	189.0
158.70	110.0
160.60	128.0
170.60	123.0
171.90	843.0
173.90	74728.0
174.90	5813.0
175.90	73240.0
176.90	4570.0
177.80	110.0

Instrument :
MSVOA_V
ClientSampleId :
BFB42