

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV073020\
 Data File : VV017754.D
 Acq On : 30 Jul 2020 17:33
 Operator : SY/MD
 Sample : L3419-20
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK02

Quant Time: Jul 31 02:39:29 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM073020WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jul 31 02:37:22 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	333768	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	308891	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	152312	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	73249	45.01	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	90.02%
7) Chloroethane-d5	1.58	69	62106	44.69	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	89.38%
11) 1,1-Dichloroethene-d2	2.12	63	128367	32.82	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	65.64%
21) 2-Butanone-d5	3.91	46	118763	97.04	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	97.04%
24) Chloroform-d	4.37	84	200730	45.13	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	90.26%
26) 1,2-Dichloroethane-d4	5.05	65	155025	47.71	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.42%
32) Benzene-d6	5.07	84	359621	49.21	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	98.42%
36) 1,2-Dichloropropane-d6	6.09	67	102559	50.81	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	101.62%
41) Toluene-d8	7.34	98	347276	48.46	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	96.92%
43) trans-1,3-Dichloropropene-	7.64	79	59690	44.75	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	89.50%
47) 2-Hexanone-d5	8.11	63	83235	95.95	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	95.95%
57) 1,1,2,2-Tetrachloroethane-	10.24	84	138304	45.38	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	90.76%
64) 1,2-Dichlorobenzene-d4	11.65	152	150566	50.36	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	100.72%


Target Compounds					Ovalue
39) cis-1,3-Dichloropropene	7.01	75	4351	1.234 ug/L	83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV073020\
Data File : VV017754.D
Acq On : 30 Jul 2020 17:33
Operator : SY/MD
Sample : L3419-20
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK02

Quant Time: Jul 31 02:39:29 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM073020WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jul 31 02:37:22 2020
Response via : Initial Calibration

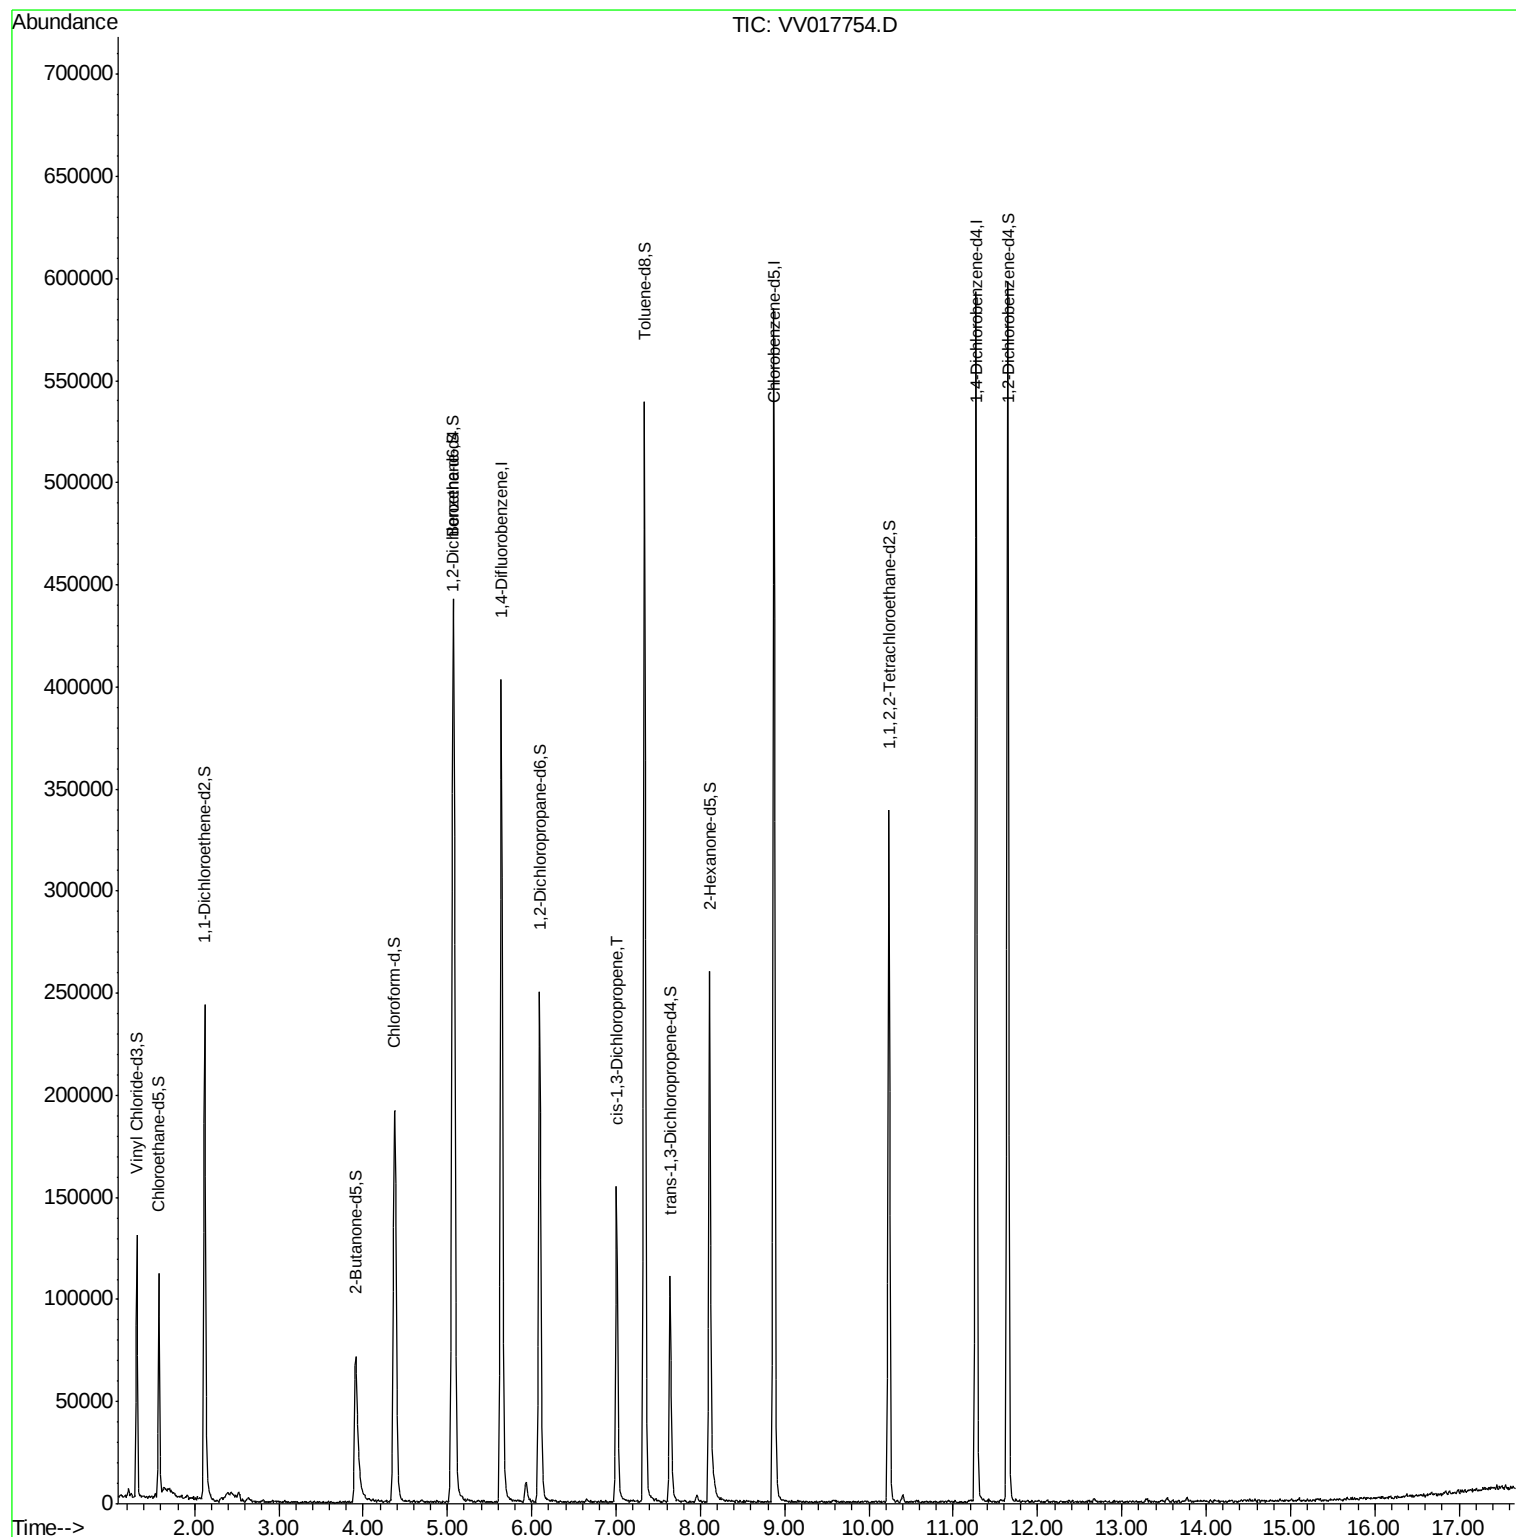

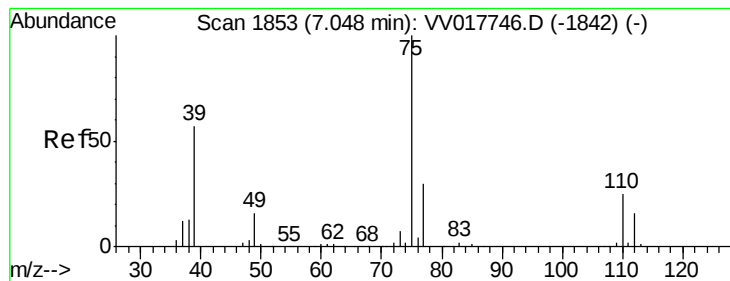

#39
 cis-1,3-Dichloropropene
 Concen: 1.234 ug/L
 RT: 7.01 min Scan# 1841
 Delta R.T. -0.04 min
 Lab File: VV017754.D
 Acq: 30 Jul 2020 17:33

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK02

Tot Ion: 75 Resp: 4351
 Ion Ratio Lower Upper
 75 100
 77 42.9 23.2 43.0

