
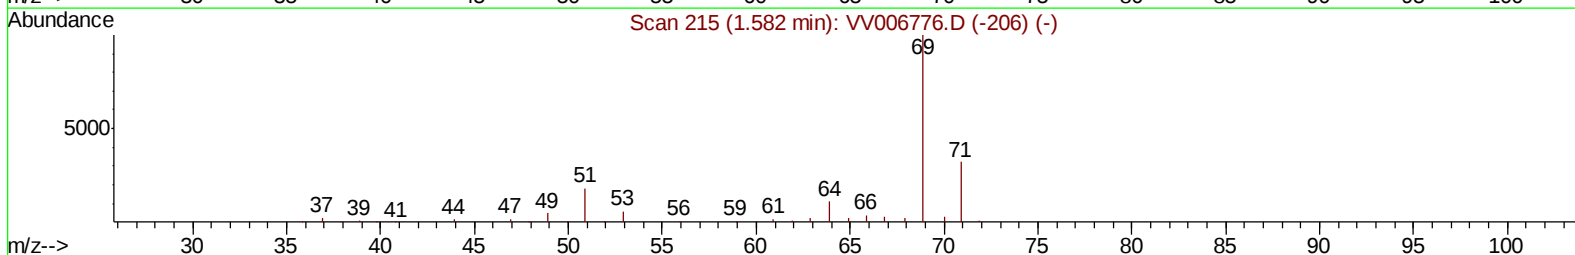
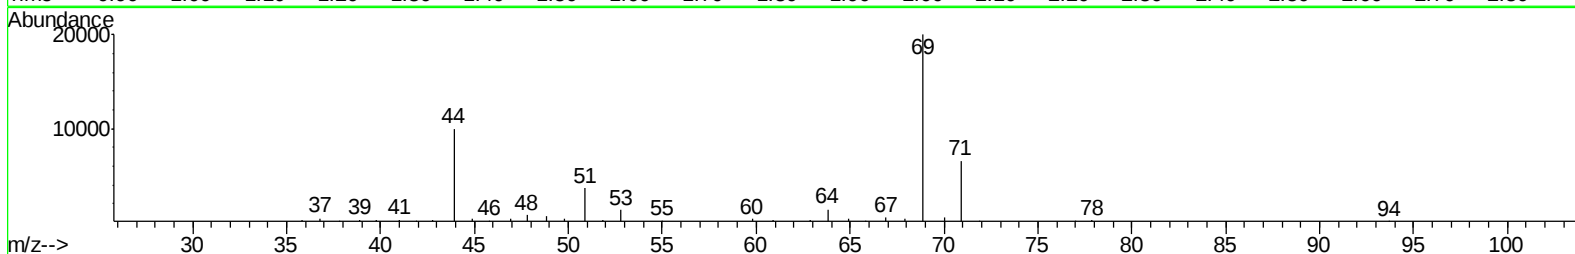


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV073118\
Data File : VV006783.D
Acq On : 31 Jul 2018 14:04
Operator : SY/MD
Sample : J4225-11
Misc : 25 mL/MSVOA V/WATER
ALS Vial : 10 Sample Multiplier: 1

Quant Time: Aug 01 02:16:51 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072318WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Aug 01 01:43:21 2018
Response via : Initial Calibration

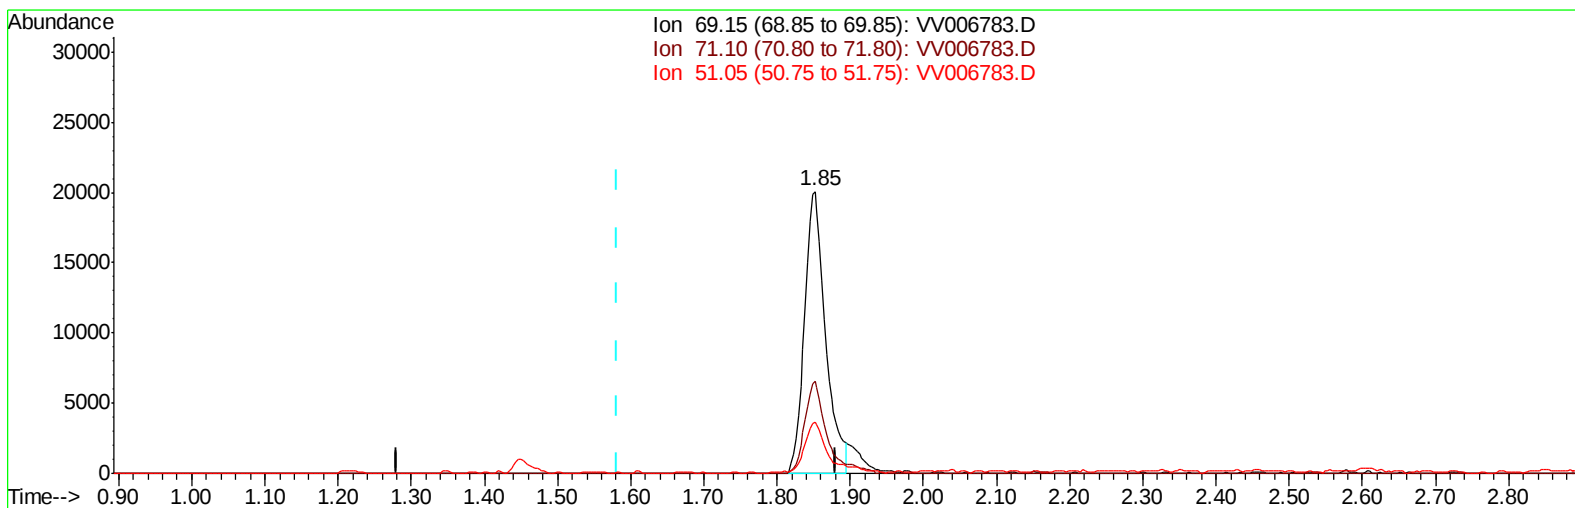

TIC: VV006783.D

(7) Chloroethane-d5 (S)

1.852min (+0.270) 25.73ug/L m

response 39871

Ion	Exp%	Act%
69.15	100	100
71.10	32.50	27.39
51.05	27.00	16.06#
0.00	0.00	0.00