
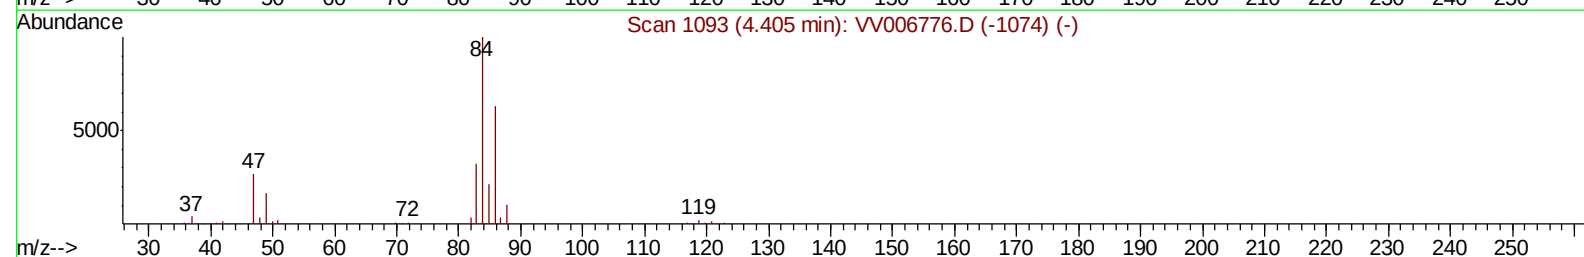
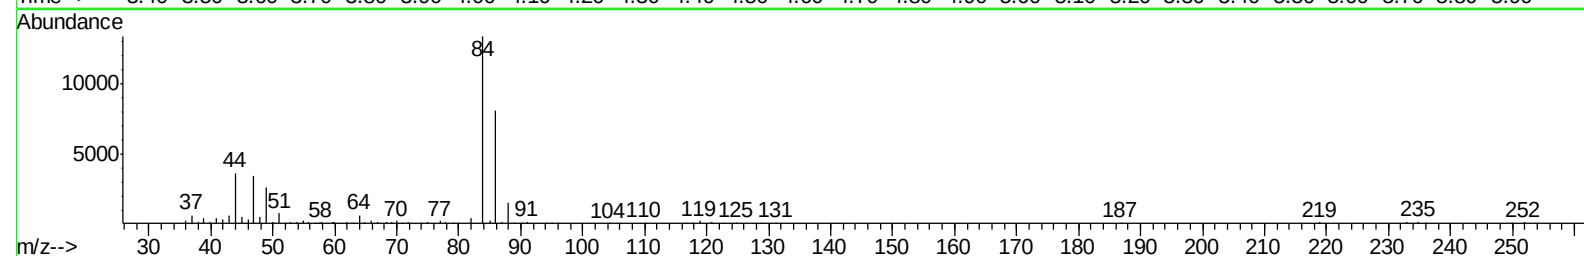


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV073118\
 Data File : VV006783.D
 Acq On : 31 Jul 2018 14:04
 Operator : SY/MD
 Sample : J4225-11
 Misc : 25 mL/MSVOA V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Quant Time: Aug 01 02:16:51 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072318WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Aug 01 01:43:21 2018
 Response via : Initial Calibration

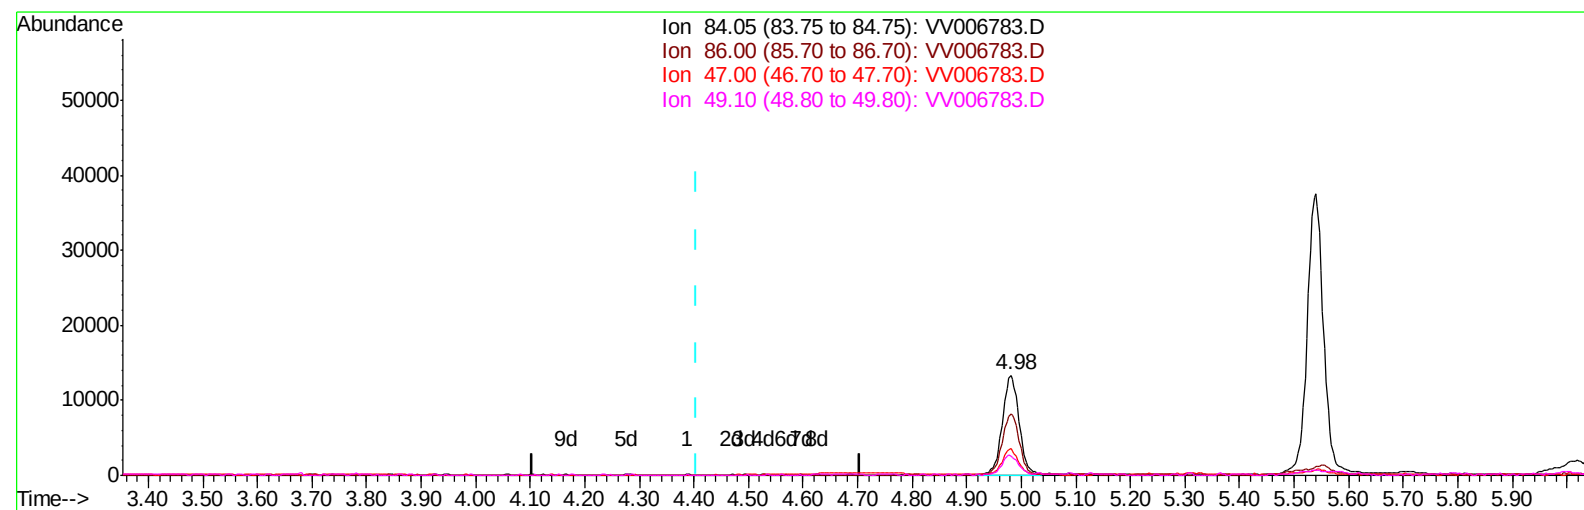

TIC: VV006783.D

(24) Chloroform-d (S)

4.980min (+0.575) 7.68ug/L m

response 28425

Ion	Exp%	Act%
84.05	100	100
86.00	62.50	0.00#
47.00	44.20	0.07#
49.10	24.70	0.07#