

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV073118\
 Data File : VV006778.D
 Acq On : 31 Jul 2018 11:24
 Operator : SY/MD
 Sample : J4225-05
 Misc : 25 mL/MSVOA V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ESWP2

Quant Time: Aug 01 01:57:14 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072318WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Aug 01 01:43:21 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	172799	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	160779	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	63587	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	48218	5.36	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	107.20%
7) Chloroethane-d5	1.58	69	42012	5.95	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	119.00%
11) 1,1-Dichloroethene-d2	2.13	63	67242	3.81	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	76.20%
20) 2-Butanone-d5	3.94	46	138310	49.22	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	98.44%
24) Chloroform-d	4.40	84	94532	5.60	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	112.00%
26) 1,2-Dichloroethane-d4	5.09	65	48511	5.90	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	118.00%
32) Benzene-d6	5.10	84	188755	5.71	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	114.20%
36) 1,2-Dichloropropane-d6	6.12	67	62622	5.61	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	112.20%
41) Toluene-d8	7.36	98	151206	5.23	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	104.60%
43) trans-1,3-Dichloropropene-	7.67	79	17218	4.72	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	94.40%
46) 2-Hexanone-d5	8.14	63	95405	41.36	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	82.72%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	45636	5.01	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	100.20%
64) 1,2-Dichlorobenzene-d4	11.68	152	55810	5.89	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	117.80%


Target Compounds					Ovalue
13) Acetone	2.19	43	6255	3.50 ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV073118\
Data File : VV006778.D
Acq On : 31 Jul 2018 11:24
Operator : SY/MD
Sample : J4225-05
Misc : 25 mL/MSVOA V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ESWP2

Quant Time: Aug 01 01:57:14 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072318WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Aug 01 01:43:21 2018
Response via : Initial Calibration

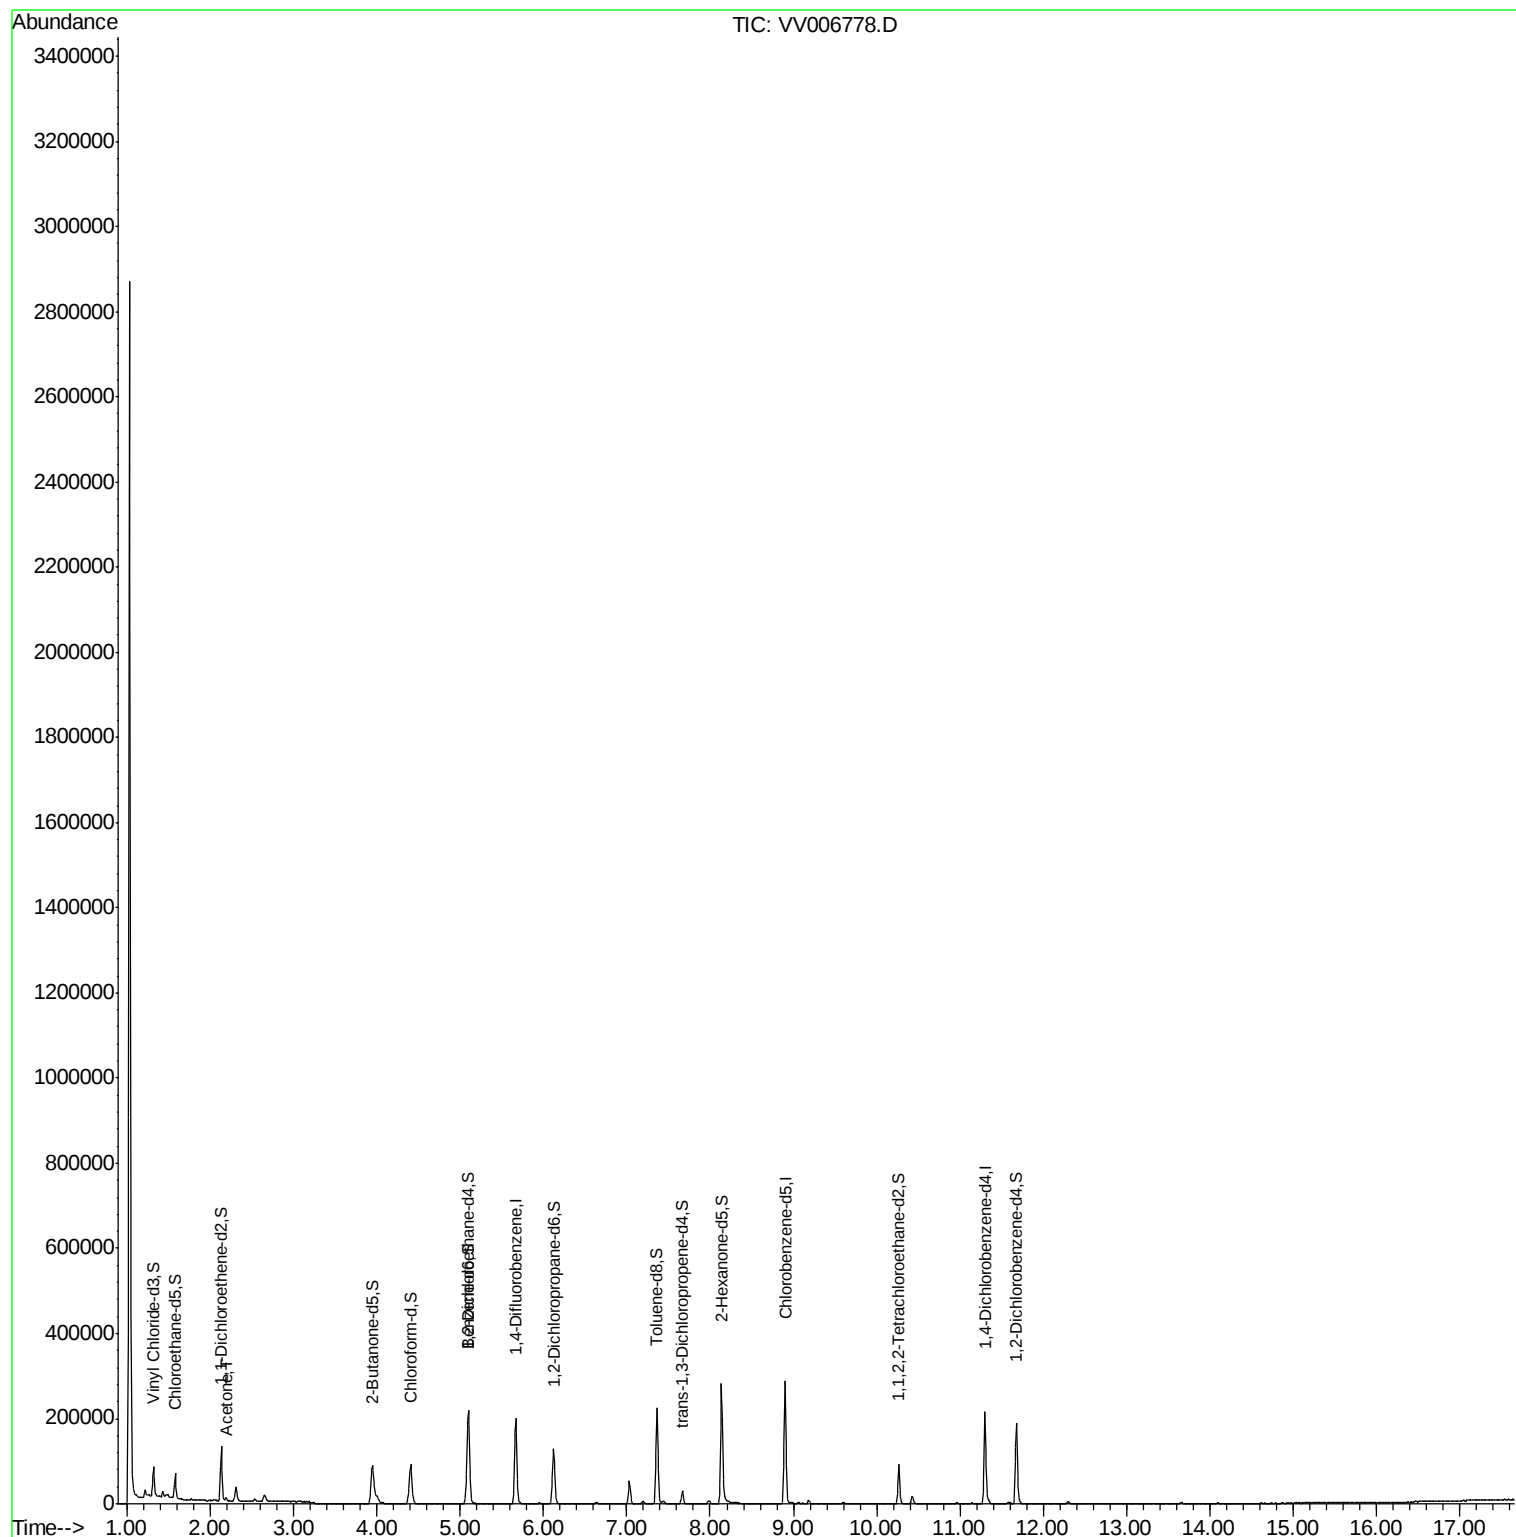

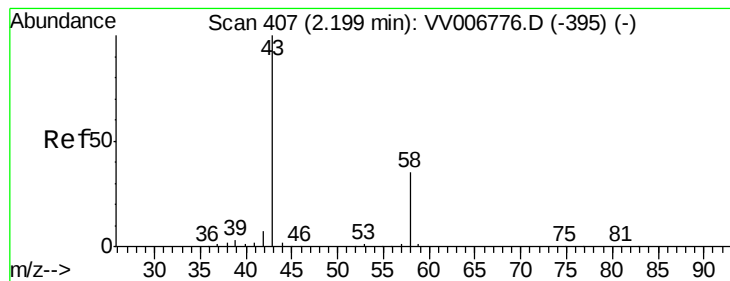

#13
 Acetone
 Concen: 3.50 ug/L
 RT: 2.19 min Scan# 404
 Delta R.T. -0.01 min
 Lab File: VV006778.D
 Acq: 31 Jul 2018 11:24

Instrument :
 MSVOA_V
 ClientSampleId :
 ESWP2

Tot Ion: 43 Resp: 6255
 Ion Ratio Lower Upper
 43 100
 58 35.5 0.0 71.4

