

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV073118\
 Data File : VV006782.D
 Acq On : 31 Jul 2018 13:11
 Operator : SY/MD
 Sample : J4225-09
 Misc : 25 mL/MSVOA V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ESWQ7

Quant Time: Aug 01 02:06:07 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072318WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Aug 01 01:43:21 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	176175	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	162987	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	63211	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	43434	4.74	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	94.80%
7) Chloroethane-d5	1.58	69	39784	5.53	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	110.60%
11) 1,1-Dichloroethene-d2	2.13	63	63773	3.55	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	71.00%
20) 2-Butanone-d5	3.95	46	147300	51.42	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	102.84%
24) Chloroform-d	4.41	84	93425	5.43	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	108.60%
26) 1,2-Dichloroethane-d4	5.09	65	48129	5.74	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	114.80%
32) Benzene-d6	5.10	84	182007	5.43	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	108.60%
36) 1,2-Dichloropropane-d6	6.12	67	61669	5.45	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	109.00%
41) Toluene-d8	7.36	98	145018	4.95	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.00%
43) trans-1,3-Dichloropropene-	7.67	79	18109	4.90	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	98.00%
46) 2-Hexanone-d5	8.14	63	100484	42.97	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	85.94%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	47829	5.18	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	103.60%
64) 1,2-Dichlorobenzene-d4	11.68	152	53667	5.70	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	114.00%


Target Compounds					Ovalue
13) Acetone	2.19	43	8247	4.52 ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV073118\
Data File : VV006782.D
Acq On : 31 Jul 2018 13:11
Operator : SY/MD
Sample : J4225-09
Misc : 25 mL/MSVOA V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ESWQ7

Quant Time: Aug 01 02:06:07 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072318WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Aug 01 01:43:21 2018
Response via : Initial Calibration

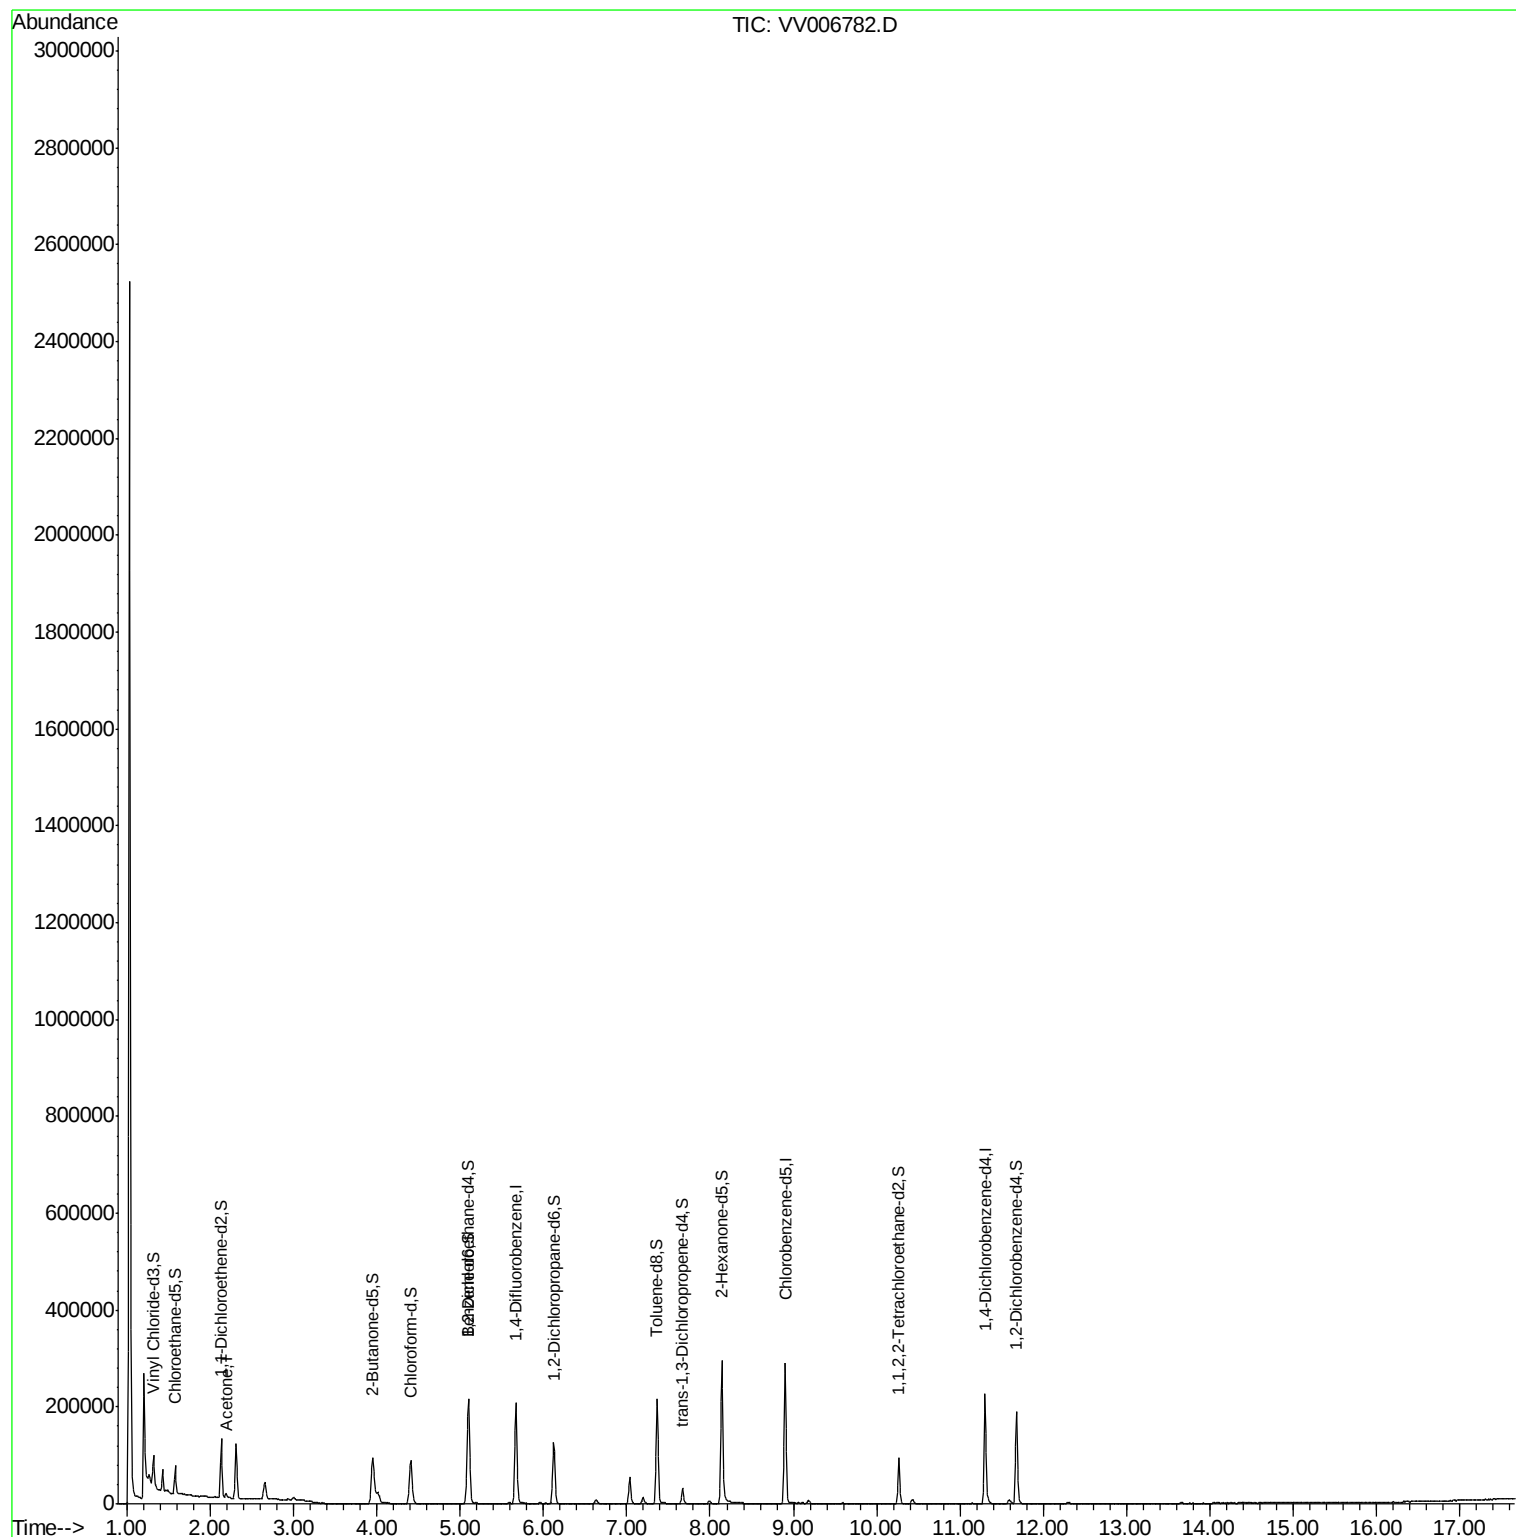

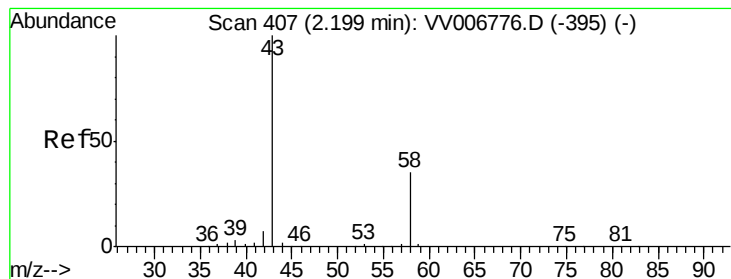

#13

Acetone

Concen: 4.52 ug/L

RT: 2.19 min Scan# 404

Delta R.T. -0.01 min

Lab File: VV006782.D

Acq: 31 Jul 2018 13:11

Instrument :
MSVOA_V
ClientSampleId :
ESWQ7

Tot Ion: 43 Resp: 8247

Ion Ratio Lower Upper

43 100

58 37.5 0.0 71.4

