


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV073119\
Data File : VV012073.D
Acq On : 30 Jul 2019 16:19
Operator : SY/MD
Sample : BFB42
Misc : 25ML/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB42

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR073119WMA.M
Title : TRACE VOA SOM01.0
Last Update : Thu Aug 01 17:59:13 2019

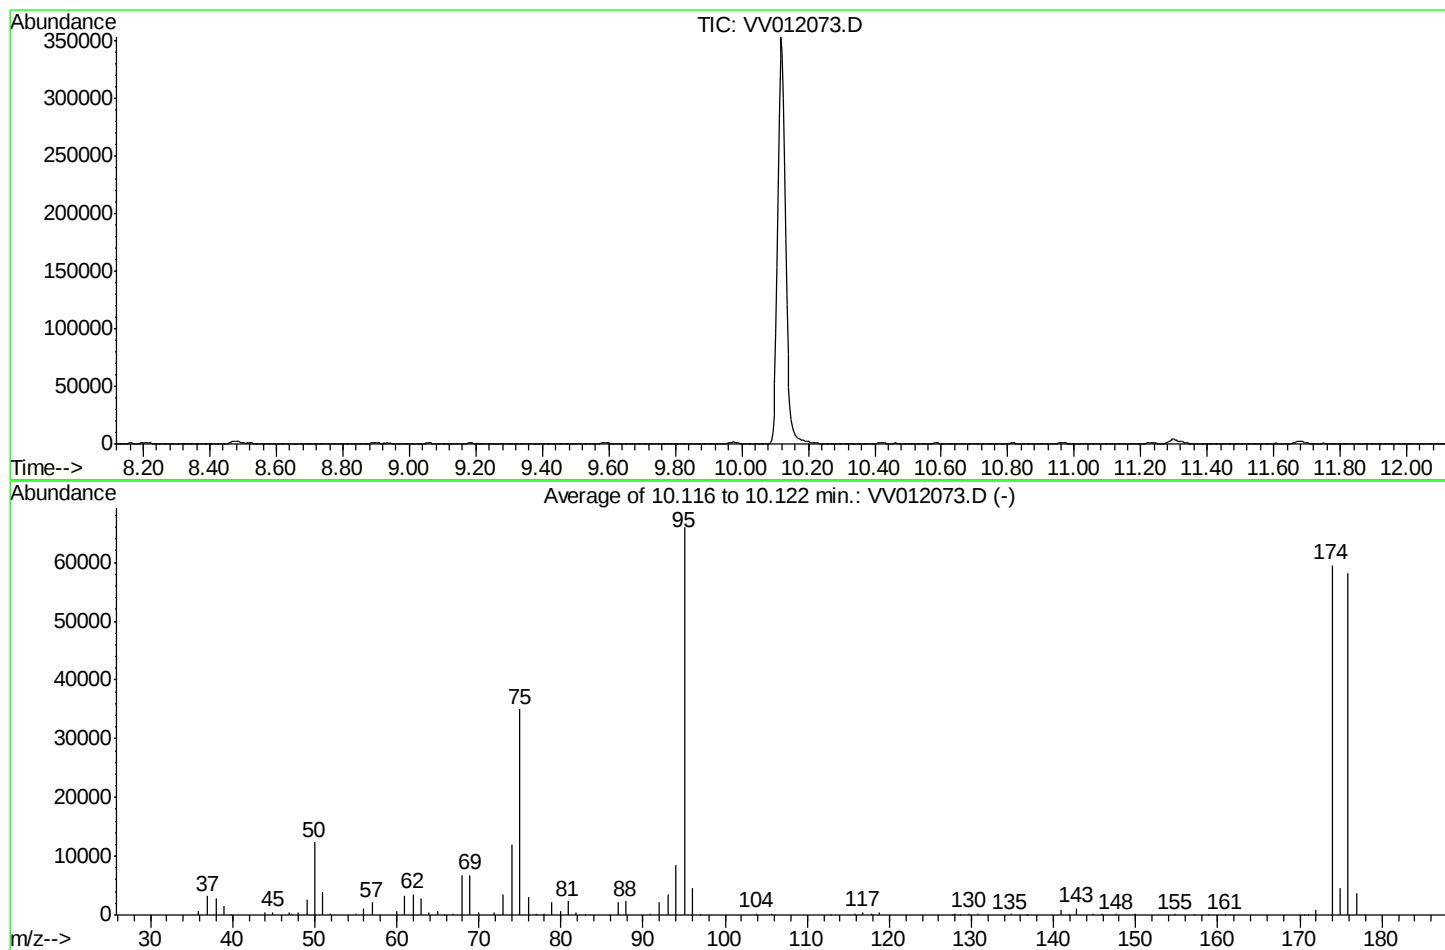

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2794

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.8	12407	PASS
75	95	30	80	53.1	35008	PASS
95	95	100	100	100.0	65989	PASS
96	95	5	9	7.0	4630	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	90.3	59562	PASS
175	174	5	9	7.6	4547	PASS
176	174	95	101	97.9	58290	PASS
177	176	5	9	6.5	3805	PASS

m/z	Abundance
39.70	157.0
43.90	219.0

Instrument :
MSVOA_V
ClientSampleId :
BFB42

m/z	Abundance
35.90	571.0
37.00	3076.0
38.00	2679.0
39.00	1418.0
39.90	285.0
43.90	714.0
44.90	596.0
46.90	517.0
48.00	452.0
49.00	2613.0
50.00	12235.0
51.00	3940.0
52.00	181.0
54.90	248.0
56.00	1045.0
57.00	2122.0
59.90	522.0
61.00	3319.0
62.00	3626.0
63.00	2743.0
64.00	354.0
65.00	581.0
66.80	280.0
67.90	6473.0
68.90	6569.0
70.00	498.0
71.90	372.0
73.00	3271.0
74.00	11531.0
75.00	34688.0
76.00	2927.0
77.00	280.0
78.00	280.0
78.90	2059.0
79.90	595.0
80.90	2205.0
81.90	421.0
87.00	2226.0
87.90	2283.0
90.80	208.0
92.00	2037.0
93.00	3348.0
94.00	8542.0
95.00	65176.0
96.00	4658.0
97.00	194.0
103.80	284.0
105.70	368.0
115.80	249.0
116.80	459.0
117.80	278.0
118.90	462.0
127.70	207.0
128.00	209.0
128.60	123.0
129.90	169.0
130.80	139.0
134.80	135.0
136.70	130.0
140.80	861.0
141.90	152.0
142.80	1142.0
144.80	265.0
145.80	121.0
147.70	237.0
149.90	184.0
154.80	189.0
157.10	105.0
160.90	124.0
170.50	128.0
171.90	762.0
173.90	57128.0
174.90	4483.0
175.90	56672.0
176.90	3711.0

Instrument :
MSVOA_V
ClientSampleId :
BFB42

m/z	Abundance
35.90	592.0
37.00	3355.0
38.00	2852.0
39.00	1524.0
39.80	266.0
43.90	768.0
44.90	562.0
46.80	520.0
47.20	495.0
47.90	515.0
49.00	2702.0
50.00	12760.0
51.00	4137.0
52.00	149.0
55.00	228.0
56.00	1061.0
57.00	2228.0
60.00	625.0
61.00	3473.0
62.00	3631.0
63.00	2878.0
63.90	376.0
65.00	610.0
65.80	135.0
66.80	334.0
67.90	7058.0
69.00	7028.0
70.00	566.0
71.90	455.0
73.00	3595.0
74.00	12253.0
75.00	36048.0
76.00	3069.0
77.00	283.0
77.90	316.0
78.90	2210.0
79.90	664.0
80.80	2383.0
81.80	494.0
85.90	105.0
87.00	2187.0
87.90	2410.0
90.90	233.0
92.00	2286.0
93.00	3553.0
94.00	8843.0
95.00	67944.0
96.00	4760.0
96.90	137.0
103.80	324.0
105.70	329.0
115.70	247.0
116.80	572.0
117.80	328.0
118.90	492.0
128.00	249.0
128.60	115.0
129.70	264.0
130.90	170.0
134.80	149.0
136.70	122.0
140.90	856.0
141.90	120.0
142.90	1131.0
144.80	278.0
145.90	161.0
147.70	205.0
149.90	176.0
154.80	218.0
158.80	144.0
160.90	110.0
170.50	111.0
171.10	102.0
171.90	842.0
173.90	61328.0
174.90	4629.0
175.90	60104.0
176.90	3929.0
177.80	103.0

Instrument :
MSVOA_V
ClientSampleId :
BFB42

m/z	Abundance
35.90	534.0
36.90	3304.0
38.00	2783.0
38.90	1438.0
39.90	237.0
43.90	738.0
44.90	483.0
46.80	522.0
47.90	507.0
49.00	2667.0
50.00	12226.0
51.00	3871.0
51.90	127.0
55.00	210.0
56.00	992.0
57.00	2002.0
60.00	676.0
61.00	3348.0
62.00	3234.0
63.00	2718.0
63.90	358.0
65.00	548.0
65.80	120.0
66.80	289.0
68.00	7033.0
69.00	7016.0
70.00	591.0
71.90	442.0
73.00	3319.0
74.00	11887.0
75.00	34288.0
76.00	2863.0
76.90	299.0
77.90	292.0
78.90	2111.0
79.90	644.0
80.80	2313.0
81.80	526.0
82.90	112.0
86.00	122.0
86.90	1966.0
87.90	2341.0
90.90	233.0
91.90	2245.0
93.00	3415.0
94.00	8356.0
95.00	64848.0
96.00	4473.0
103.90	314.0
106.00	291.0
112.90	123.0
115.70	224.0
116.80	588.0
117.80	355.0
118.80	427.0
127.90	267.0
129.70	325.0
130.90	164.0
134.80	150.0
136.90	123.0
140.90	792.0
142.90	1024.0
144.80	293.0
145.90	187.0
147.60	182.0
149.90	144.0
154.80	217.0
158.80	165.0
171.00	144.0
171.90	797.0
173.90	60232.0
174.90	4531.0
175.90	58096.0
176.90	3777.0
177.90	110.0

Instrument :
MSVOA_V
ClientSampleId :
BFB42