

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV073120\
 Data File : VV017773.D
 Acq On : 31 Jul 2020 14:22
 Operator : SY/MD
 Sample : L3520-10
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 D0AC3

Manual Integrations
 APPROVED

MMDadoda
 8/4/2020 9:45:03 AM

Quant Time: Aug 01 05:59:49 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072320WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Aug 01 04:42:38 2020
 Response via : Initial Calibration

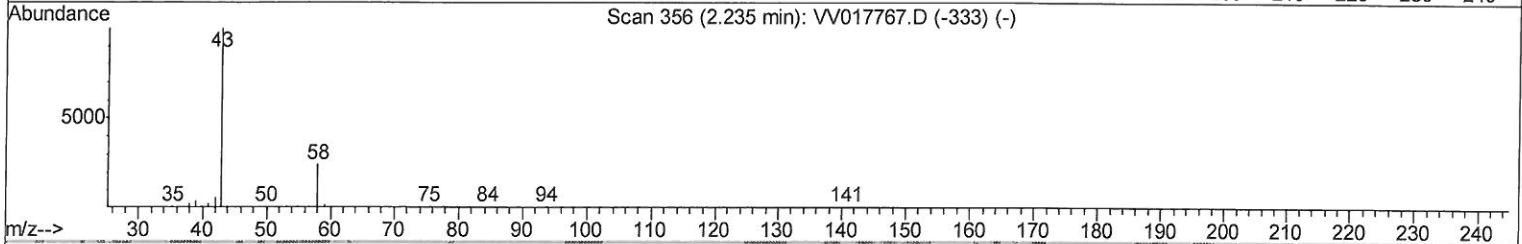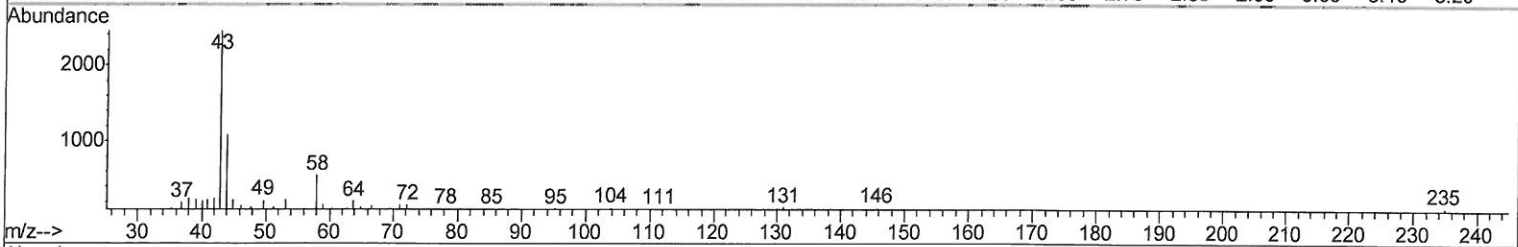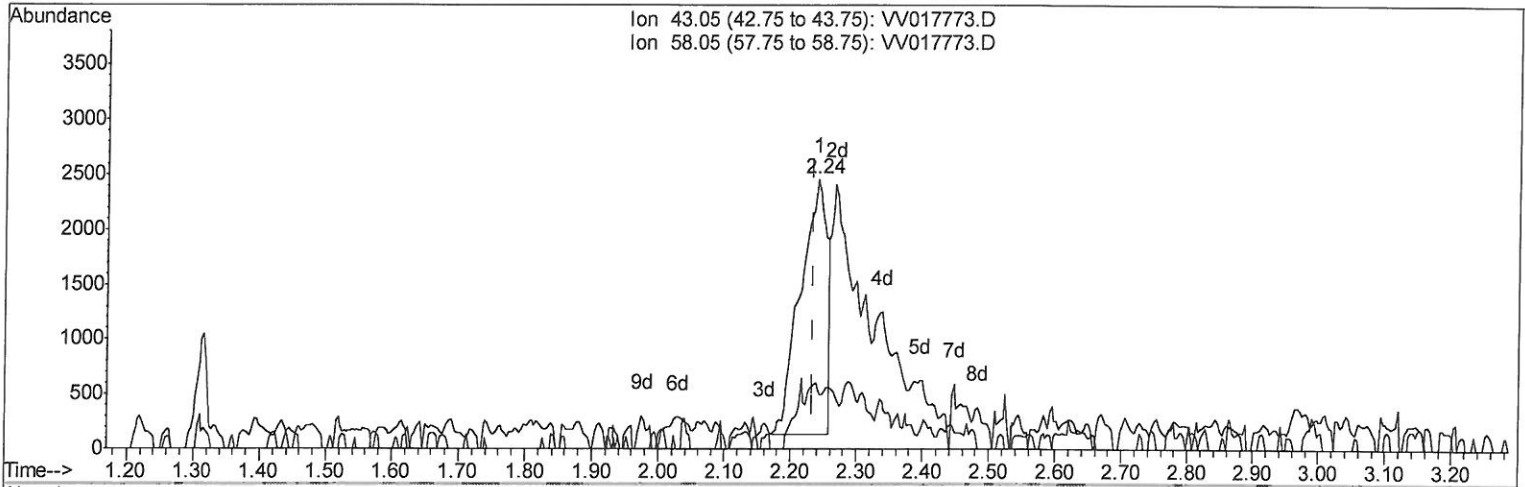

TIC: VV017773.D

(13) Acetone (T)

2.241min (+0.006) 4.84ug/L

response 6441

Ion	Exp%	Act%
43.05	100	100
58.05	9.30	11.58
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV073120\
Data File : VV017773.D
Acq On : 31 Jul 2020 14:22
Operator : SY/MD
Sample : L3520-10
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
D0AC3

Manual Integrations
APPROVED

MMDadoda
8/4/2020 9:45:03 AM

Quant Time: Aug 01 05:59:49 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072320WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Aug 01 04:42:38 2020
Response via : Initial Calibration

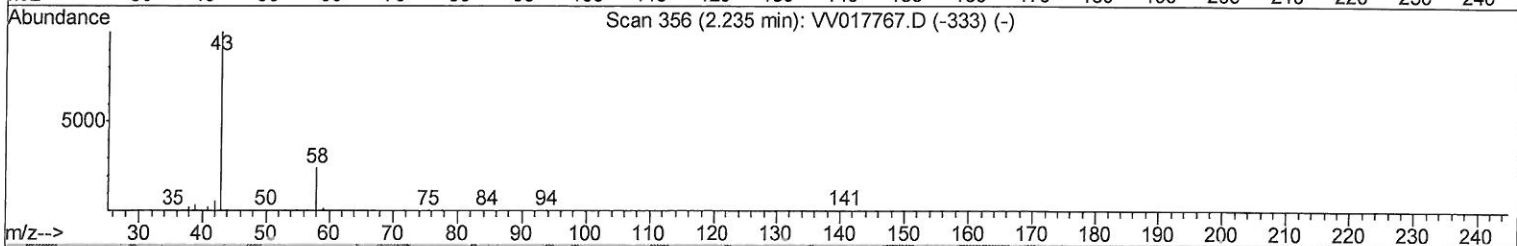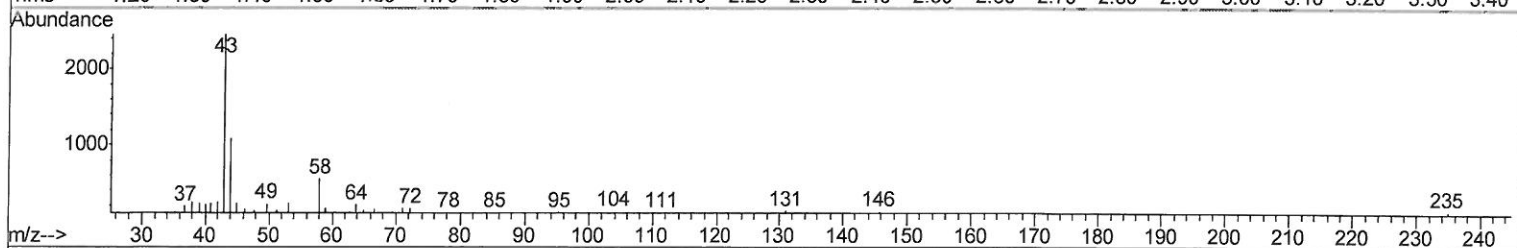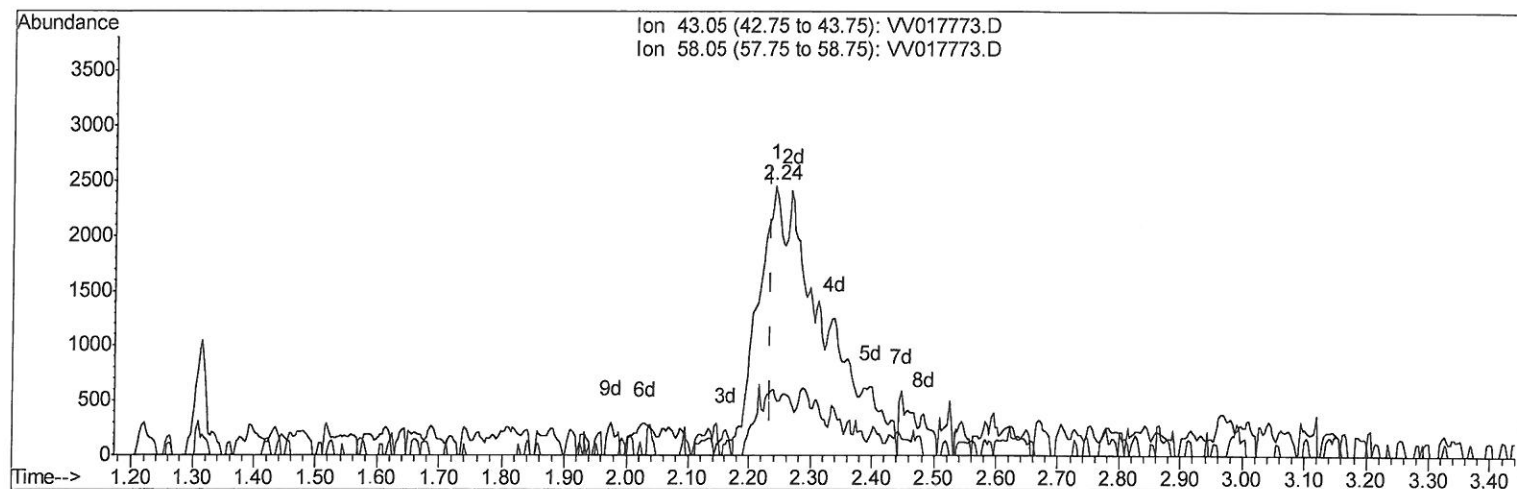

TIC: VV017773.D

(13) Acetone (T)

2.241min (+0.006) 13.61ug/L m

208/10/1254

response 18106

Ion	Exp%	Act%
43.05	100	100
58.05	9.30	4.12
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV073120\
 Data File : VV017773.D
 Acq On : 31 Jul 2020 14:22
 Operator : SY/MD
 Sample : L3520-10
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
ClientSampleId :
 D0AC3

Manual Integrations
APPROVED

MMDadoda
 8/4/2020 9:45:03 AM

Quant Time: Aug 01 05:59:49 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072320WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Aug 01 04:42:38 2020
 Response via : Initial Calibration

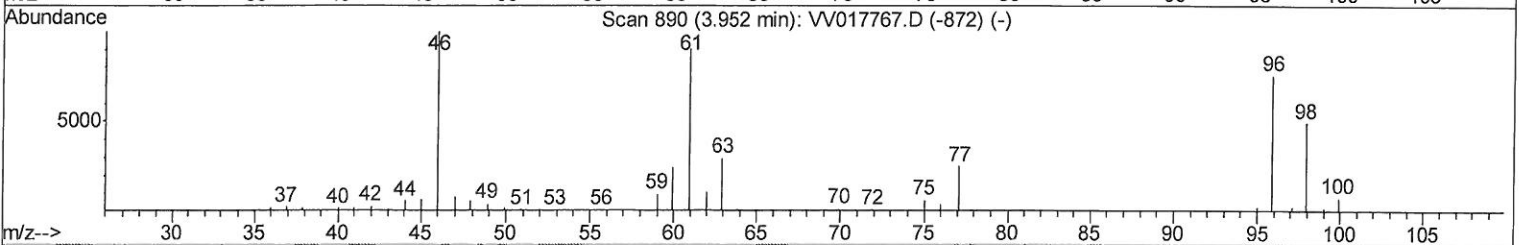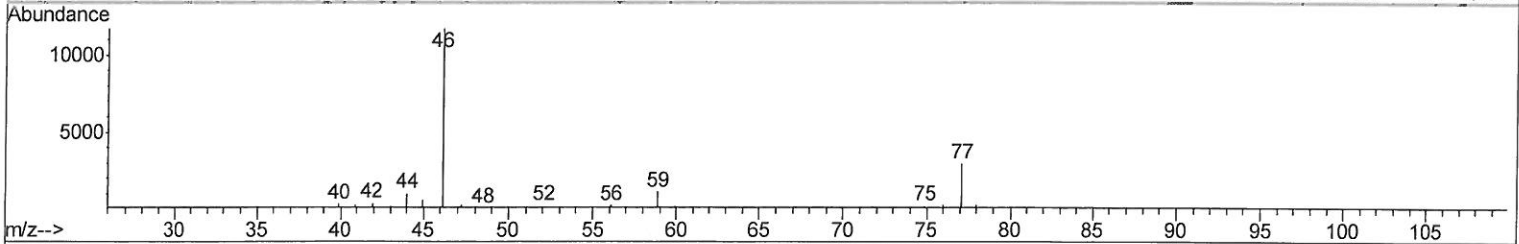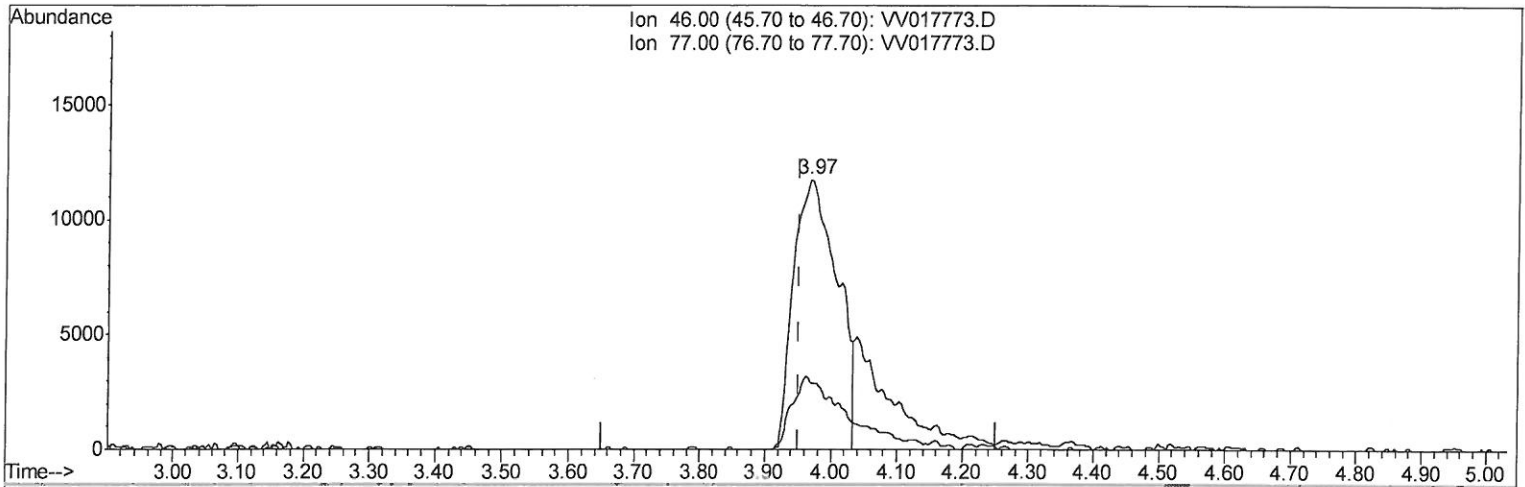

TIC: VV017773.D

(20) 2-Butanone-d5 (S)
 3.968min (+0.016) 31.56ug/L
 response 53656

Ion	Exp%	Act%
46.00	100	100
77.00	11.20	18.55#
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV073120\
 Data File : VV017773.D
 Acq On : 31 Jul 2020 14:22
 Operator : SY/MD
 Sample : L3520-10
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampled :
 D0AC3

Manual Integrations
 APPROVED

MMDadoda
 8/4/2020 9:45:03 AM

Quant Time: Aug 01 05:59:49 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072320WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Aug 01 04:42:38 2020
 Response via : Initial Calibration

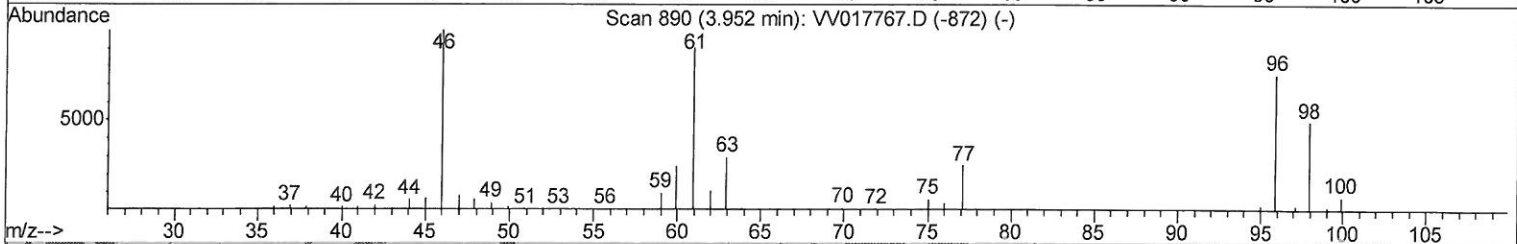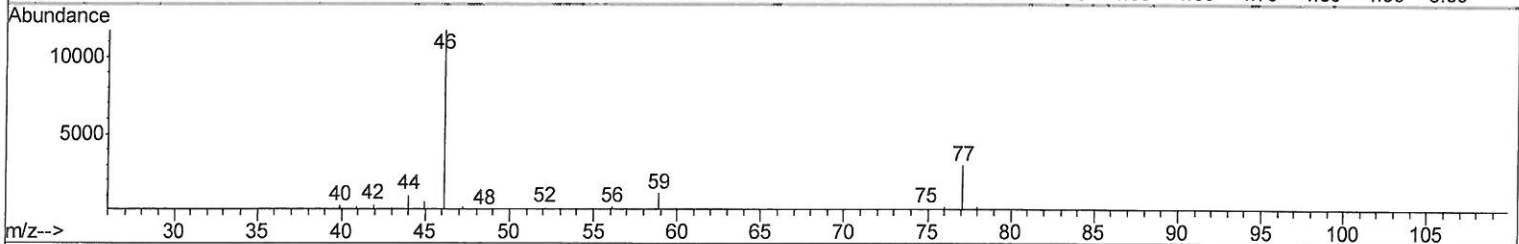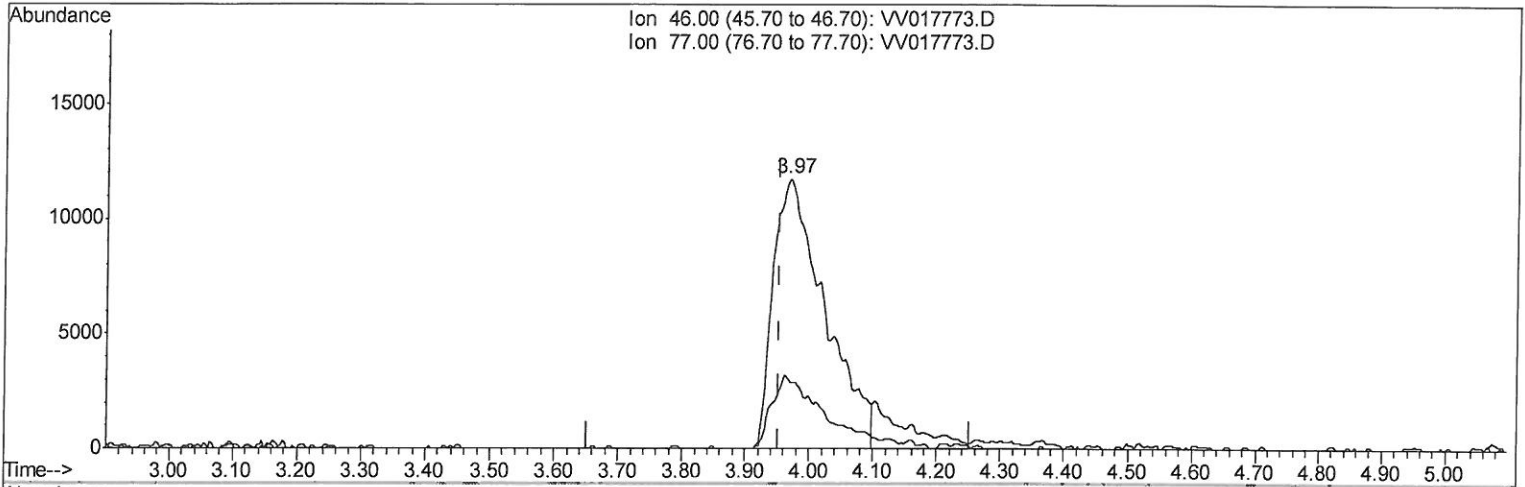

TIC: VV017773.D

(20) 2-Butanone-d5 (S)

3.968min (+0.016) 38.89ug/L m

response 66109

Ion	Exp%	Act%
46.00	100	100
77.00	11.20	15.06#
0.00	0.00	0.00
0.00	0.00	0.00

708/101284

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV073120\
 Data File : VV017773.D
 Acq On : 31 Jul 2020 14:22
 Operator : SY/MD
 Sample : L3520-10
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 D0AC3

Manual Integrations
 APPROVED

MMDadoda
 8/4/2020 9:45:03 AM

Quant Time: Aug 01 06:02:58 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072320WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Aug 01 04:42:38 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	148815	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	139263	5.00	ug/L	0.00
61) 1,4-Dichlorobenzene-d4	11.27	152	71691	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.31	65	29527	4.16	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	83.20%
7) Chloroethane-d5	1.58	69	27013	4.97	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	99.40%
11) 1,1-Dichloroethene-d2	2.12	63	49201	3.09	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	61.80%
20) 2-Butanone-d5	3.97	46	66109m	38.89	ug/L	0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	77.78%
24) Chloroform-d	4.37	84	74235	4.32	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	86.40%
26) 1,2-Dichloroethane-d4	5.06	65	42948	4.84	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.80%
32) Benzene-d6	5.07	84	126646	4.13	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	82.60%
36) 1,2-Dichloropropane-d6	6.10	67	34494	4.04	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	80.80%
41) Toluene-d8	7.34	98	112956	3.84	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	76.80%
45) trans-1,3-Dichloropropene-	7.65	79	15396	3.98	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	79.60%
48) 2-Hexanone-d5	8.12	63	46933	39.16	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	78.32%
59) 1,1,2,2-Tetrachloroethane-	10.24	84	24702	4.16	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	83.20%
65) 1,2-Dichlorobenzene-d4	11.65	152	50711	4.68	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	93.60%

Target Compounds

13) Acetone	2.24	43	18106m	13.606	ug/L	Ovalue
-------------	------	----	--------	--------	------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV073120\
Data File : VV017773.D
Acq On : 31 Jul 2020 14:22
Operator : SY/MD
Sample : L3520-10
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
D0AC3

Manual Integrations
APPROVED

MMDadoda
8/4/2020 9:45:03 AM

Quant Time: Aug 01 06:02:58 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR072320WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Aug 01 04:42:38 2020
Response via : Initial Calibration

